
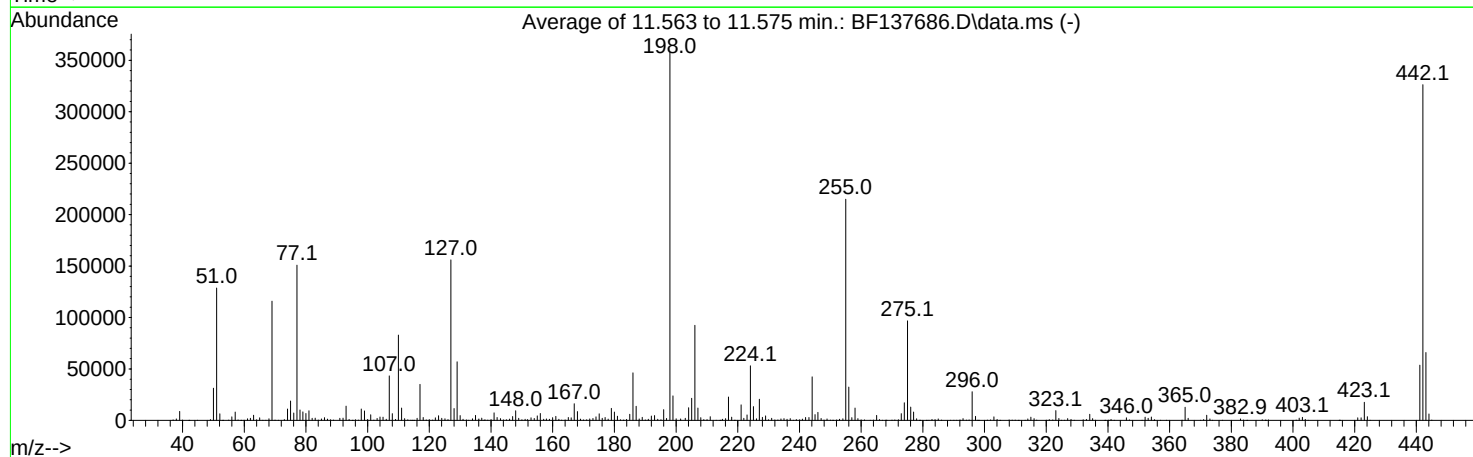


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF032624\  
Data File : BF137686.D  
Acq On : 26 Mar 2024 14:34  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF032624.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Wed Mar 27 01:52:09 2024

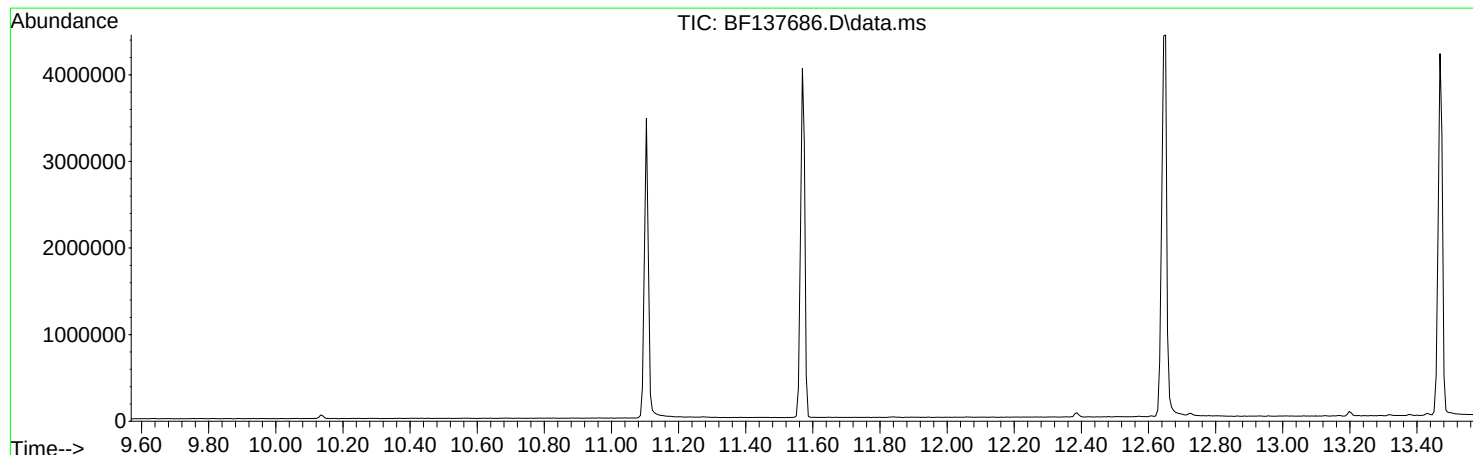




AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1605

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 36.0         | 128643     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.4          | 1602       | PASS                |
| 69             | 198             | 0.00            | 100             | 32.4         | 115904     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.3          | 399        | PASS                |
| 127            | 198             | 10              | 80              | 43.6         | 155979     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.5          | 1817       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 357568     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 23787      | PASS                |
| 275            | 198             | 10              | 60              | 27.1         | 96829      | PASS                |
| 365            | 198             | 1               | 100             | 3.6          | 12839      | PASS                |
| 441            | 198             | 0.01            | 100             | 15.0         | 53725      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 326243     | PASS                |
| 443            | 442             | 15              | 24              | 20.2         | 65976      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF032624\  
Data File : BF137686.D  
Acq On : 26 Mar 2024 14:34  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Mar 27 02:04:40 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF032624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Mar 27 01:52:09 2024  
Response via : Initial Calibration

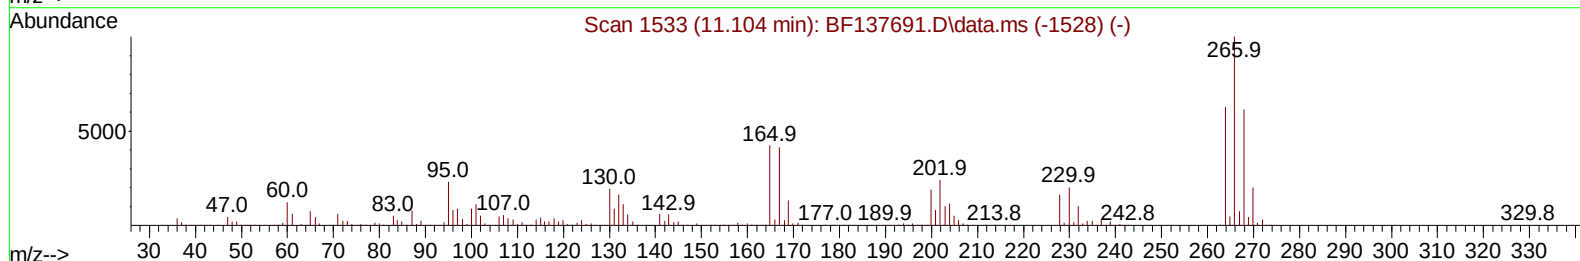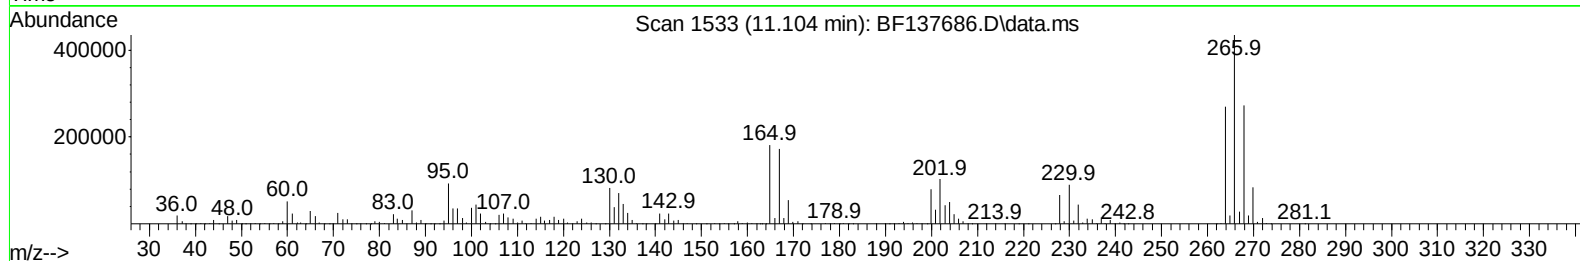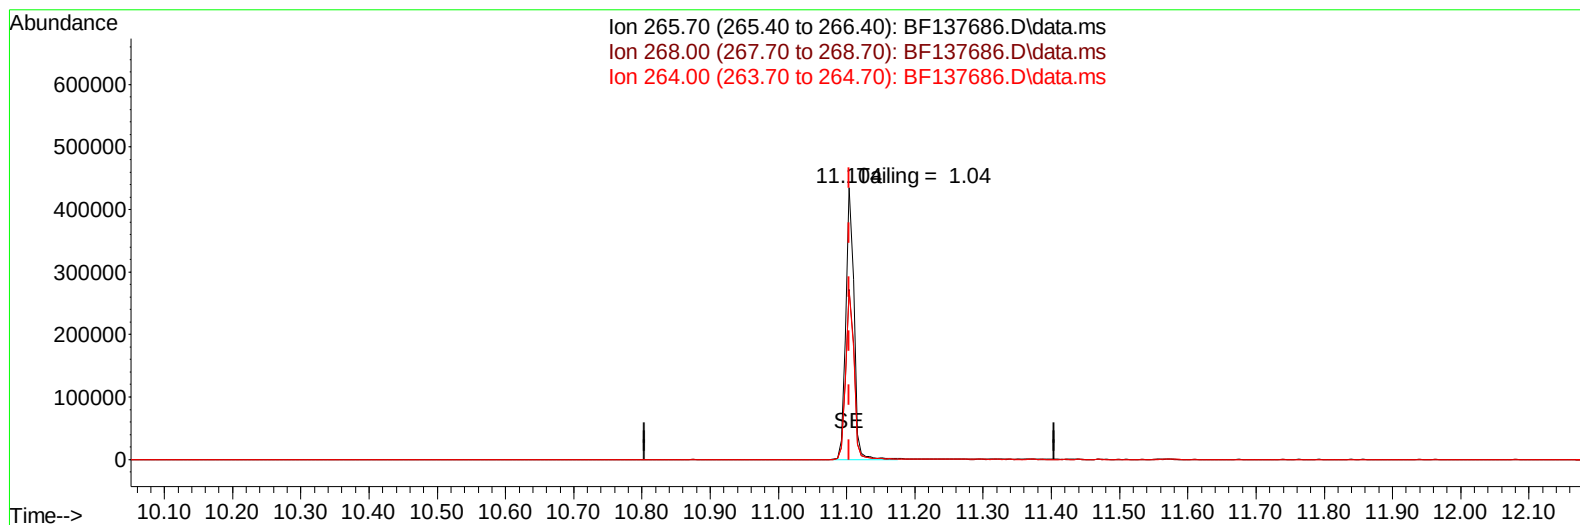

TIC: BF137686.D\data.ms

**(70) Pentachlorophenol (C)**

**11.104min (-0.000) 345367.38 ng**




**response 360499**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.30  | 62.61  |
| 264.00 | 62.70  | 62.12  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF032624\  
Data File : BF137686.D  
Acq On : 26 Mar 2024 14:34  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Mar 27 02:04:40 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF032624.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Mar 27 01:52:09 2024  
Response via : Initial Calibration

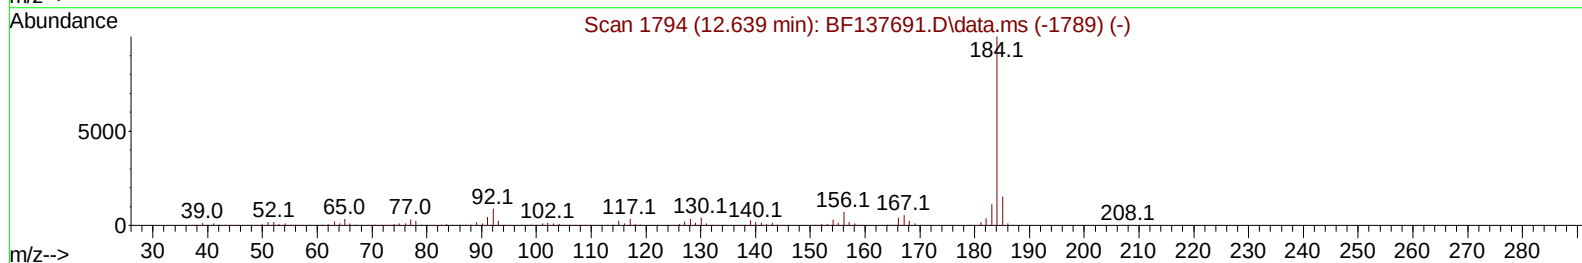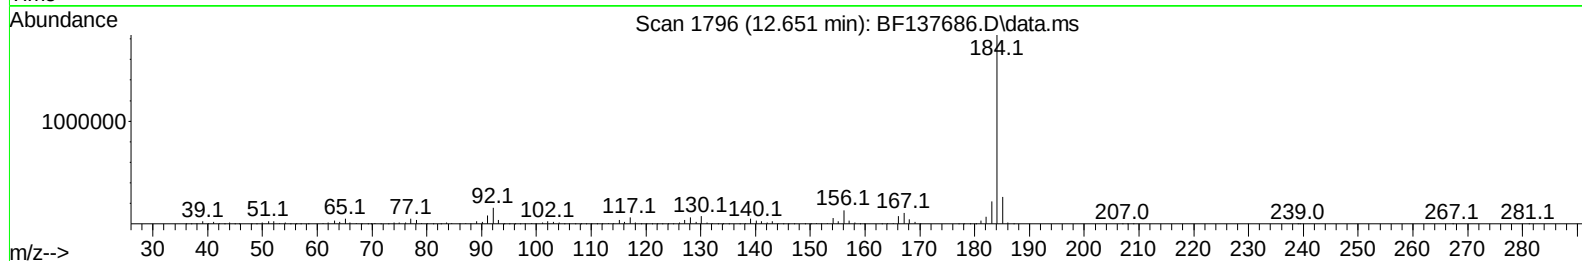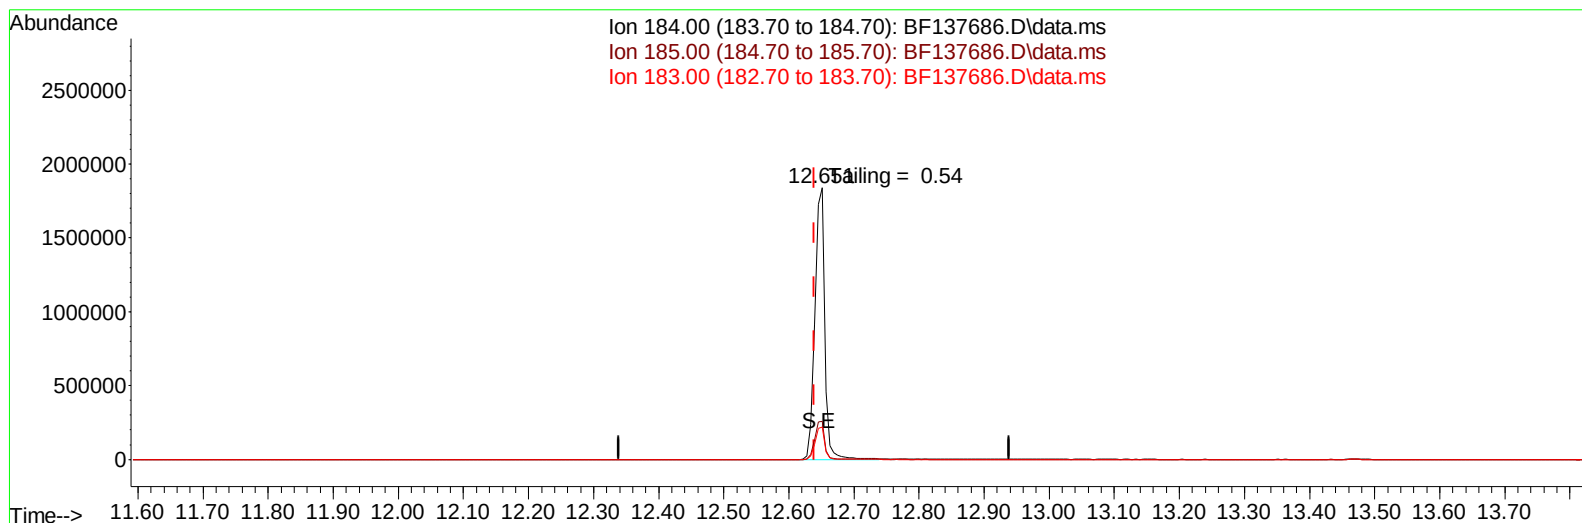

TIC: BF137686.D\data.ms

**(77) Benzidine**

**12.651min (+ 0.012) 9594.38 ng m**

**response 1943475**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.30  | 14.11  |
| 183.00 | 11.30  | 11.95  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 3/26/2024     | BNA_F            | <u>BF137686.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 614690           | 13.468             |
| DDD           | 5395             | 13.198             |
| DDE           | 57               | 12.833             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 5452          | 620142           | 0.88               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP