

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF032719\
 Data File : BF113362.D
 Acq On : 28 Mar 2019 7:21
 Operator : JU/SJ
 Sample : K2097-11
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CS-17

Quant Time: Mar 28 09:10:29 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF032519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 26 03:32:08 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.70	152	181873	20.00	ng	0.00
21) Naphthalene-d8	7.98	136	651118	20.00	ng	0.00
39) Acenaphthene-d10	9.73	164	291823	20.00	ng	0.00
64) Phenanthrene-d10	11.21	188	509788	20.00	ng	0.00
76) Chrysene-d12	13.83	240	428957	20.00	ng	-0.01
87) Perylene-d12	15.24	264	318800	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.33	112	1229086	110.50	ng	0.02
7) Phenol-d6	6.36	99	1440061	102.34	ng	0.00
23) Nitrobenzene-d5	7.27	82	1052720	95.96	ng	0.00
42) 2,4,6-Tribromophenol	10.52	330	366947	101.80	ng	0.00
45) 2-Fluorobiphenyl	9.06	172	1907951	107.05	ng	0.00
79) Terphenyl-d14	12.79	244	1674974	86.07	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF032719\
Data File : BF113362.D
Acq On : 28 Mar 2019 7:21
Operator : JU/SJ
Sample : K2097-11
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CS-17

Quant Time: Mar 28 09:10:29 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF032519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 26 03:32:08 2019
Response via : Initial Calibration

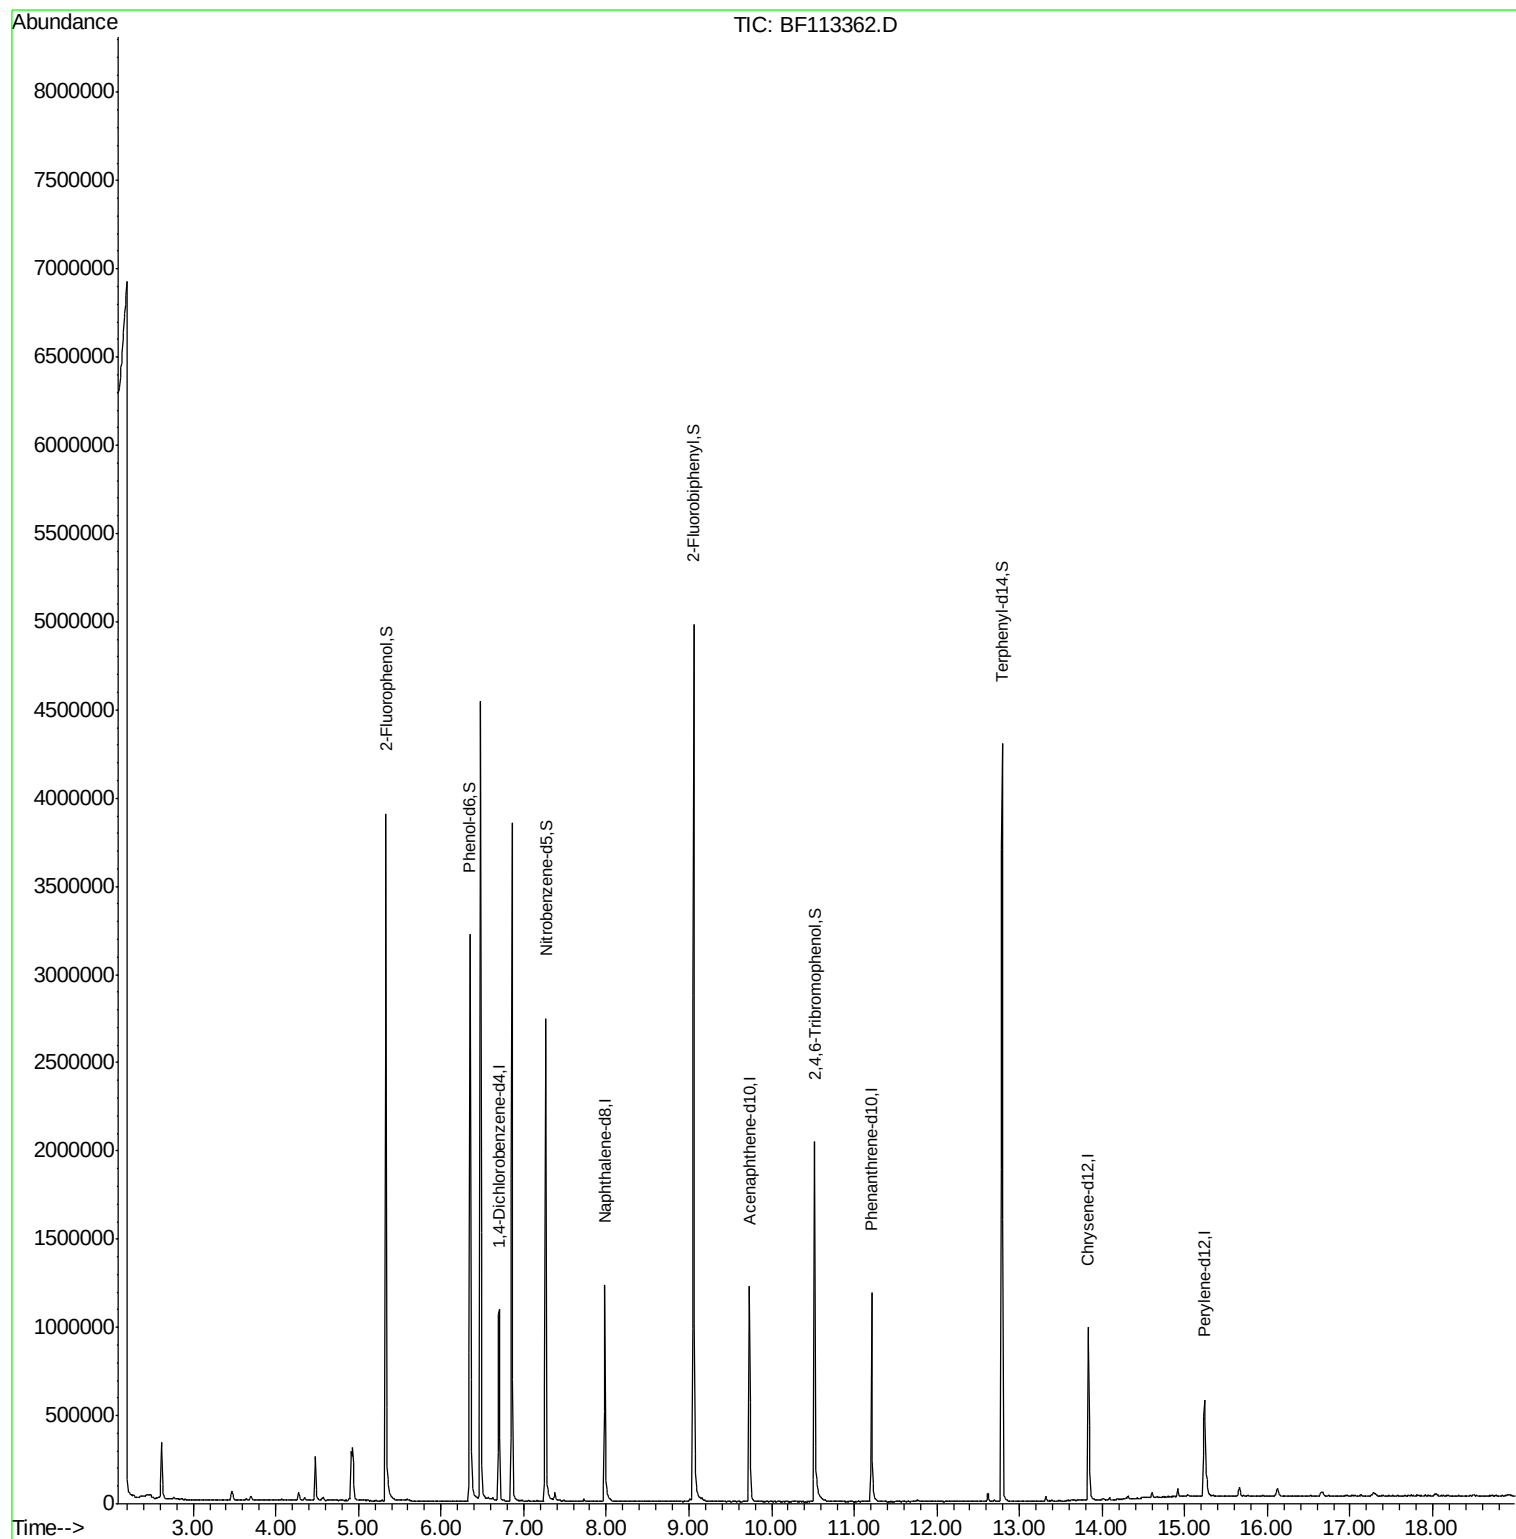

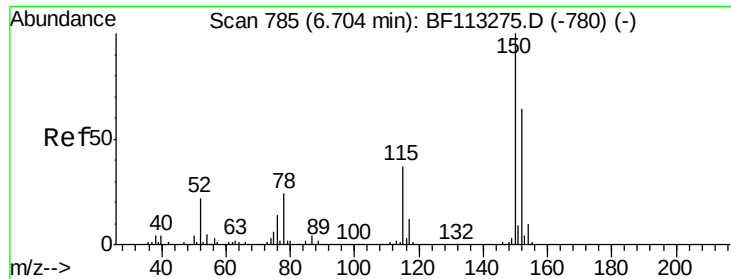


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.70 min Scan# 785
Delta R.T. 0.00 min
Lab File: BF113362.D
Acq: 28 Mar 2019 7:21

Instrument :
BNA_F
ClientSampleId :
CS-17

Tot Ion	Ratio	Lower	Upper
152	100		
150	154.4	124.7	187.1
115	53.8	46.0	69.0



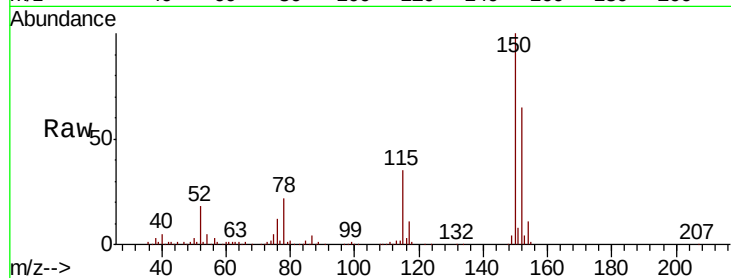


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

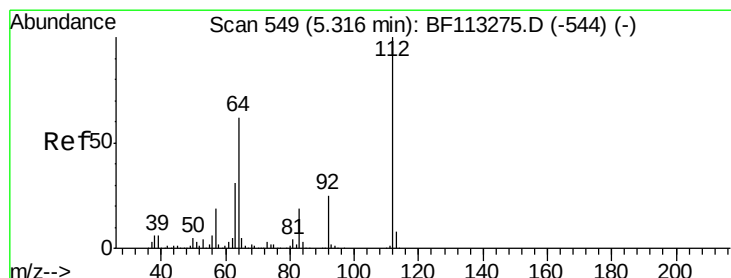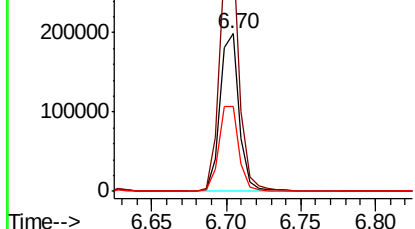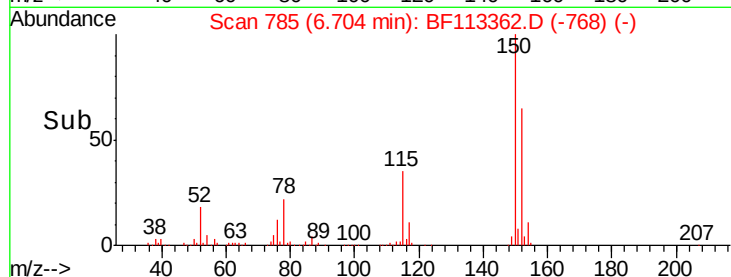

#5

2-Fluorophenol
Concen: 110.500 ng
RT: 5.33 min Scan# 552
Delta R.T. 0.02 min
Lab File: BF113362.D
Acq: 28 Mar 2019 7:21

Tgt Ion	Ratio	Lower	Upper
112	100		
64	60.2	49.2	73.8
63	31.0	24.9	37.3


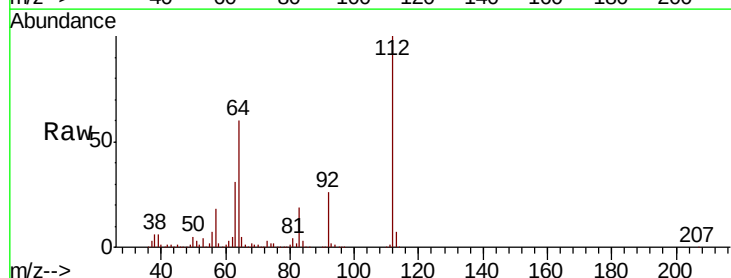



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

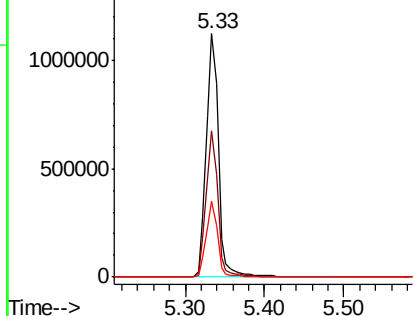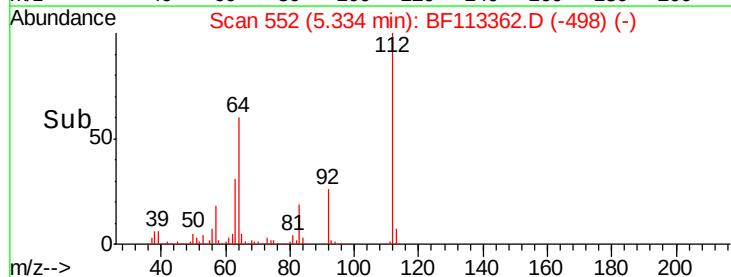

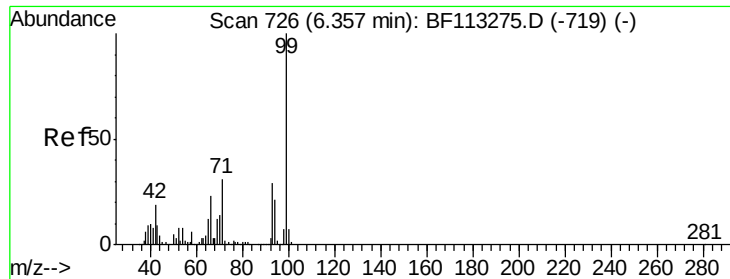

#7

Phenol-d6

Concen: 102.342 ng

RT: 6.36 min Scan# 726

Delta R.T. 0.00 min

Lab File: BF113362.D

Acq: 28 Mar 2019 7:21

Instrument :

BNA_F

ClientSampleId :

CS-17


Tot Ion: 99 Resp: 1440061

Ion Ratio Lower Upper




99 100

42 16.8 14.8 22.2

71 30.2 24.9 37.3

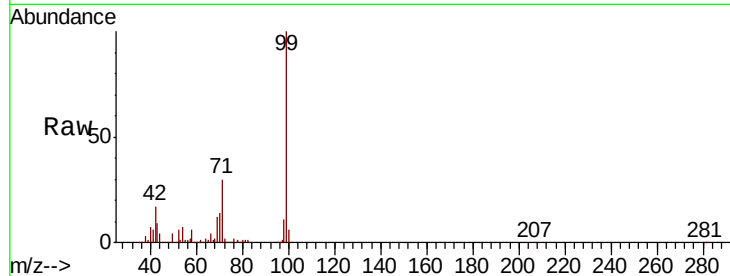

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

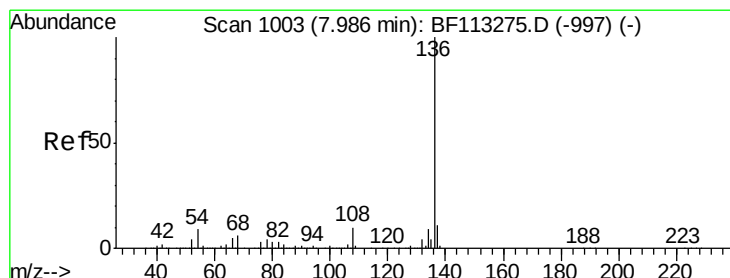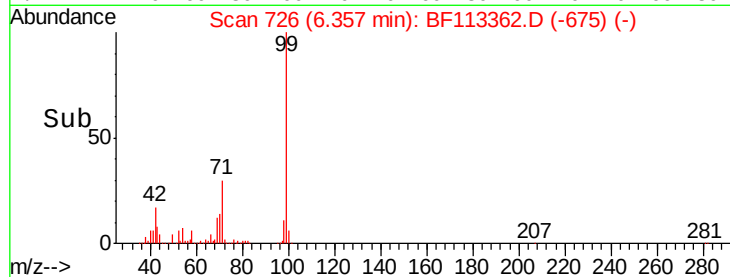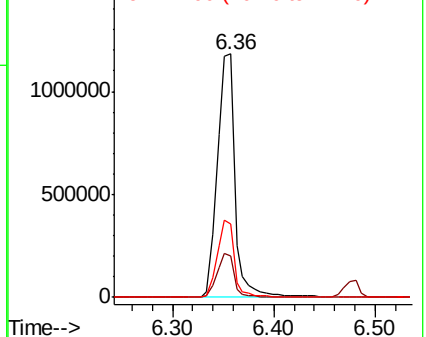

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.98 min Scan# 1002

Delta R.T. -0.01 min

Lab File: BF113362.D

Acq: 28 Mar 2019 7:21

Tgt Ion: 136 Resp: 651118


Ion Ratio Lower Upper

136 100



137 11.3 8.9 13.3


54 8.4 7.0 10.6

68 6.6 4.8 7.2

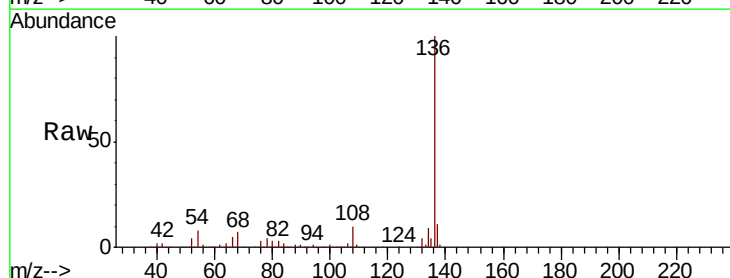

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1



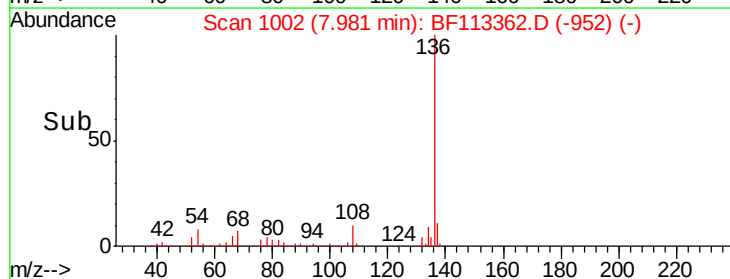
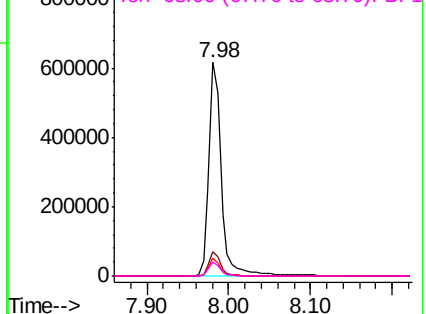


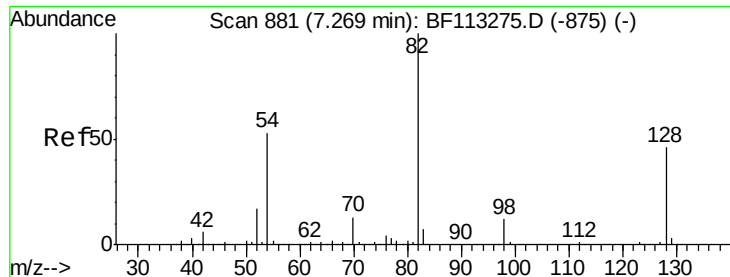

#23
Nitrobenzene-d5
Concen: 95.963 ng
RT: 7.27 min Scan# 881
Delta R.T. 0.00 min
Lab File: BF113362.D
Acq: 28 Mar 2019 7:21




Instrument :
BNA_F
ClientSampleId :
CS-17


Tot Ion: 82 Resp: 1052720
Ion Ratio Lower Upper
82 100
128 49.4 36.5 54.7
54 50.5 42.2 63.2

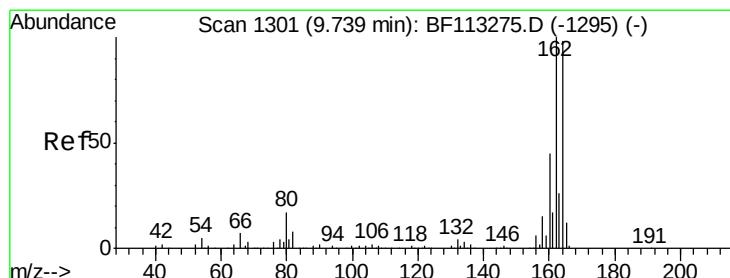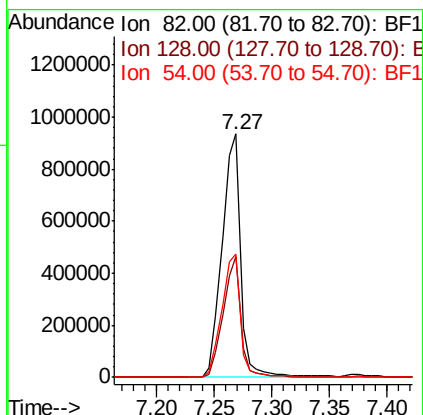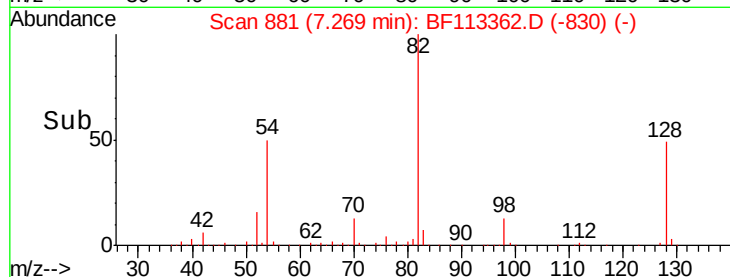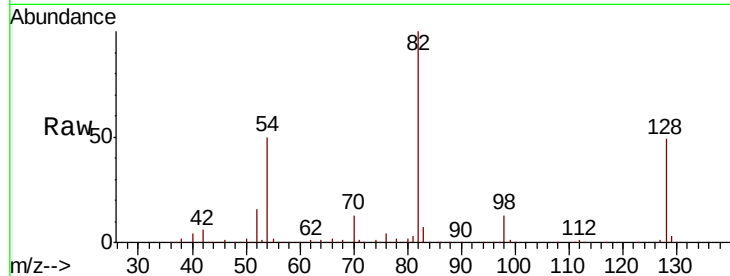

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.73 min Scan# 1300
Delta R.T. -0.01 min
Lab File: BF113362.D
Acq: 28 Mar 2019 7:21

Tgt Ion:164 Resp: 291823
Ion Ratio Lower Upper
164 100
162 102.0 81.8 122.6
160 45.2 36.4 54.6

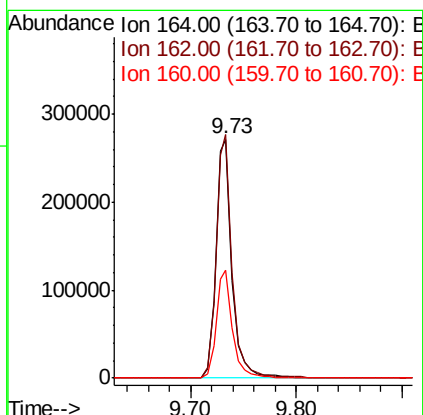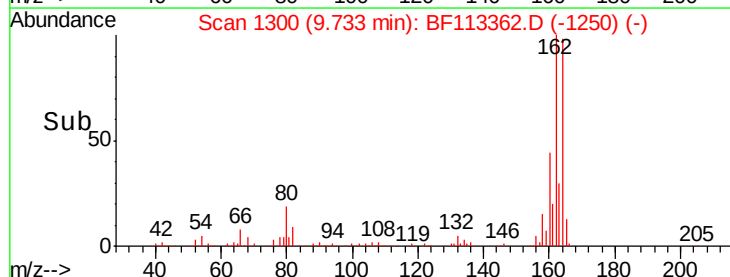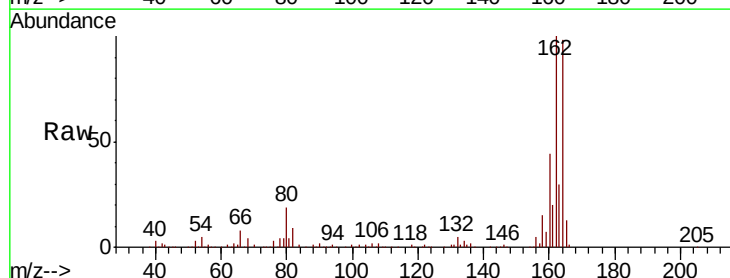

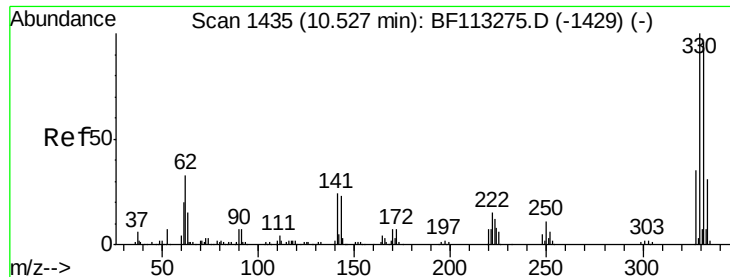

#42

2,4,6-Tribromophenol

Concen: 101.797 ng

RT: 10.52 min Scan# 1434

Delta R.T. -0.01 min

Lab File: BF113362.D

Acq: 28 Mar 2019 7:21

Instrument :

BNA_F

ClientSampleId :

CS-17


Tot Ion:330 Resp: 366947

Ion Ratio Lower Upper




330 100

332 97.4 77.8 116.6

141 27.1 22.7 34.1

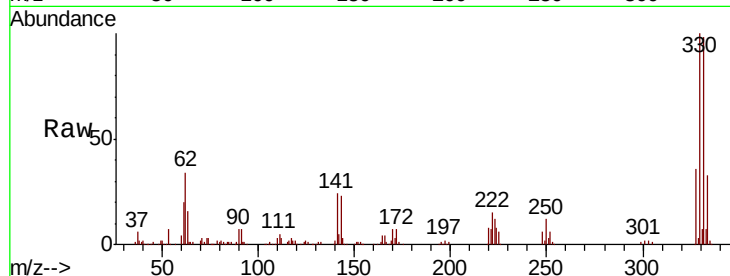

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

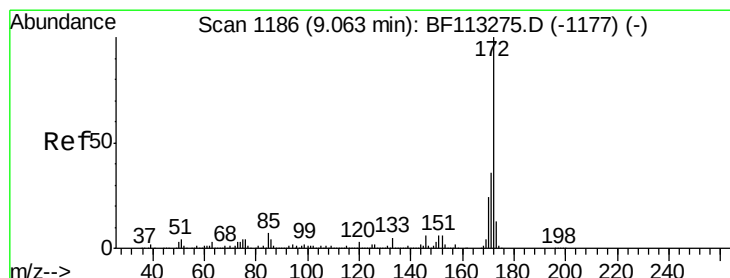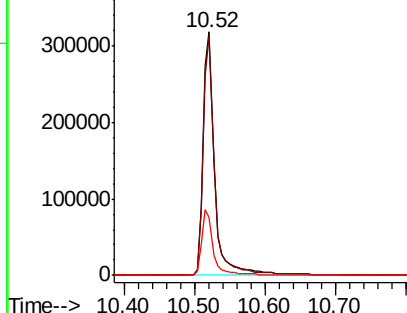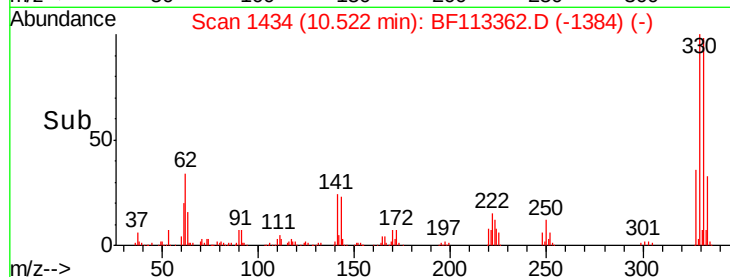

#45

2-Fluorobiphenyl

Concen: 107.050 ng

RT: 9.06 min Scan# 1185

Delta R.T. -0.00 min

Lab File: BF113362.D

Acq: 28 Mar 2019 7:21


Tgt Ion:172 Resp: 1907951

Ion Ratio Lower Upper



172 100


171 36.7 29.0 43.6

170 24.7 19.5 29.3

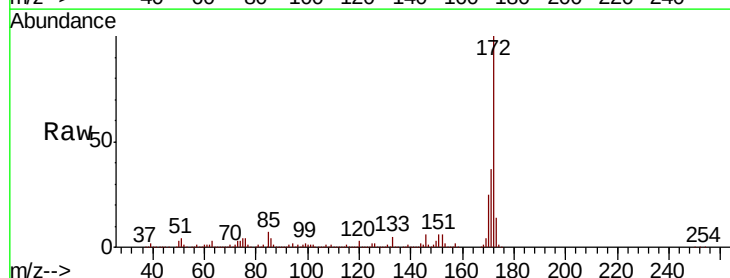

Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E



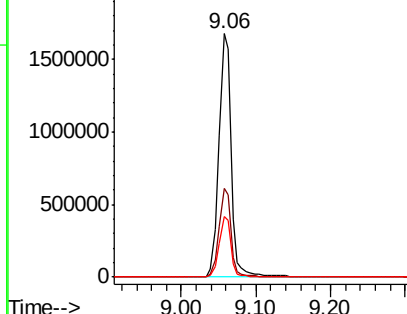
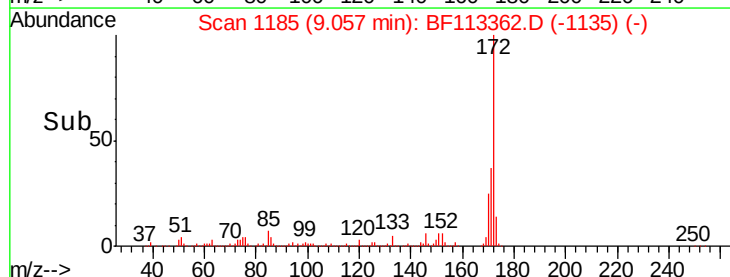


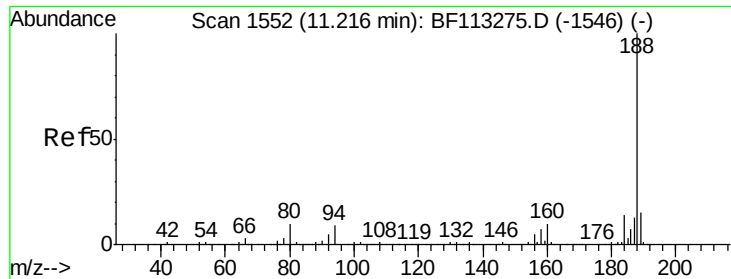

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.21 min Scan# 1551
Delta R.T. -0.01 min
Lab File: BF113362.D
Acq: 28 Mar 2019 7:21




Instrument :
BNA_F
ClientSampleId :
CS-17


Tot Ion:188 Resp: 509788
Ion Ratio Lower Upper
188 100
94 9.1 7.0 10.6
80 9.9 7.7 11.5

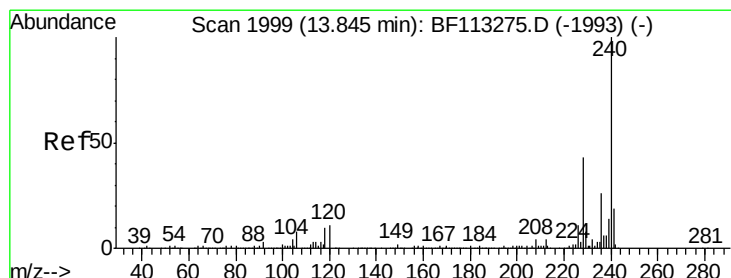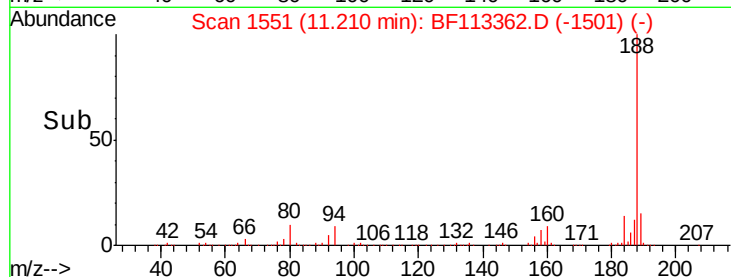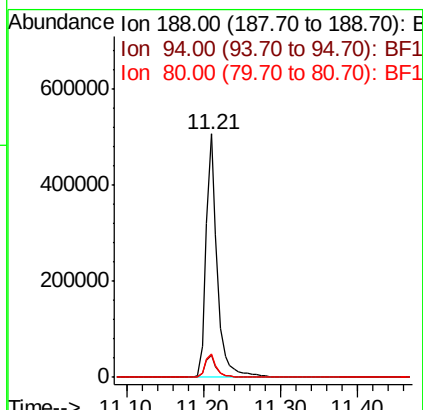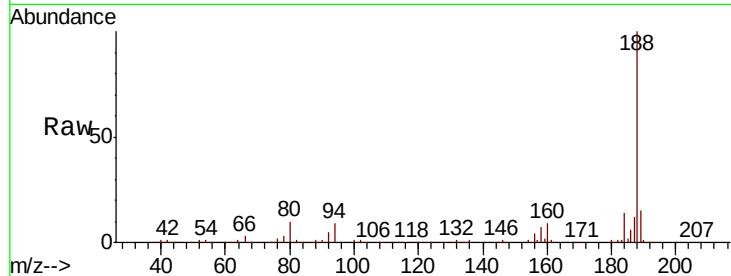

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.83 min Scan# 1997
Delta R.T. -0.01 min
Lab File: BF113362.D
Acq: 28 Mar 2019 7:21

Tgt Ion:240 Resp: 428957
Ion Ratio Lower Upper
240 100
120 11.7 8.8 13.2
236 25.5 20.9 31.3


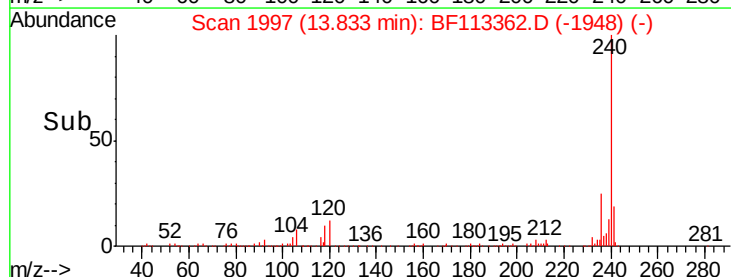
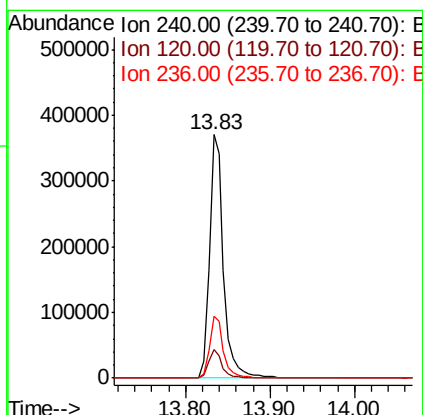
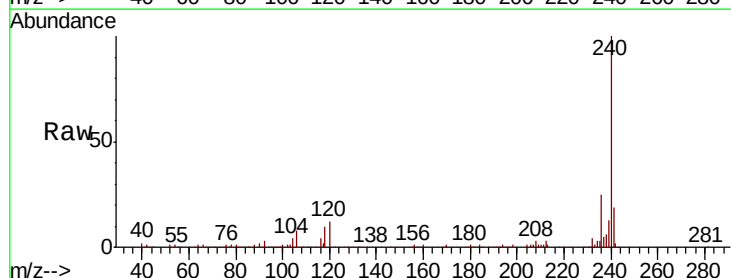


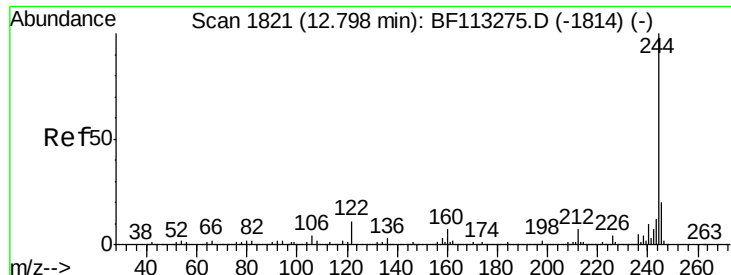

#79
 Terphenyl-d14
 Concen: 86.067 ng
 RT: 12.79 min Scan# 1820
 Delta R.T. -0.00 min
 Lab File: BF113362.D
 Acq: 28 Mar 2019 7:21

Instrument :
 BNA_F
 ClientSampleId :
 CS-17

Tot Ion:244 Resp: 1674974
 Ion Ratio Lower Upper
 244 100
 212 6.7 5.5 8.3
 122 10.7 8.6 13.0

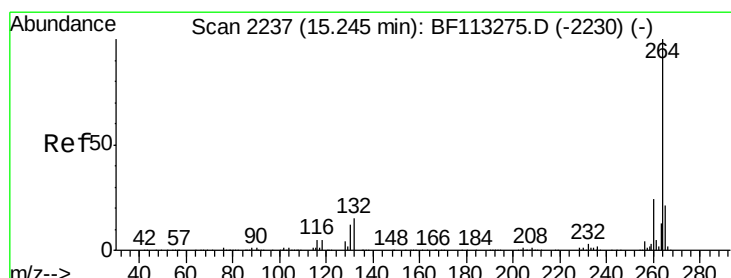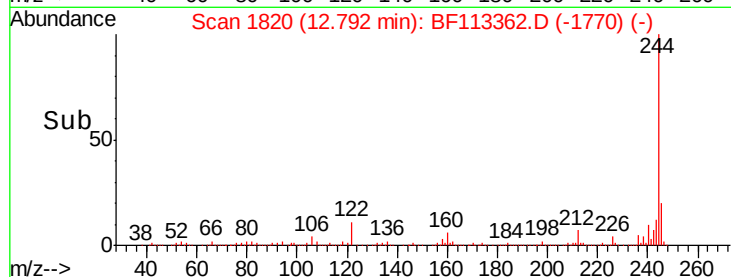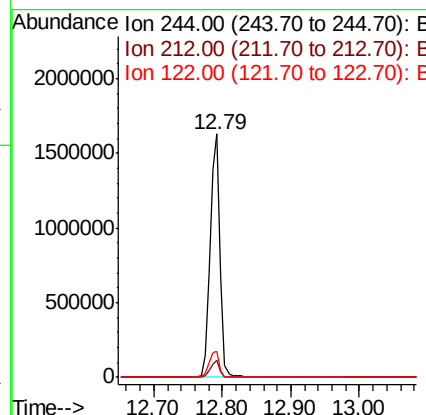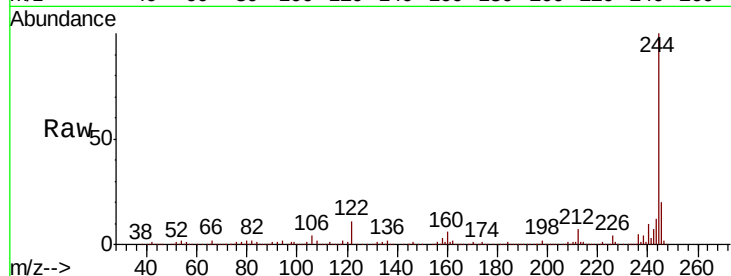

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.24 min Scan# 2236
 Delta R.T. -0.01 min
 Lab File: BF113362.D
 Acq: 28 Mar 2019 7:21

Tgt Ion:264 Resp: 318800
 Ion Ratio Lower Upper
 264 100
 260 23.2 19.1 28.7
 265 21.9 17.1 25.7

