

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032719\
 Data File : BF113365.D
 Acq On : 28 Mar 2019 9:13
 Operator : JU/SJ
 Sample : PB118325BL
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB118325BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.316	546	549	574	rBV	1796005	2152739	67.23%	9.086%
2	6.345	720	724	742	rBV	2493002	2623336	81.93%	11.072%
3	6.475	742	746	765	rVB	2089455	2287793	71.45%	9.656%
4	6.698	781	784	795	rVB	1086827	971160	30.33%	4.099%
5	6.857	807	811	827	rVB	2491274	2177822	68.02%	9.192%
6	7.263	876	880	898	rBV	1546227	1556084	48.60%	6.568%
7	7.980	998	1002	1026	rBV	1147849	1230134	38.42%	5.192%
8	9.057	1181	1185	1214	rVB	3294159	3201890	100.00%	13.514%
9	9.733	1296	1300	1321	rVB	1166746	1293638	40.40%	5.460%
10	10.521	1431	1434	1449	rBV	160705	246020	7.68%	1.038%
11	11.210	1547	1551	1566	rBV	1073325	1193227	37.27%	5.036%
12	12.786	1815	1819	1832	rBV	2853910	2628232	82.08%	11.093%
13	13.833	1993	1997	2011	rBV	918713	1081870	33.79%	4.566%
14	14.915	2178	2181	2187	rVB	28281	32186	1.01%	0.136%
15	15.239	2231	2236	2248	rBV	540913	850390	26.56%	3.589%
16	15.662	2303	2308	2314	rVB	42329	61270	1.91%	0.259%
17	16.121	2381	2386	2393	rVB2	36125	63408	1.98%	0.268%
18	16.656	2472	2477	2483	rVB4	20878	41575	1.30%	0.175%


Sum of corrected areas: 23692774

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF032719\
Data File : BF113365.D
Acq On : 28 Mar 2019 9:13
Operator : JU/SJ
Sample : PB118325BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB118325BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF032519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

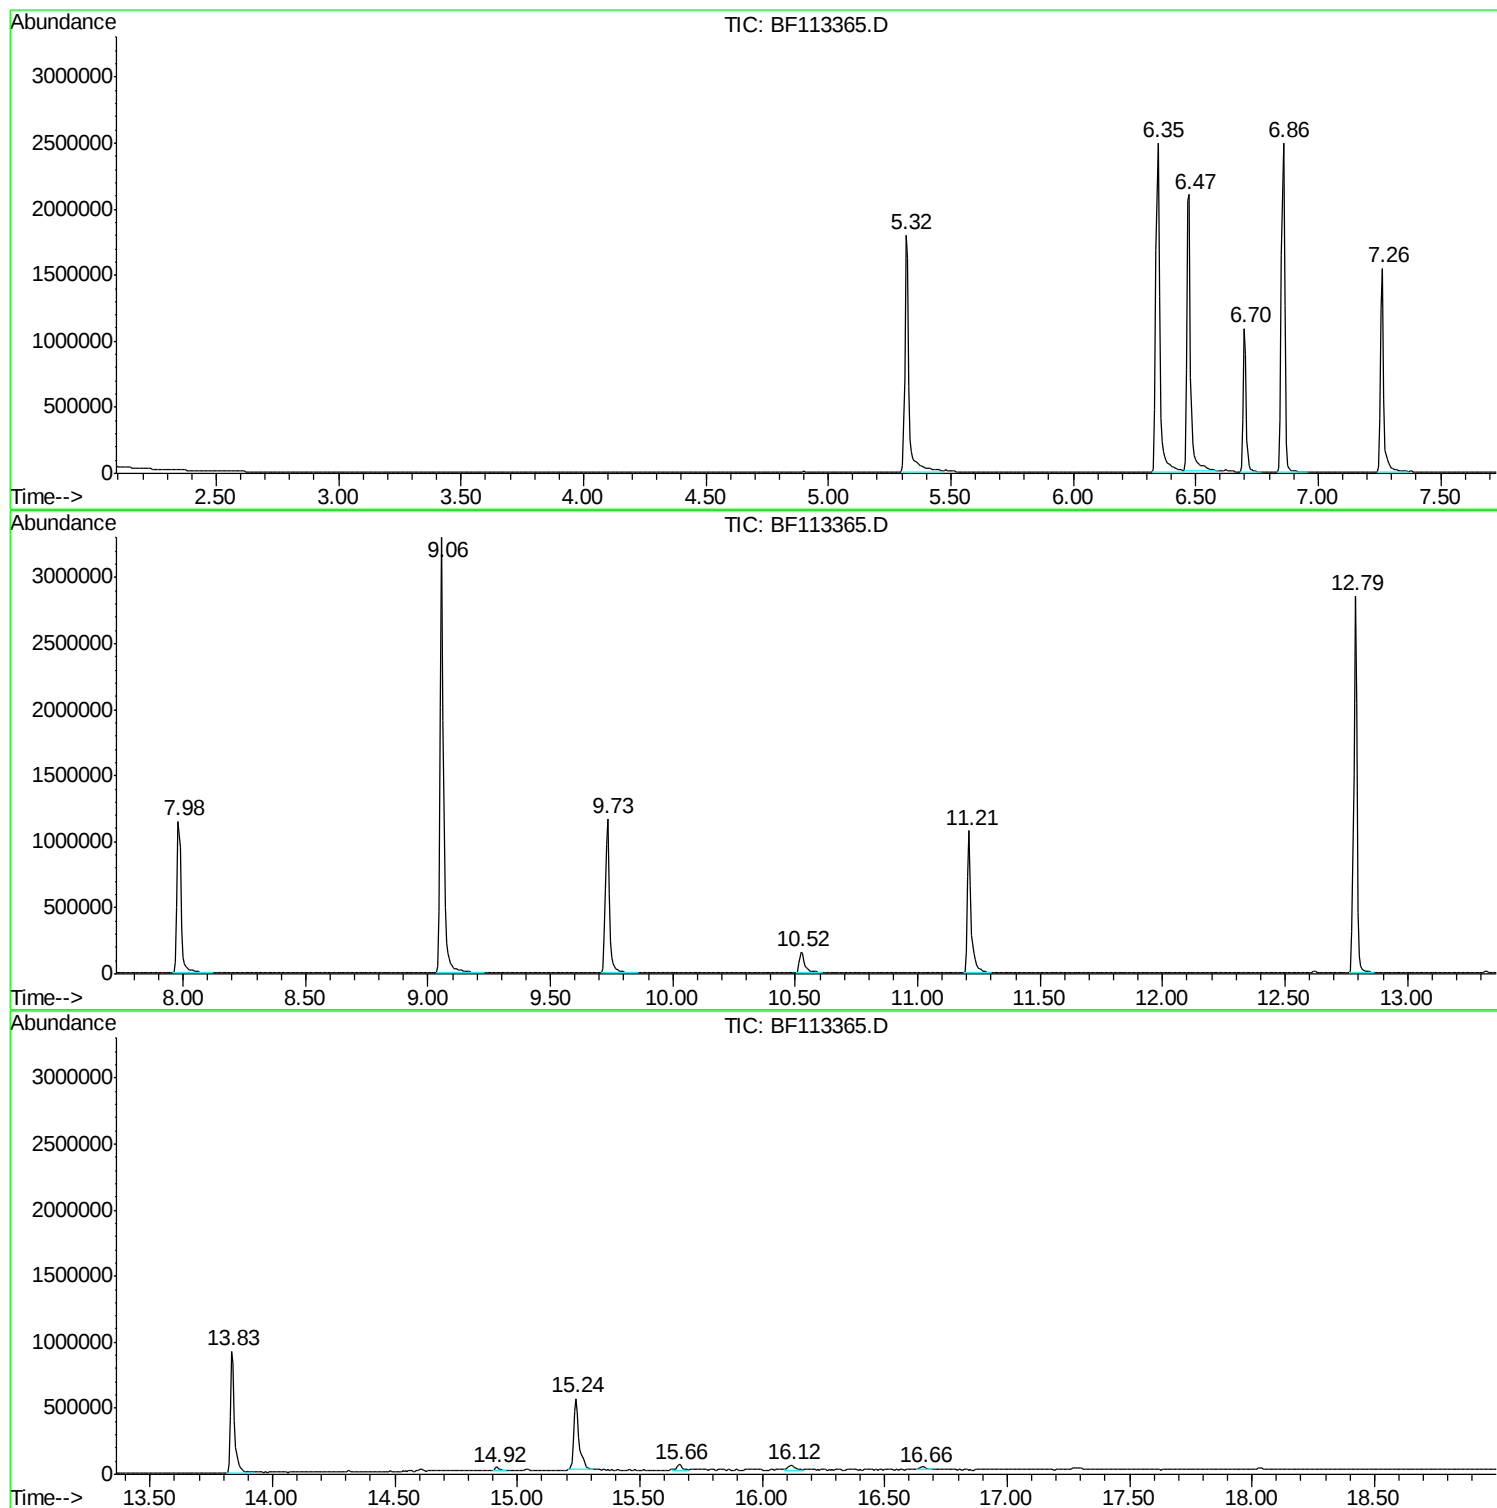

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF032719\
Data File : BF113365.D
Acq On : 28 Mar 2019 9:13
Operator : JU/SJ
Sample : PB118325BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB118325BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF032519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.47 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.47	47.11 ng	2287790	1,4-Dichlorobenzene-d4	6.70

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	43
2			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
3			Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	16
4			5-Aminoindole	132	C8H8N2	005192-03-0	16
5			Xenon	132	Xe	007440-63-3	9

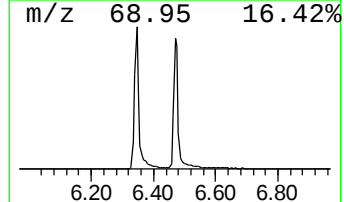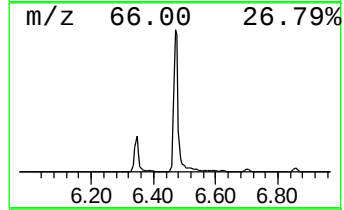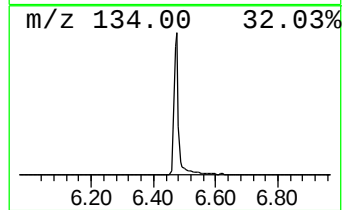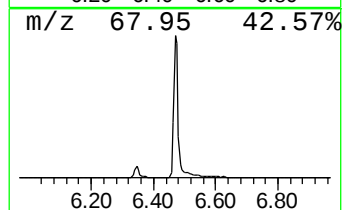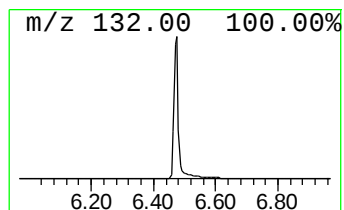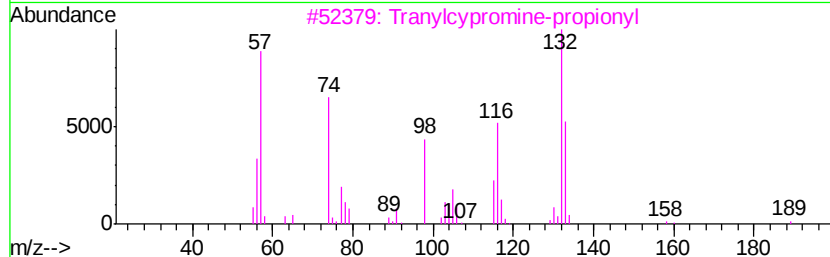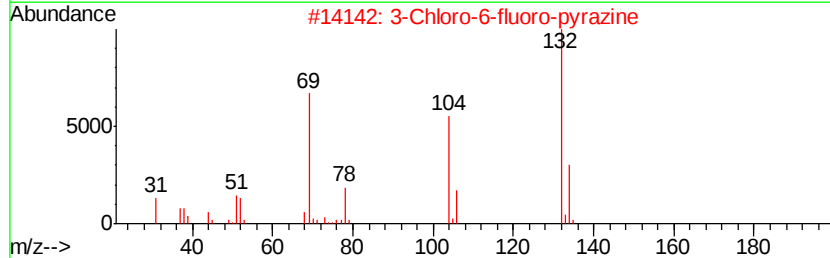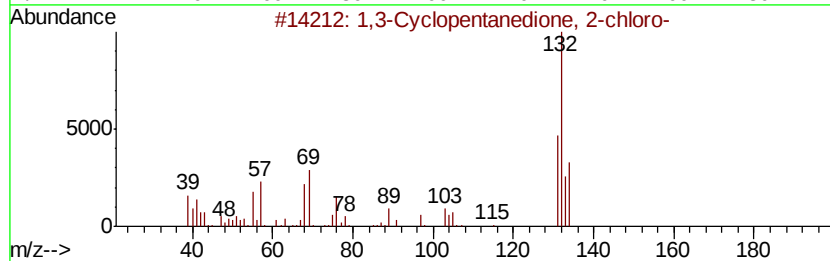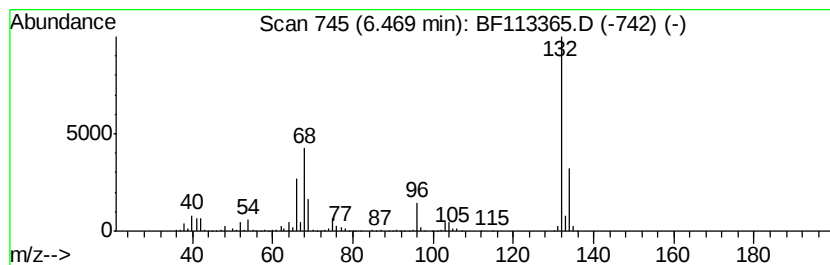

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032719\
Data File : BF113365.D
Acq On : 28 Mar 2019 9:13
Operator : JU/SJ
Sample : PB118325BL
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB118325BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.47	6.47	47.1	ng	2287790	1	6.70	971160	20.0