


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032719\
 Data File : BF113345.D
 Acq On : 27 Mar 2019 23:02
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 26 03:32:08 2019

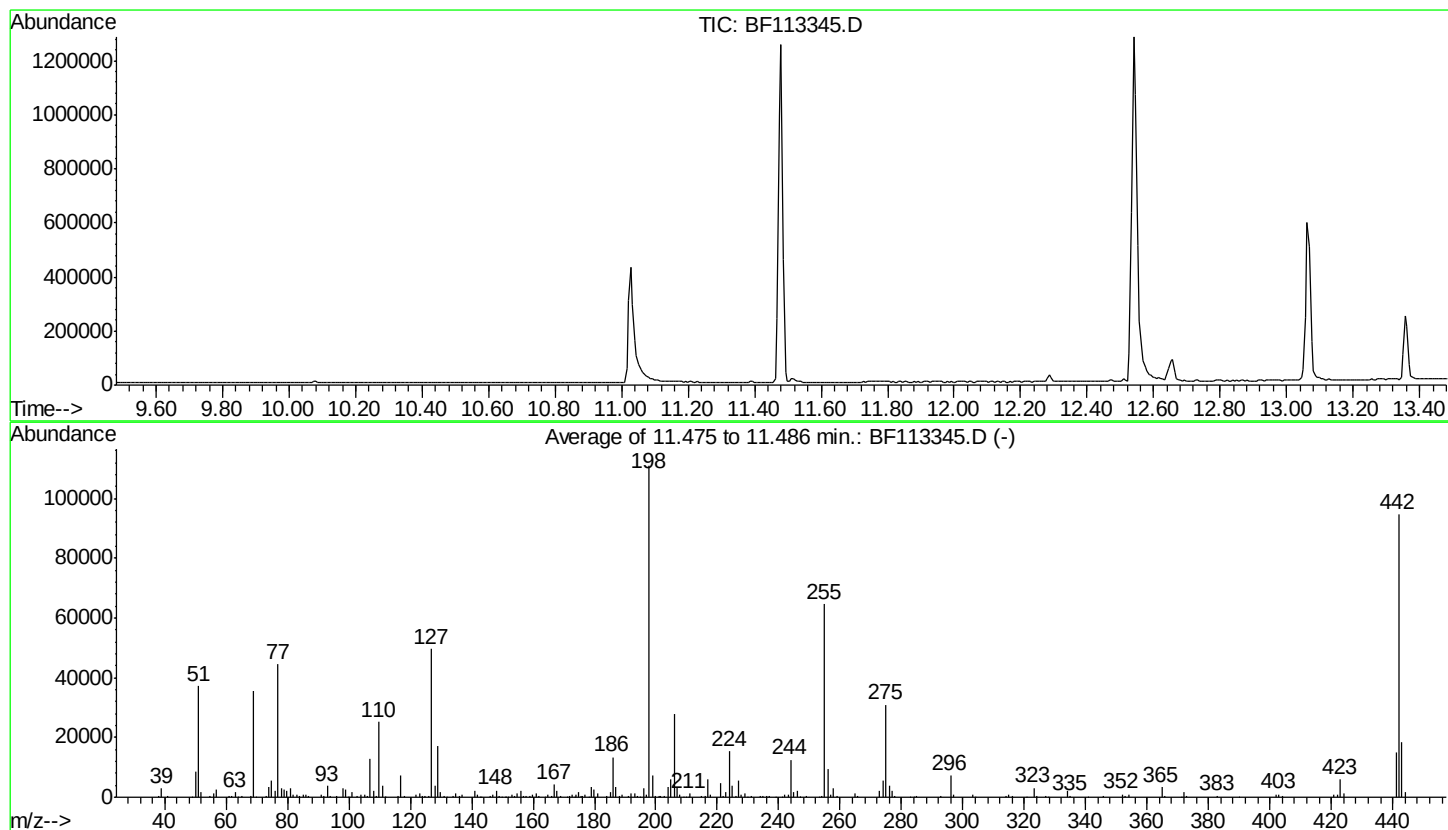

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	37217	PASS
68	69	0.00	2	1.3	467	PASS
69	198	0.00	100	31.9	35413	PASS
70	69	0.00	2	0.3	108	PASS
127	198	10	80	44.6	49546	PASS
197	198	0.00	2	0.7	744	PASS
198	198	100	100	100.0	110968	PASS
199	198	5	9	6.7	7473	PASS
275	198	10	60	27.8	30890	PASS
365	198	1	100	3.1	3413	PASS
441	198	0.01	100	13.6	15127	PASS
442	198	50	100	85.2	94576	PASS
443	442	15	24	19.4	18359	PASS