
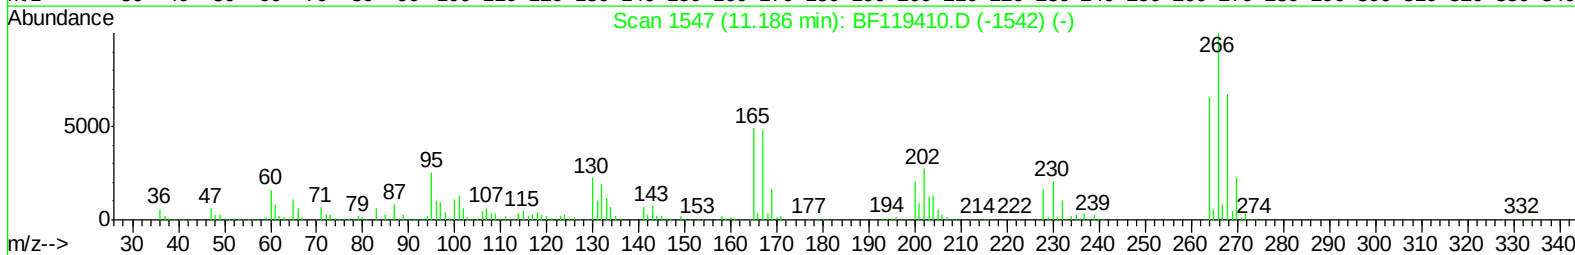
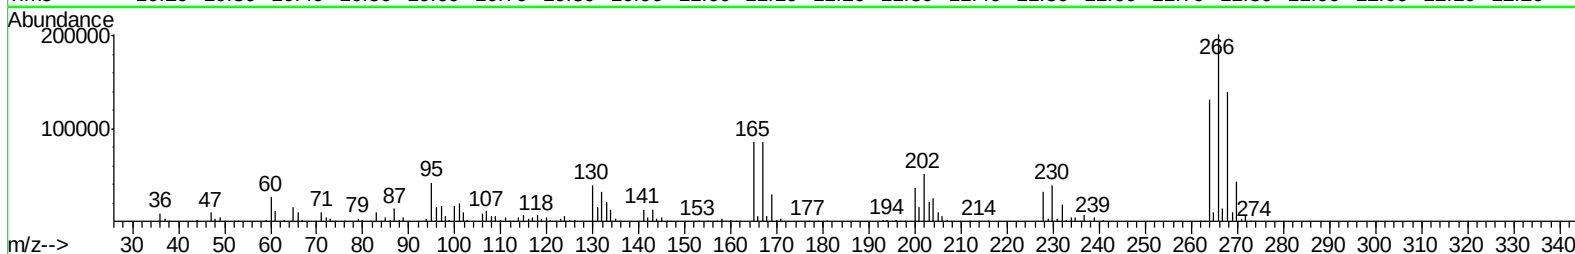


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032720\
Data File : BF119569.D
Acq On : 27 Mar 2020 16:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 07:16:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 27 07:52:09 2020
Response via : Initial Calibration

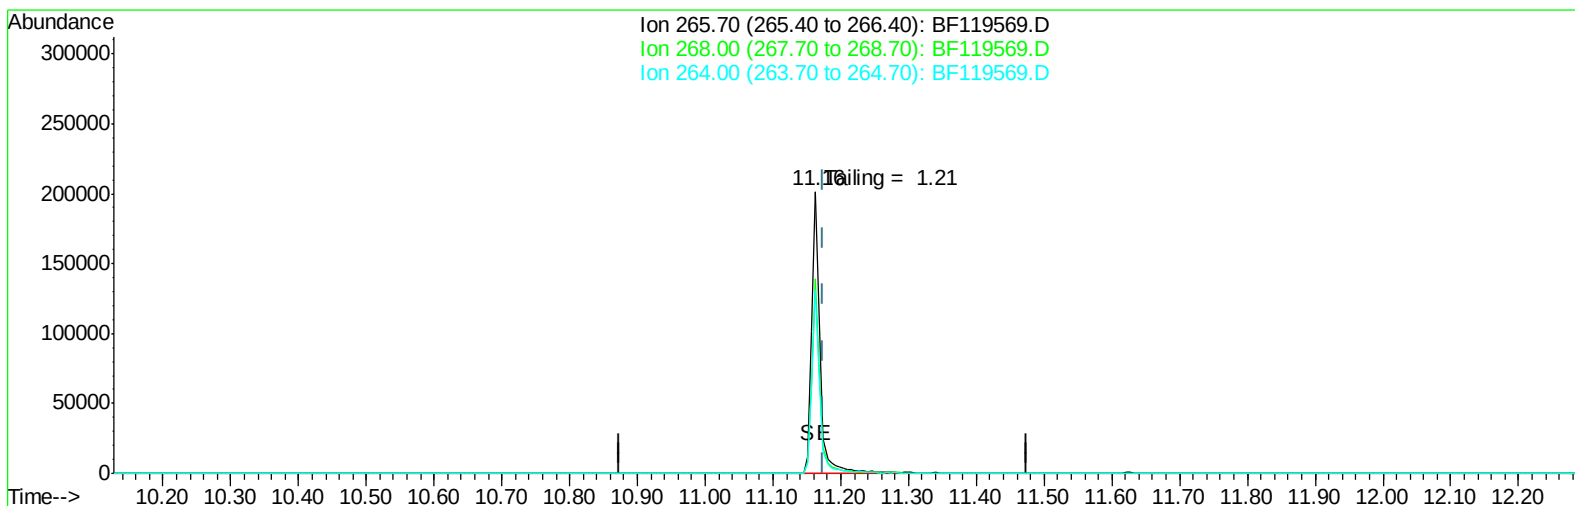

TIC: BF119569.D

(70) Pentachlorophenol (C)




11.163min (-0.012) 30055.10ng

response 177273

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	69.08
264.00	61.20	64.85
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032720\
 Data File : BF119569.D
 Acq On : 27 Mar 2020 16:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 07:16:20 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 27 07:52:09 2020
 Response via : Initial Calibration

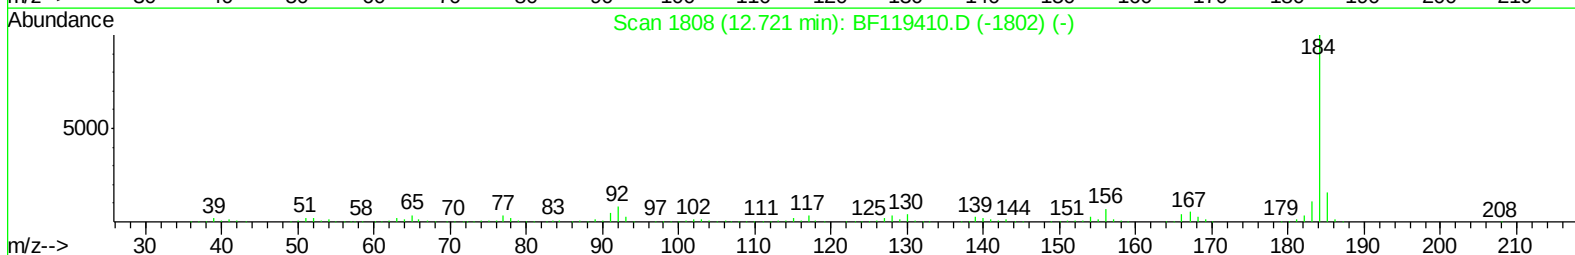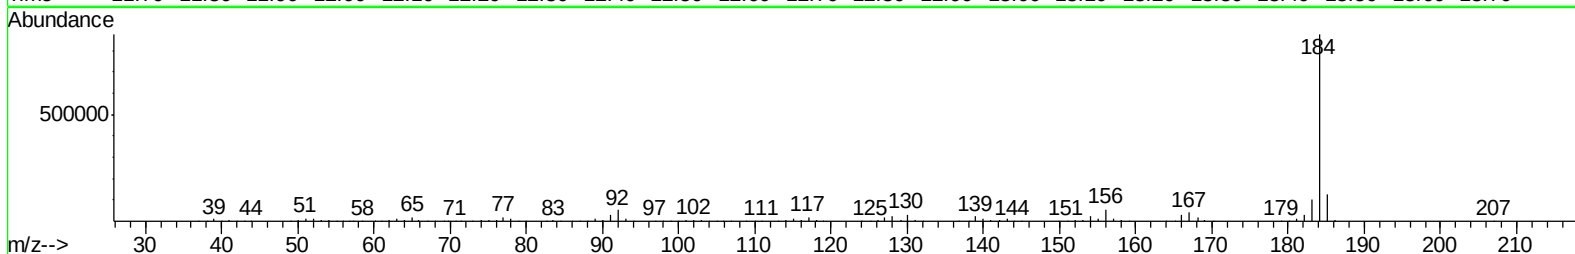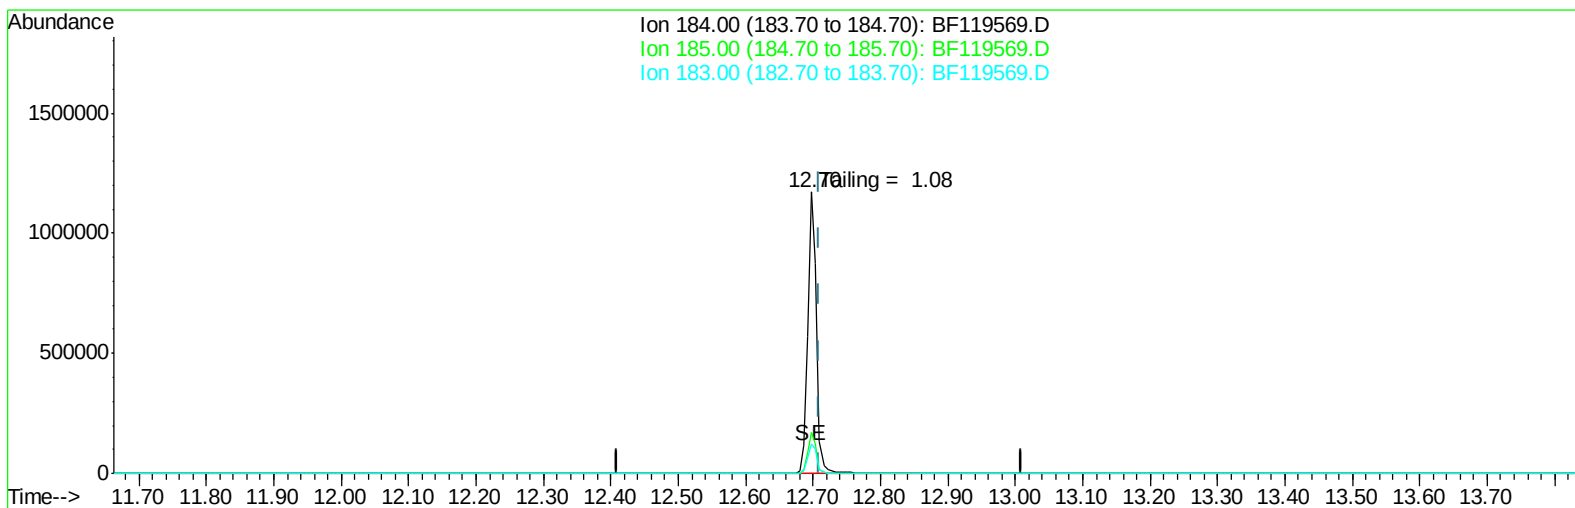

TIC: BF119569.D

(77) Benzidine

12.698min (-0.012) 0.00ng

response 1052823

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	14.73
183.00	11.30	10.68
0.00	0.00	0.00