
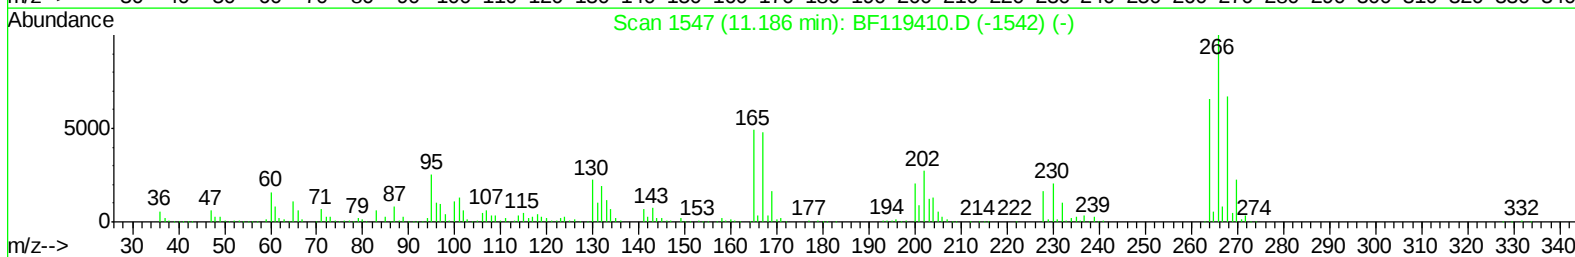
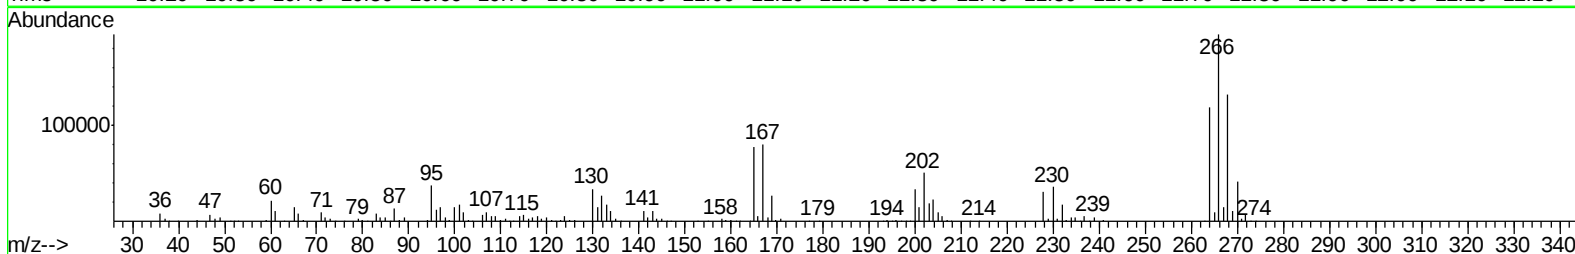


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032720\
Data File : BF119609.D
Acq On : 28 Mar 2020 11:22
Operator : CG/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 23:57:33 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 27 07:52:09 2020
Response via : Initial Calibration

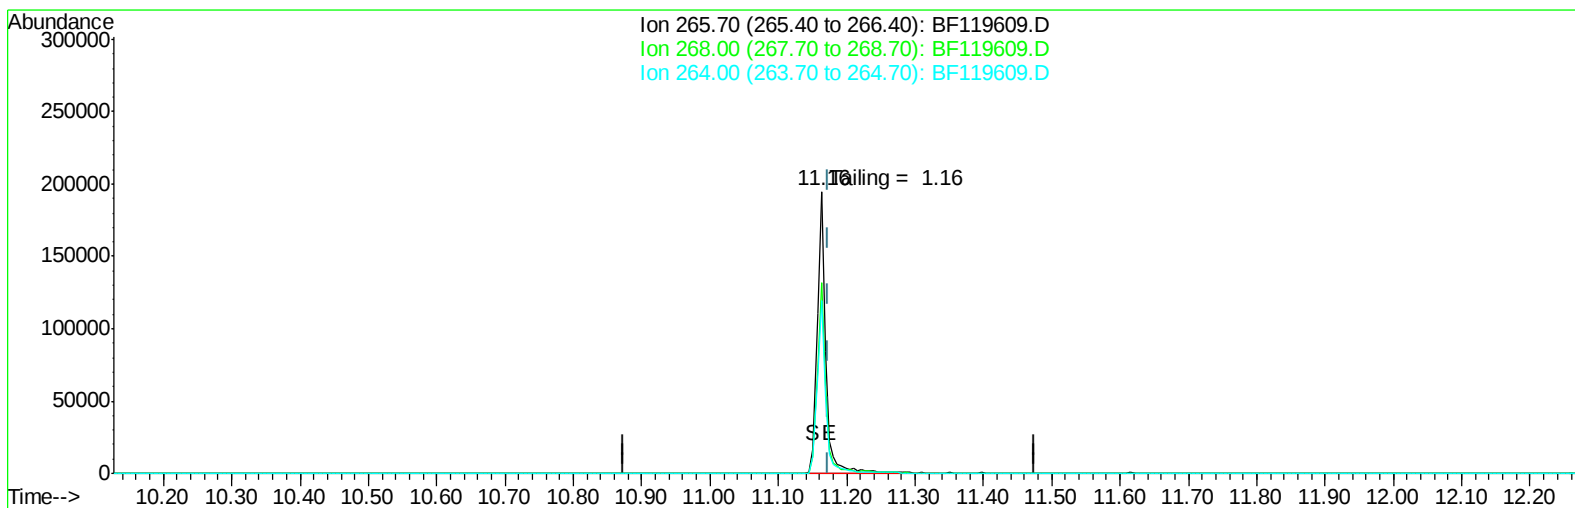

TIC: BF119609.D

(70) Pentachlorophenol (C)




11.163min (-0.012) 90750.42ng

response 168086

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	67.54
264.00	61.20	61.18
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032720\
 Data File : BF119609.D
 Acq On : 28 Mar 2020 11:22
 Operator : CG/JU
 Sample : DFTTP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 23:57:33 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 27 07:52:09 2020
 Response via : Initial Calibration

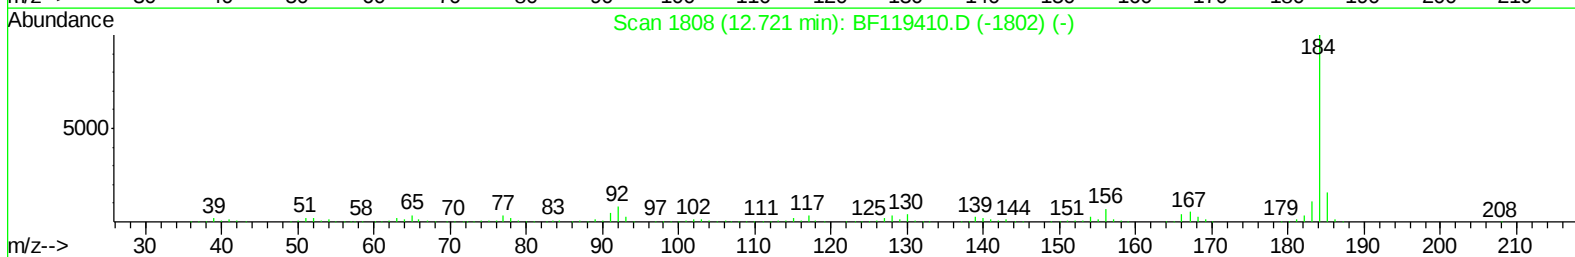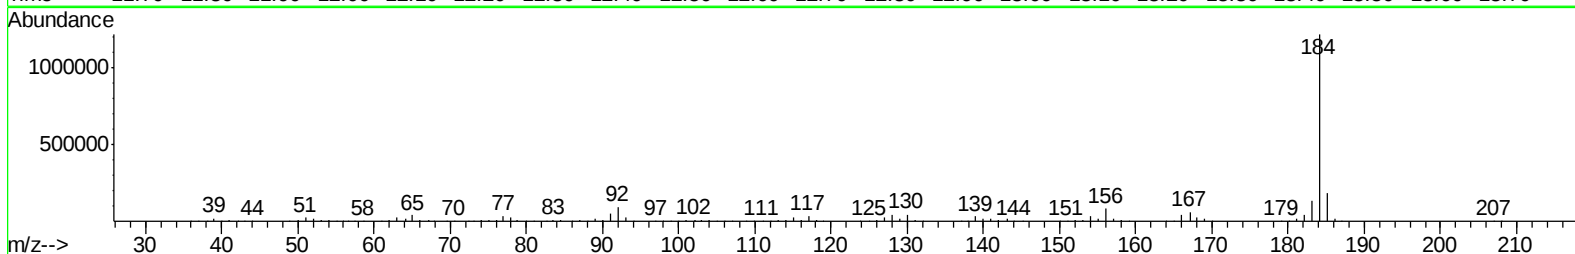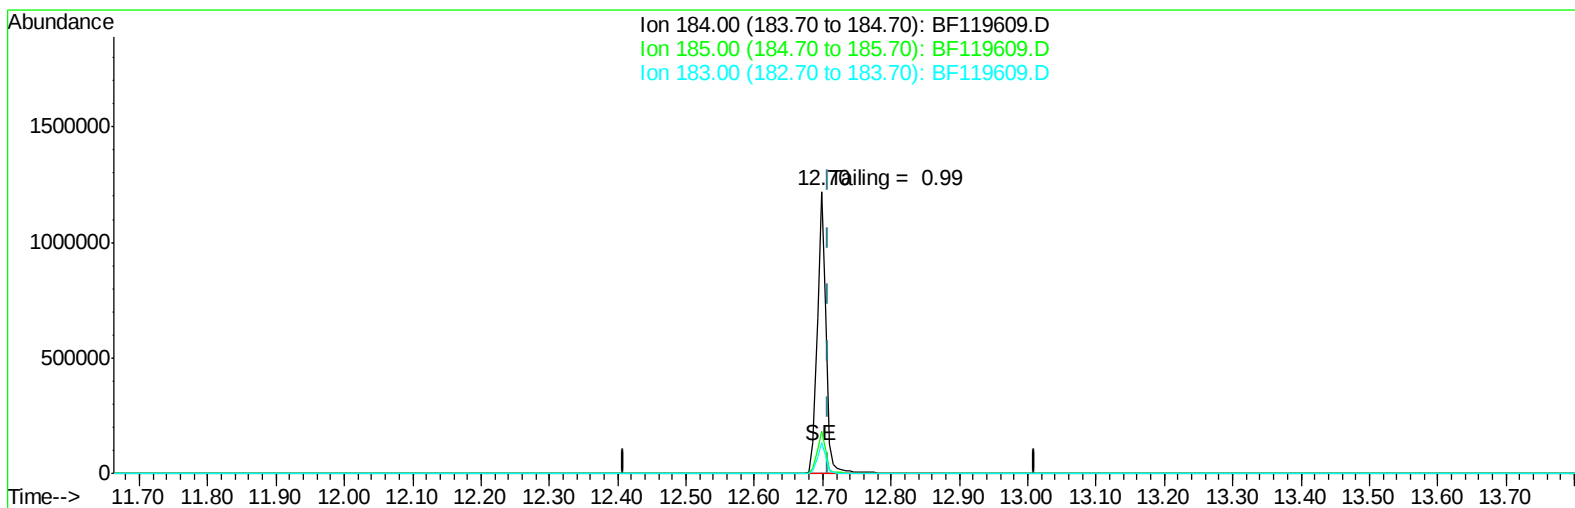

TIC: BF119609.D

(77) Benzidine

12.698min (-0.012) 217045.69ng

response 1065509

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	15.12
183.00	11.30	10.87
0.00	0.00	0.00