

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF032720\
 Data File : BF119579.D
 Acq On : 27 Mar 2020 20:55
 Operator : CG/JU
 Sample : PB127867TB
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB127867TB

Quant Time: Mar 28 03:17:42 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF031820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 27 07:52:09 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.83	152	317126	20.00	ng	0.00
21) Naphthalene-d8	8.12	136	1217362	20.00	ng	0.00
39) Acenaphthene-d10	9.87	164	651085	20.00	ng	-0.01
64) Phenanthrene-d10	11.36	188	1105989	20.00	ng	0.00
76) Chrysene-d12	14.00	240	923889	20.00	ng	-0.01
87) Perylene-d12	15.46	264	742366	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.45	112	2520480	126.52	ng	0.01
7) Phenol-d6	6.46	99	3180441	124.98	ng	0.00
23) Nitrobenzene-d5	7.39	82	2024446	90.38	ng	-0.01
42) 2,4,6-Tribromophenol	10.67	330	815725	121.44	ng	0.00
45) 2-Fluorobiphenyl	9.20	172	3607085	82.08	ng	0.00
79) Terphenyl-d14	12.96	244	3932407	83.39	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF032720\
Data File : BF119579.D
Acq On : 27 Mar 2020 20:55
Operator : CG/JU
Sample : PB127867TB
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB127867TB

Quant Time: Mar 28 03:17:42 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF031820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 27 07:52:09 2020
Response via : Initial Calibration

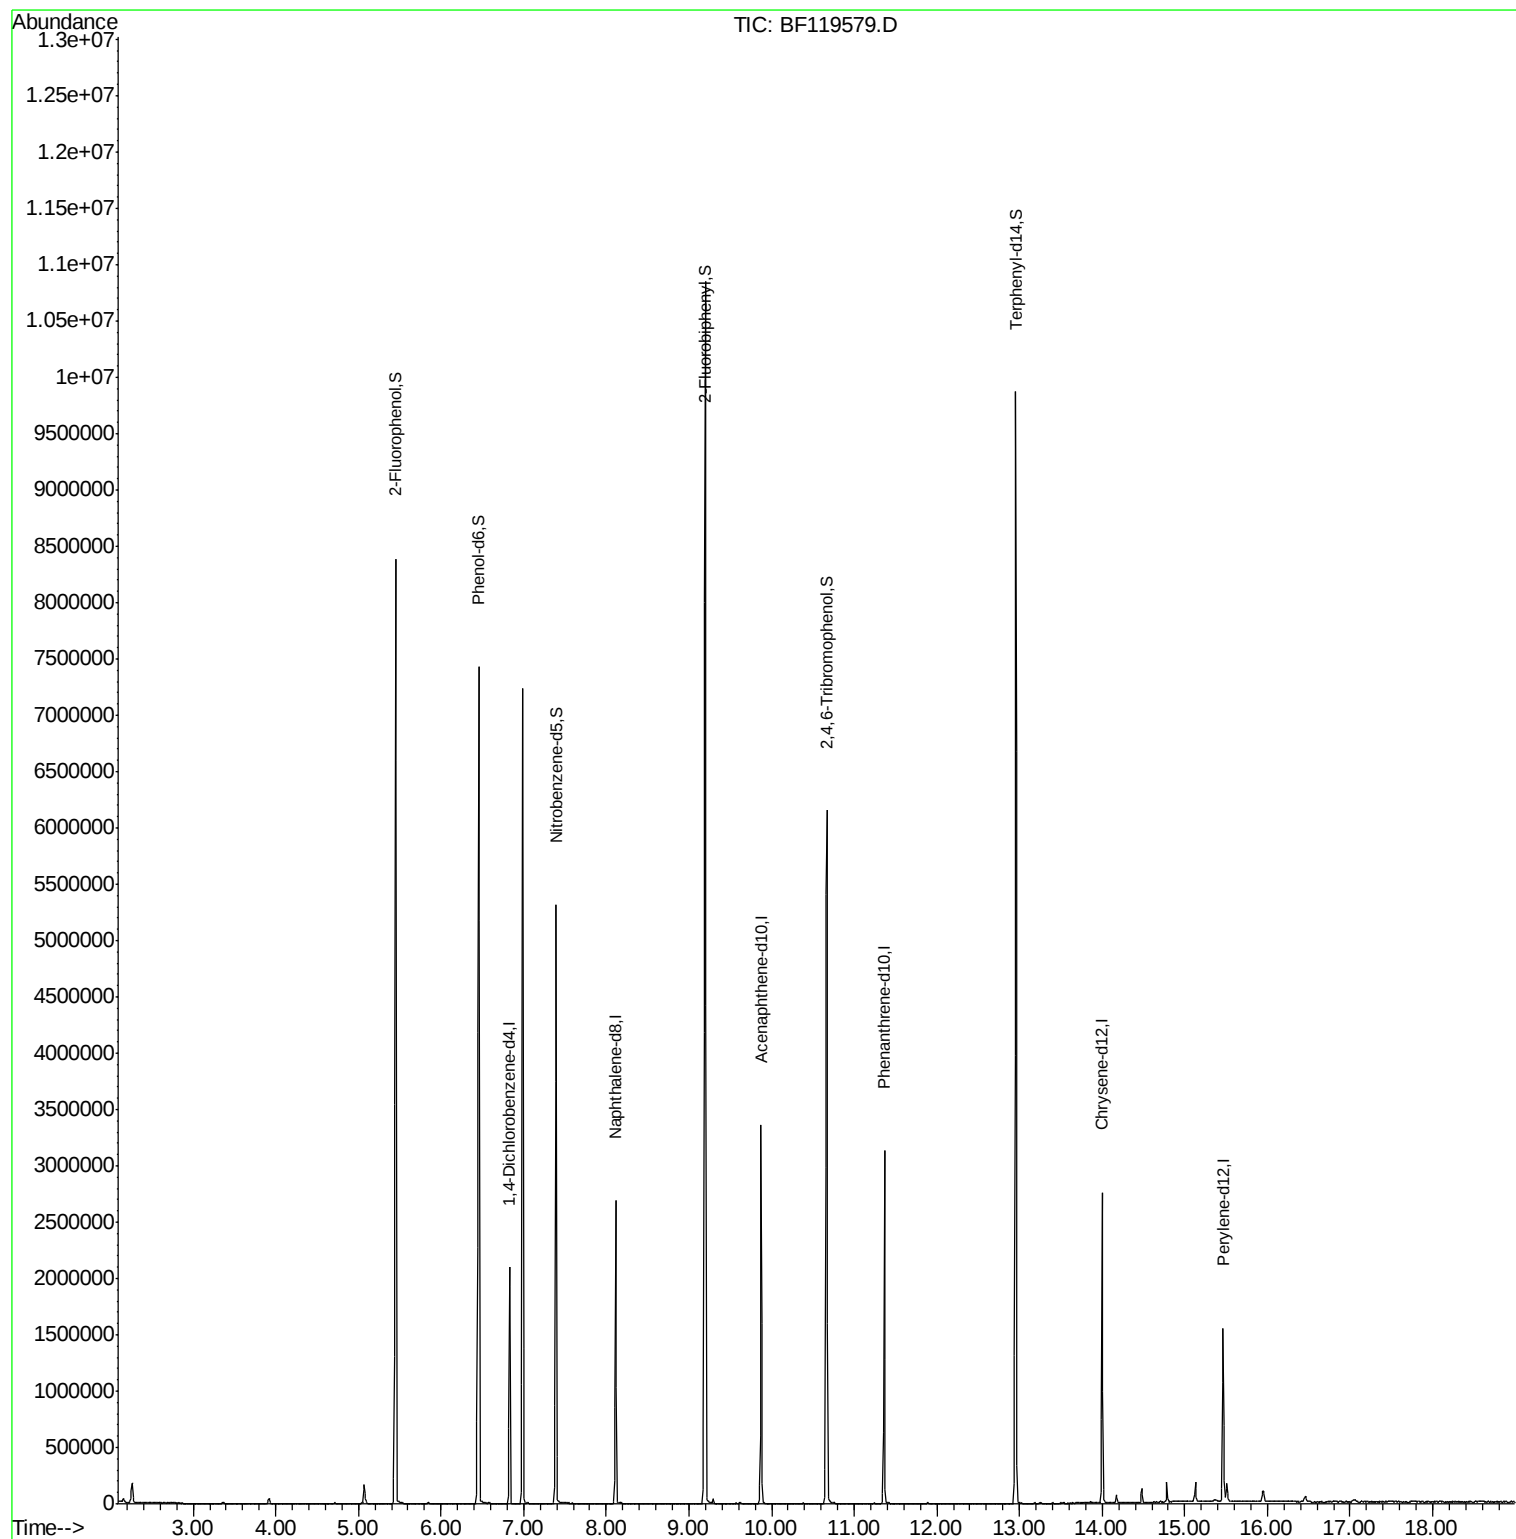

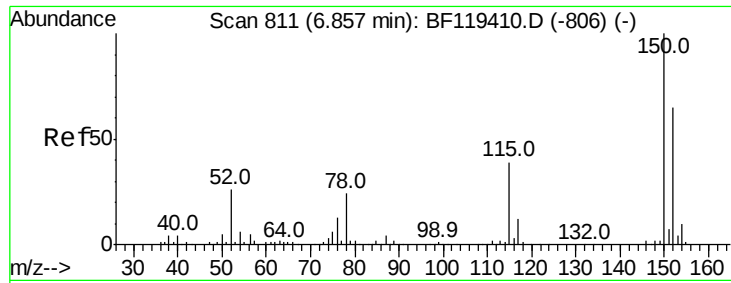


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.83 min Scan# 806
Delta R.T. -0.01 min
Lab File: BF119579.D
Acq: 27 Mar 2020 20:55

Instrument :
BNA_F
ClientSampleId :
PB127867TB

Tot Ion:152 Resp: 317126
Ion Ratio Lower Upper
152 100
150 154.5 124.5 186.7
115 62.5 49.6 74.4

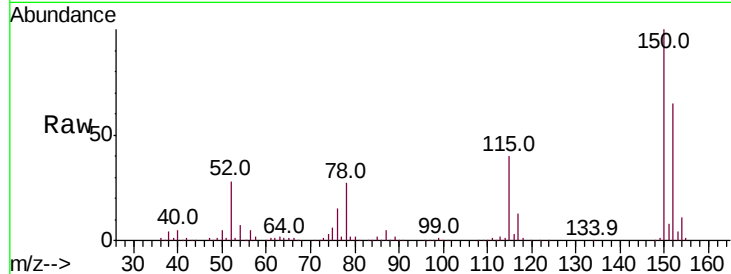


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

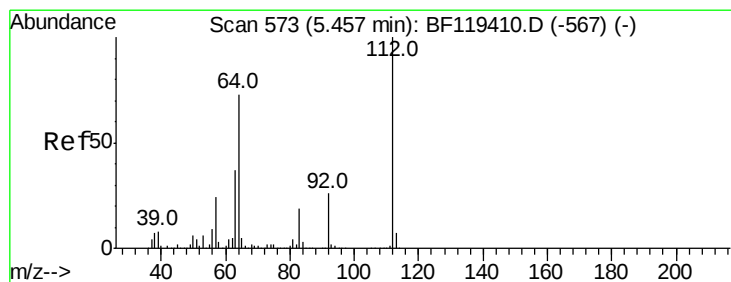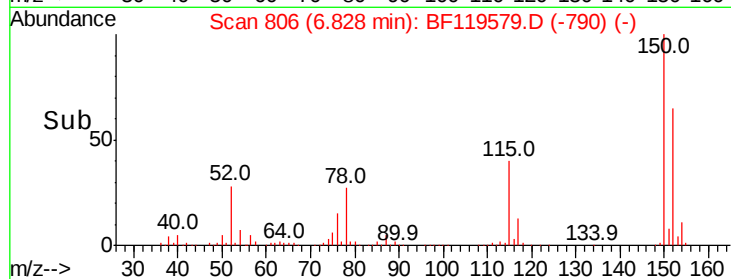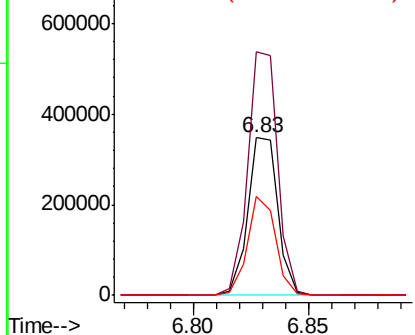



#5


2-Fluorophenol
Concen: 126.523 ng
RT: 5.45 min Scan# 572
Delta R.T. 0.01 min
Lab File: BF119579.D
Acq: 27 Mar 2020 20:55

Tgt Ion:112 Resp: 2520480
Ion Ratio Lower Upper
112 100
64 71.8 56.7 85.1
63 37.8 29.5 44.3

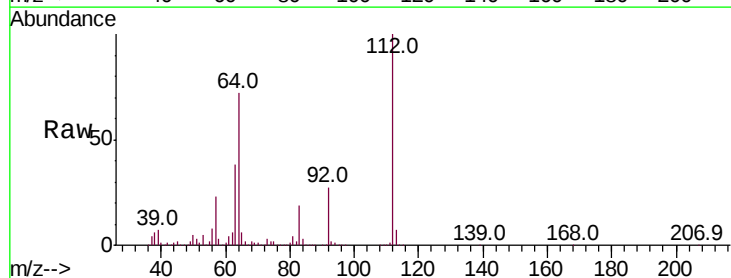

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

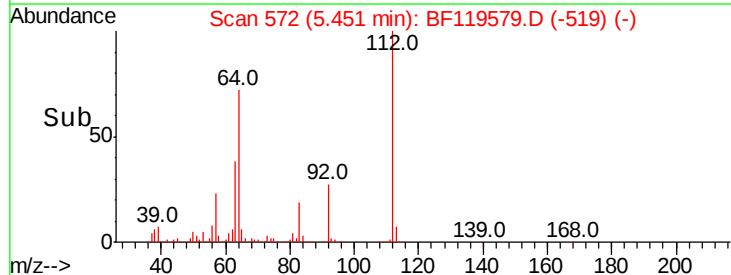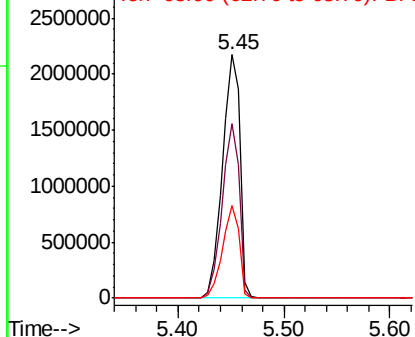

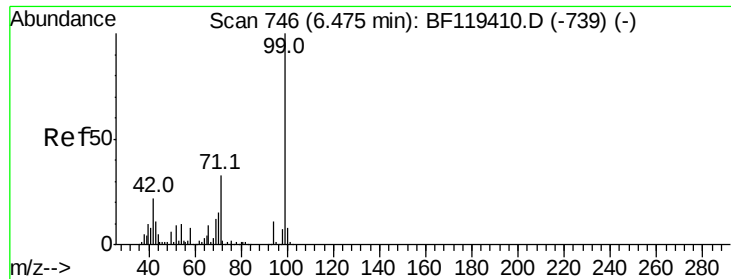

#7

Phenol-d6

Concen: 124.979 ng

RT: 6.46 min Scan# 743

Delta R.T. -0.01 min

Lab File: BF119579.D

Acq: 27 Mar 2020 20:55

Instrument :

BNA_F

ClientSampleId :

PB127867TB


Tot Ion: 99 Resp: 3180441

Ion Ratio Lower Upper

99 100

42 20.9 16.6 24.8




71 34.1 26.4 39.6

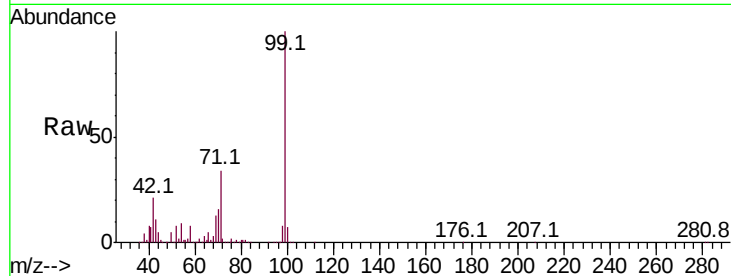

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

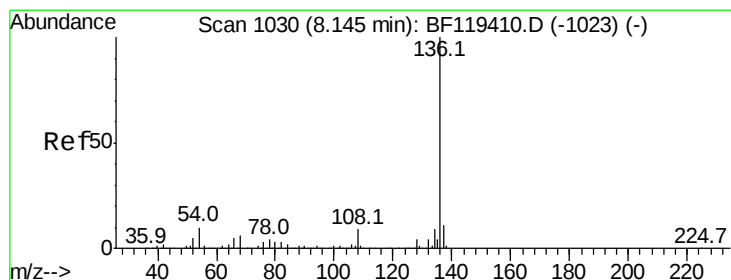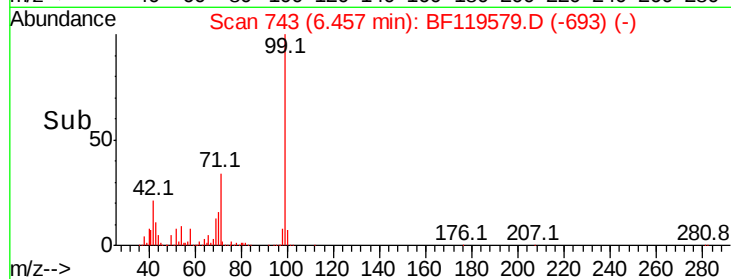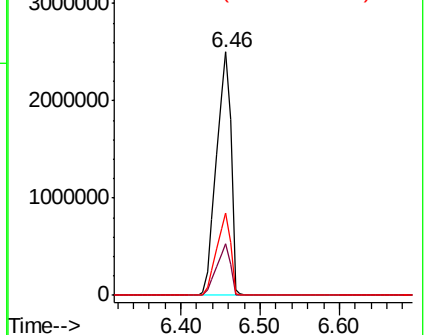

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.12 min Scan# 1025

Delta R.T. -0.01 min

Lab File: BF119579.D

Acq: 27 Mar 2020 20:55

Tgt Ion: 136 Resp: 1217362


Ion Ratio Lower Upper

136 100

137 11.4 8.7 13.1

54 10.4 9.1 13.7

68 5.9 4.6 6.8


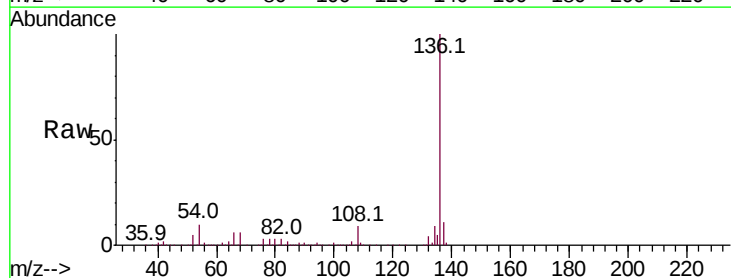



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1



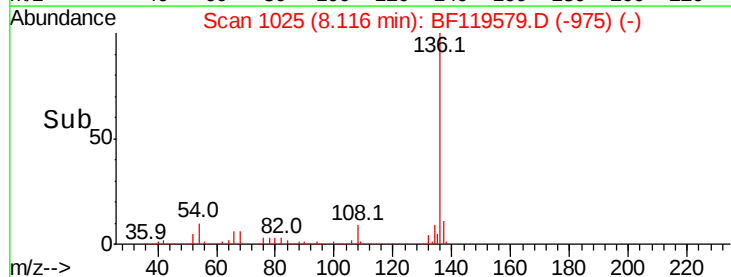
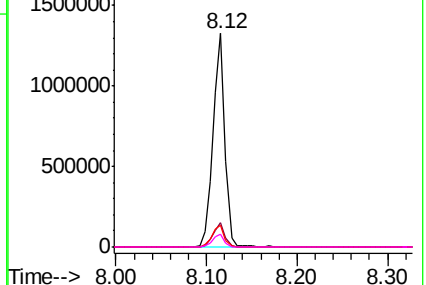


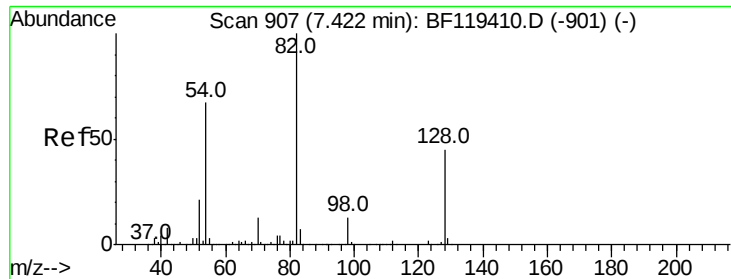

#23
Nitrobenzene-d5
Concen: 90.379 ng
RT: 7.39 min Scan# 902
Delta R.T. -0.01 min
Lab File: BF119579.D
Acq: 27 Mar 2020 20:55




Instrument :
BNA_F
ClientSampleId :
PB127867TB


Tot Ion: 82 Resp: 2024446
Ion Ratio Lower Upper
82 100
128 45.7 36.3 54.5
54 63.3 50.6 75.8

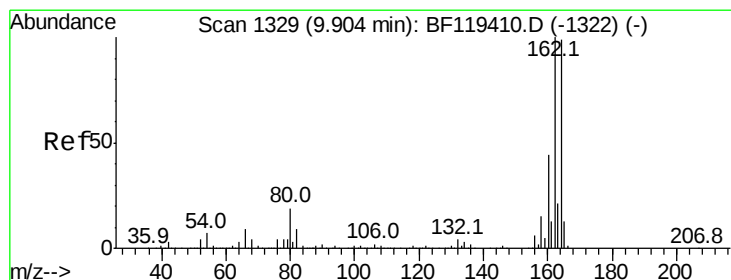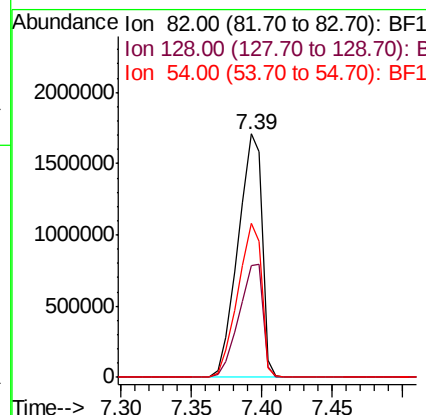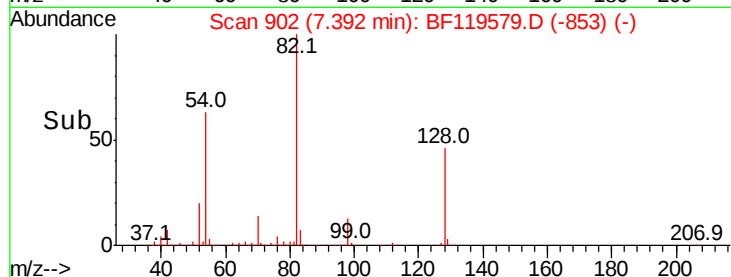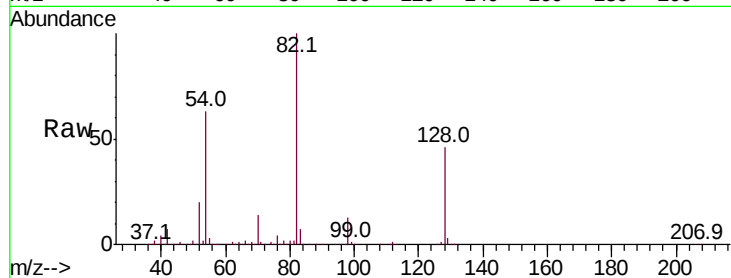

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.87 min Scan# 1324
Delta R.T. -0.01 min
Lab File: BF119579.D
Acq: 27 Mar 2020 20:55

Tgt Ion:164 Resp: 651085
Ion Ratio Lower Upper
164 100
162 102.0 80.6 121.0
160 45.8 35.7 53.5

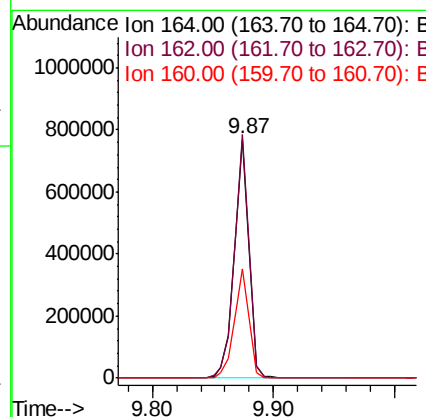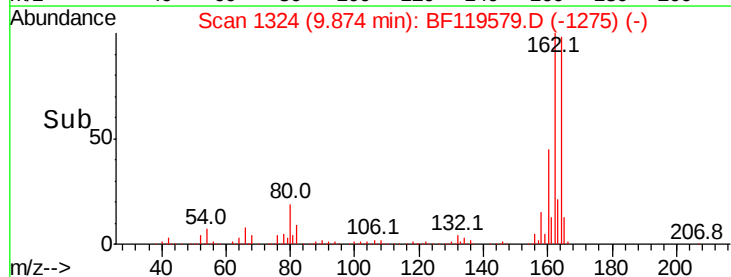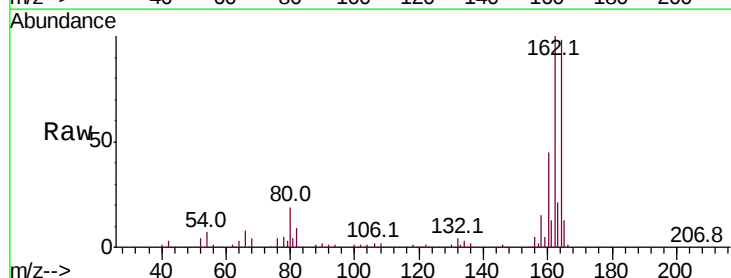


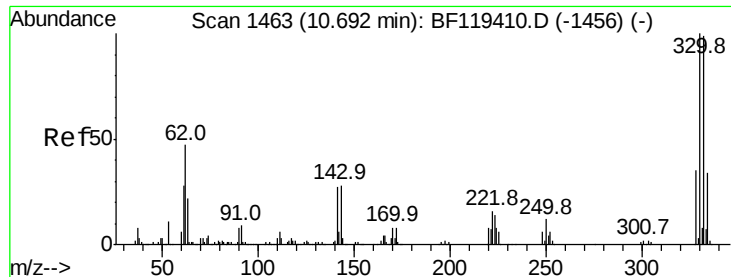




#42
 2,4,6-Tribromophenol
 Concen: 121.442 ng
 RT: 10.67 min Scan# 1459
 Delta R.T. -0.01 min
 Lab File: BF119579.D
 Acq: 27 Mar 2020 20:55

Instrument :
 BNA_F
 ClientSampleId :
 PB127867TB

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.6	75.7	113.5
141	32.3	25.4	38.0

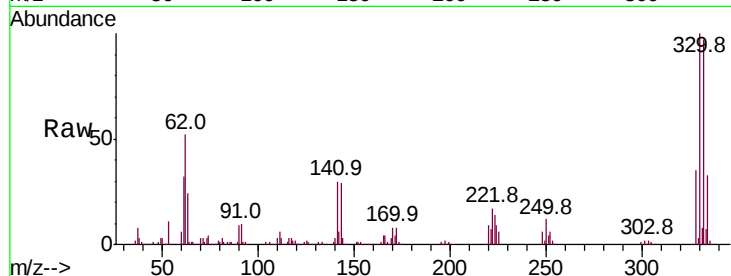


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

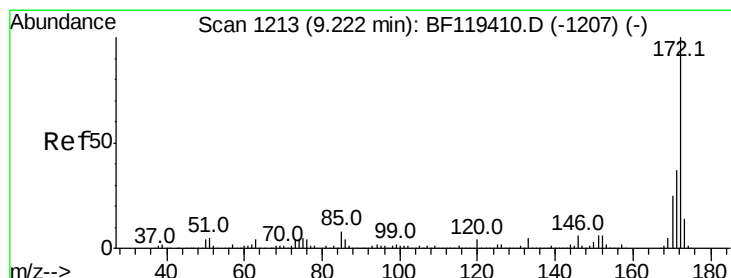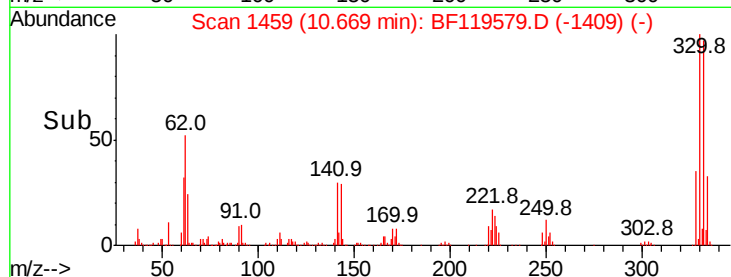
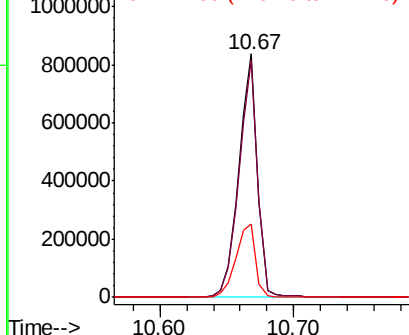



#45
 2-Fluorobiphenyl
 Concen: 82.075 ng
 RT: 9.20 min Scan# 1209
 Delta R.T. -0.01 min
 Lab File: BF119579.D
 Acq: 27 Mar 2020 20:55

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.6	29.6	44.4
170	26.0	20.2	30.2

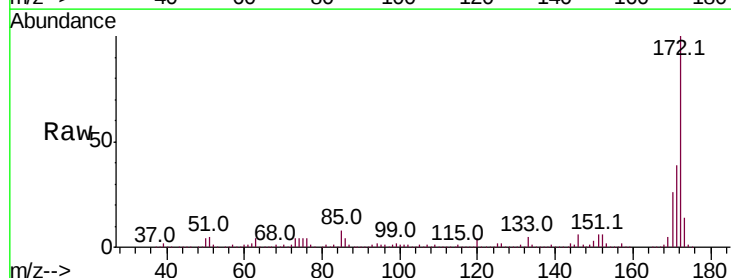

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



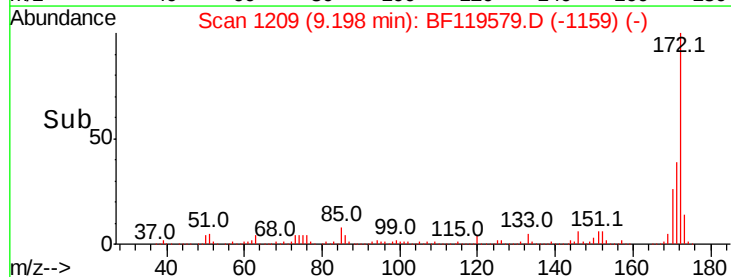
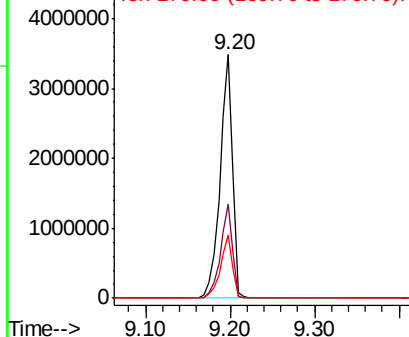


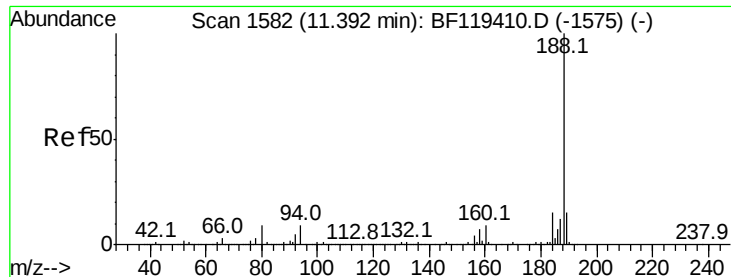

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.36 min Scan# 1577
Delta R.T. -0.01 min
Lab File: BF119579.D
Acq: 27 Mar 2020 20:55




Instrument :
BNA_F
ClientSampleId :
PB127867TB


Tot Ion:188 Resp: 1105989
Ion Ratio Lower Upper
188 100
94 8.9 7.5 11.3
80 9.8 9.0 13.4

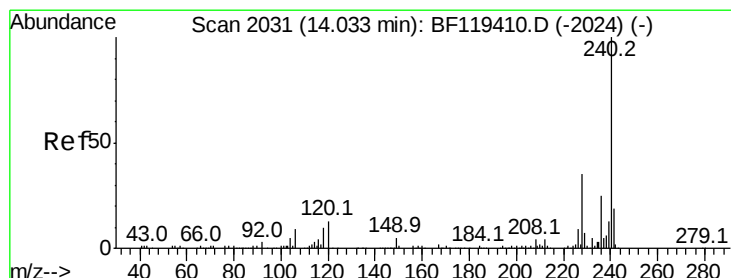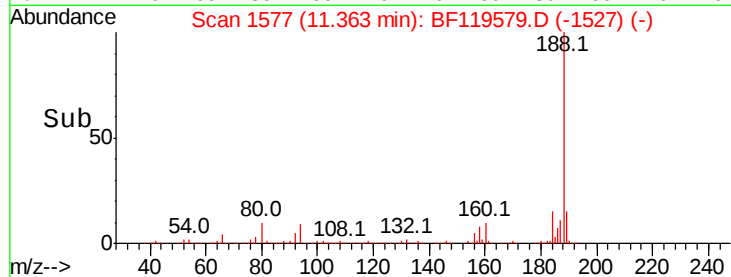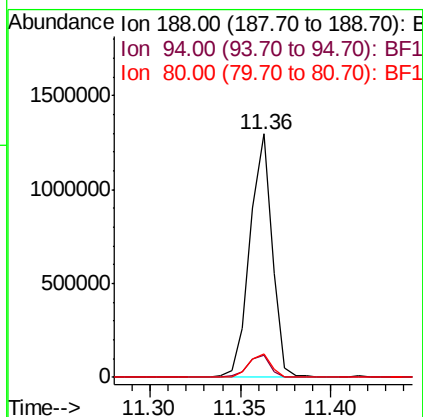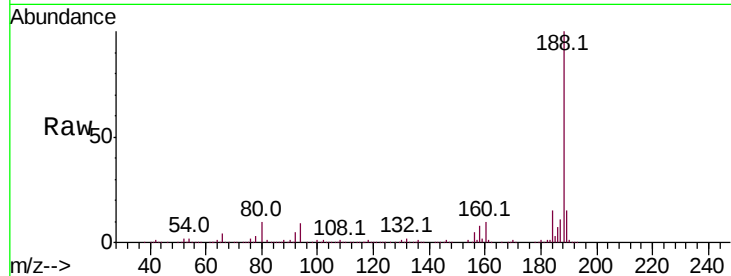

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.00 min Scan# 2026
Delta R.T. -0.01 min
Lab File: BF119579.D
Acq: 27 Mar 2020 20:55

Tgt Ion:240 Resp: 923889
Ion Ratio Lower Upper
240 100
120 11.1 10.6 15.8
236 26.1 20.2 30.2

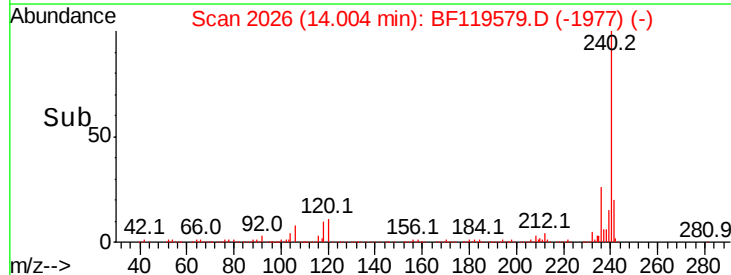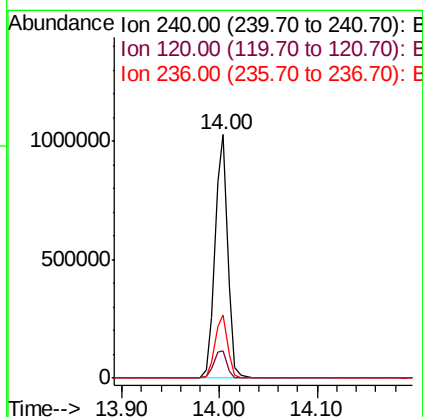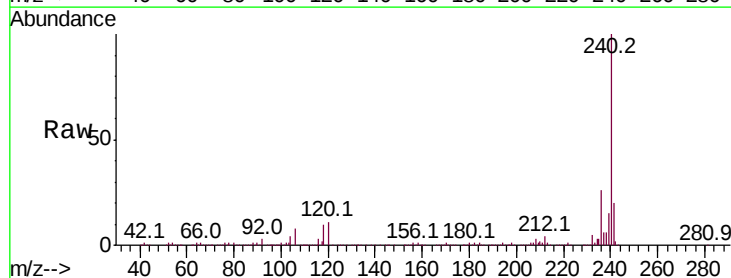

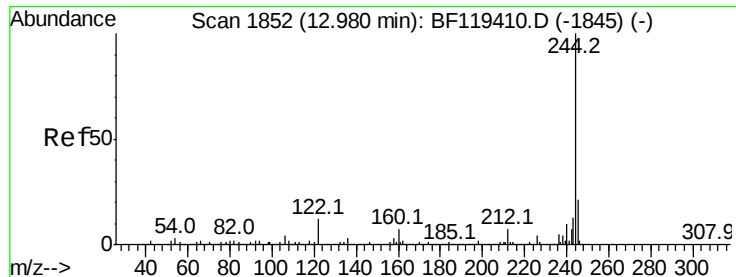

#79

Terphenyl-d14

Concen: 83.391 ng

RT: 12.96 min Scan# 1848

Delta R.T. -0.01 min

Lab File: BF119579.D

Acq: 27 Mar 2020 20:55

Instrument :


BNA_F

ClientSampleId :

PB127867TB

Tot Ion:244 Resp: 3932407




Ion	Ratio	Lower	Upper
244	100		
212	7.3	5.8	8.8
122	13.6	10.3	15.5

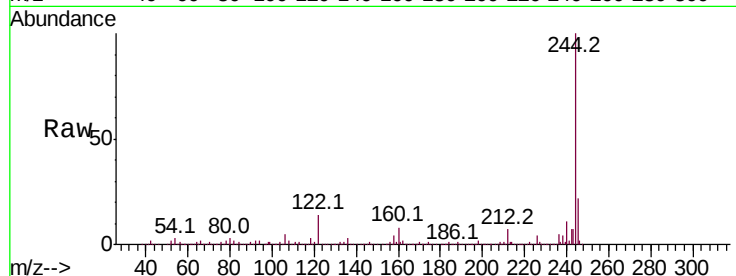

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

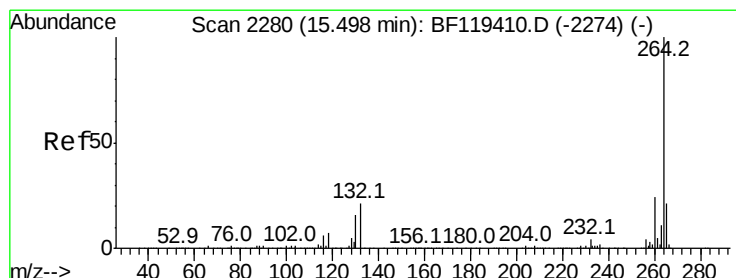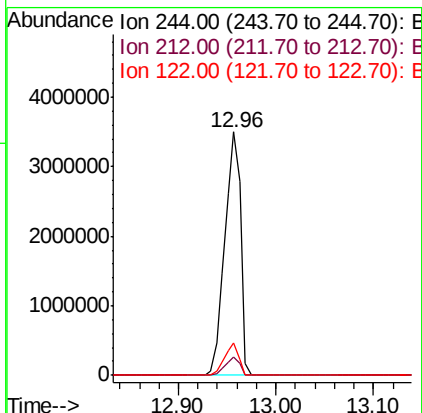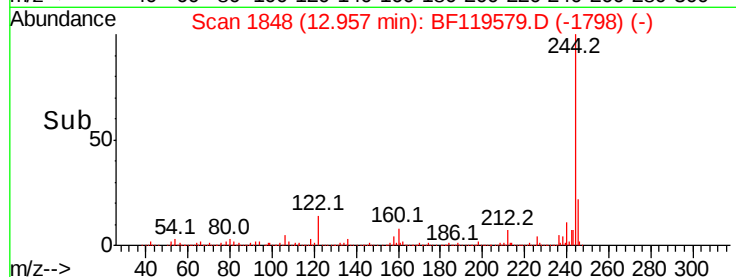

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.46 min Scan# 2274


Delta R.T. -0.02 min

Lab File: BF119579.D

Acq: 27 Mar 2020 20:55

Tgt Ion:264 Resp: 742366

Ion	Ratio	Lower	Upper
264	100		
260	23.9	18.7	28.1
265	21.3	17.7	26.5

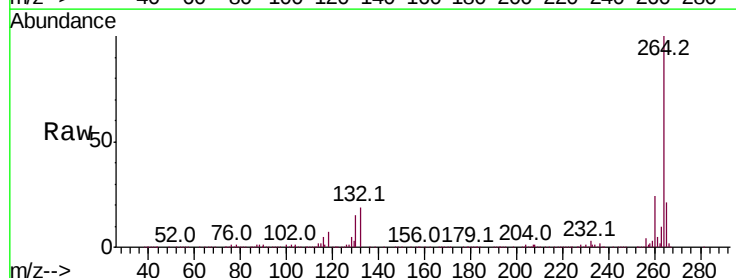

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

