

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF032720\
 Data File : BF119583.D
 Acq On : 27 Mar 2020 22:44
 Operator : CG/JU
 Sample : L2048-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 GW-1

Quant Time: Mar 28 05:24:57 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF031820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 27 07:52:09 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.83	152	314726	20.00	ng	0.00
21) Naphthalene-d8	8.12	136	1191659	20.00	ng	0.00
39) Acenaphthene-d10	9.87	164	581323	20.00	ng	-0.01
64) Phenanthrene-d10	11.36	188	1029492	20.00	ng	0.00
76) Chrysene-d12	14.00	240	744148	20.00	ng	-0.01
87) Perylene-d12	15.46	264	757067	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.45	112	1542519	78.02	ng	0.00
7) Phenol-d6	6.45	99	1311044	51.91	ng	-0.01
23) Nitrobenzene-d5	7.40	82	2124514	96.89	ng	0.00
42) 2,4,6-Tribromophenol	10.67	330	912043	152.08	ng	0.00
45) 2-Fluorobiphenyl	9.20	172	3541259	90.25	ng	0.00
79) Terphenyl-d14	12.96	244	3545789	93.35	ng	0.00
Target Compounds						
50) Dimethylphthalate	9.59	163	886854	21.478	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF032720\
Data File : BF119583.D
Acq On : 27 Mar 2020 22:44
Operator : CG/JU
Sample : L2048-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
GW-1

Quant Time: Mar 28 05:24:57 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF031820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 27 07:52:09 2020
Response via : Initial Calibration

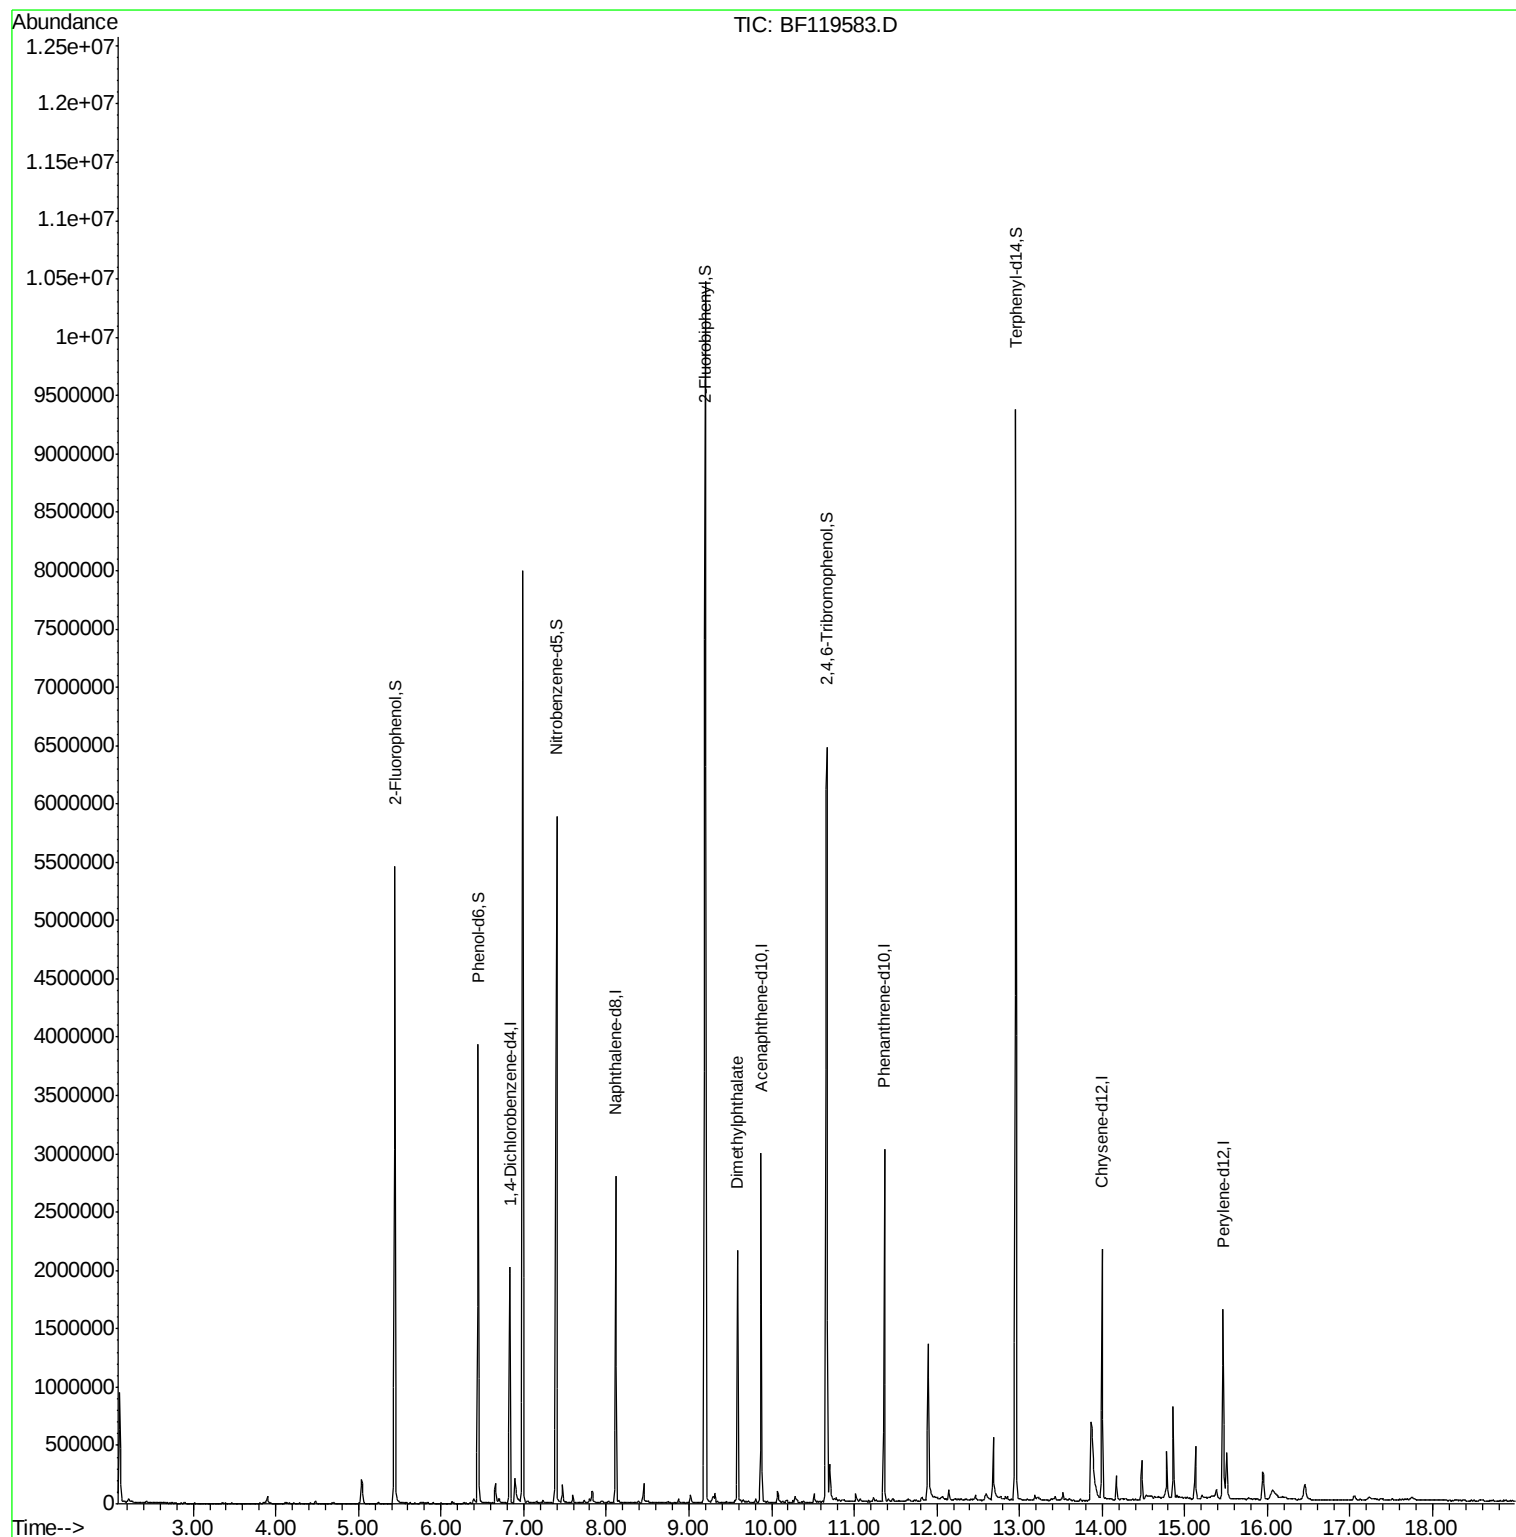

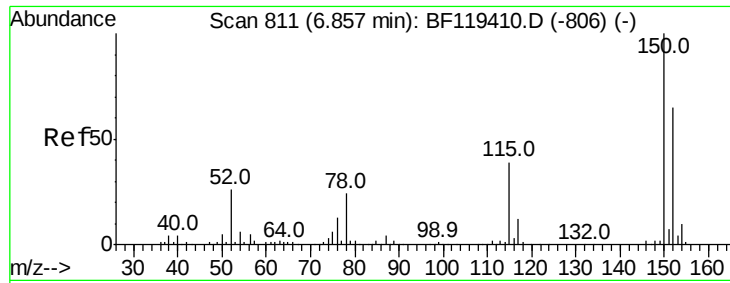


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.83 min Scan# 807
Delta R.T. -0.00 min
Lab File: BF119583.D
Acq: 27 Mar 2020 22:44

Instrument :
BNA_F
ClientSampleId :
GW-1

Tot Ion:152 Resp: 314726
Ion Ratio Lower Upper
152 100
150 152.7 124.5 186.7
115 56.4 49.6 74.4

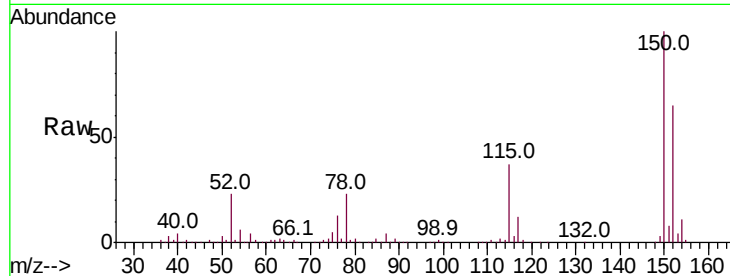


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

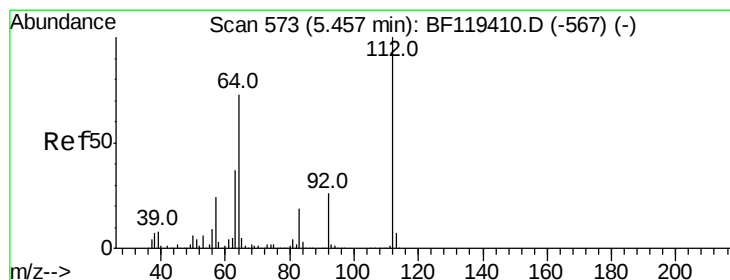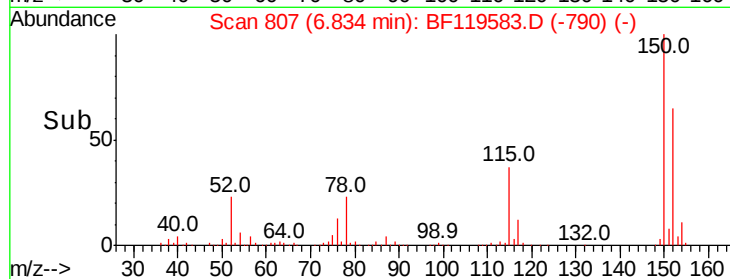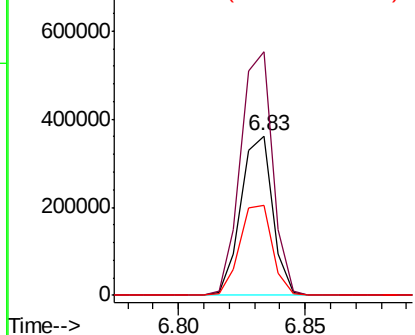



#5


2-Fluorophenol
Concen: 78.022 ng
RT: 5.45 min Scan# 571
Delta R.T. 0.01 min
Lab File: BF119583.D
Acq: 27 Mar 2020 22:44

Tgt Ion:112 Resp: 1542519
Ion Ratio Lower Upper
112 100
64 66.2 56.7 85.1
63 34.0 29.5 44.3

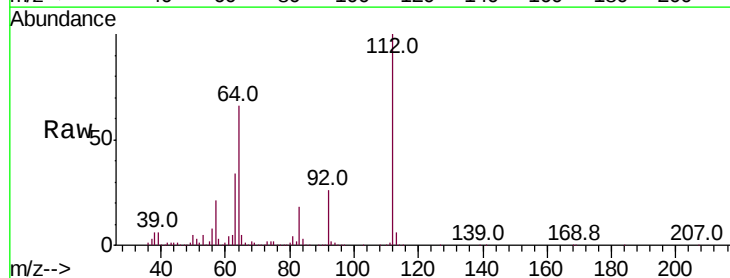

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

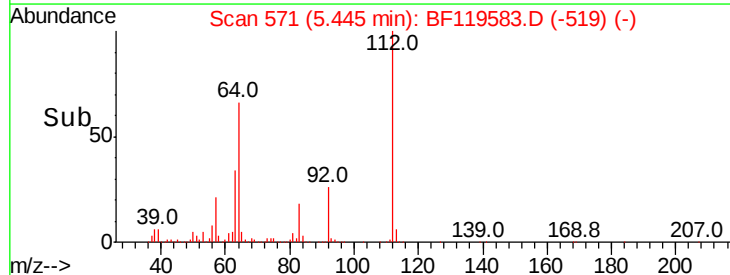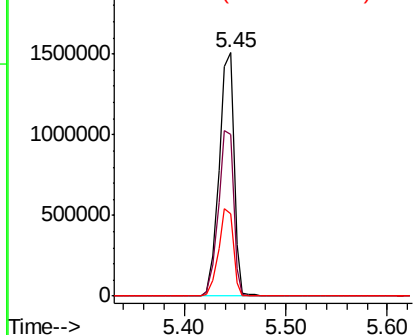



#7

Phenol-d6

Concen: 51.912 ng

RT: 6.45 min Scan# 742

Delta R.T. -0.01 min

Lab File: BF119583.D

Acq: 27 Mar 2020 22:44

Instrument :

BNA_F

ClientSampleId :

GW-1


Tot Ion: 99 Resp: 1311044

Ion Ratio Lower Upper

99 100

42 19.1 16.6 24.8




71 31.2 26.4 39.6



Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

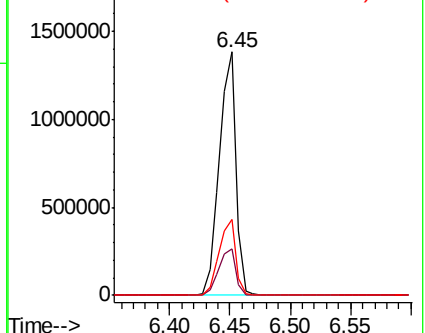

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.12 min Scan# 1025

Delta R.T. -0.01 min

Lab File: BF119583.D

Acq: 27 Mar 2020 22:44

Tgt Ion: 136 Resp: 1191659


Ion Ratio Lower Upper

136 100

137 10.9 8.7 13.1

54 10.1 9.1 13.7

68 5.9 4.6 6.8






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

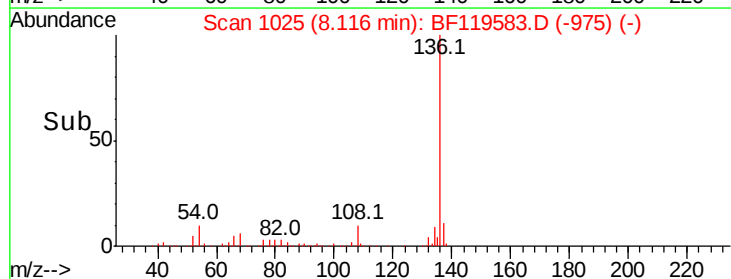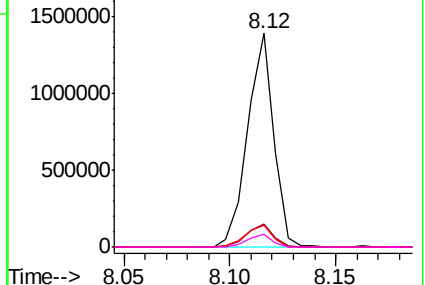




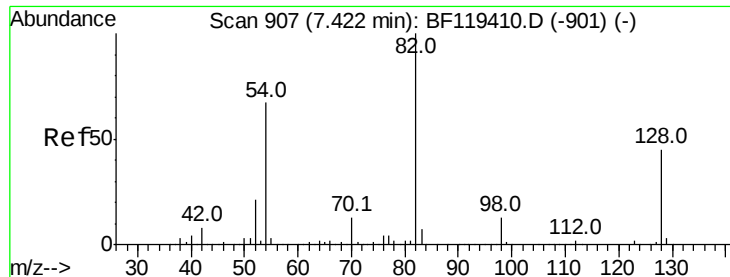


#23
 Nitrobenzene-d5
 Concen: 96.893 ng
 RT: 7.40 min Scan# 903
 Delta R.T. -0.01 min
 Lab File: BF119583.D
 Acq: 27 Mar 2020 22:44

Instrument :
 BNA_F
 ClientSampled :
 GW-1

Tot Ion: 82 Resp: 2124514




Ion	Ratio	Lower	Upper
82	100		
128	47.6	36.3	54.5
54	61.8	50.6	75.8

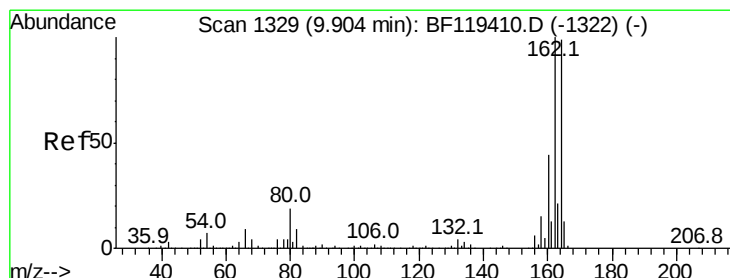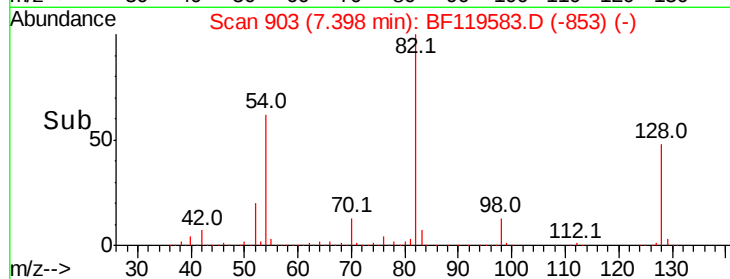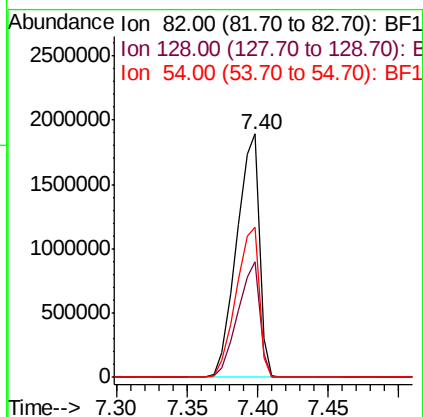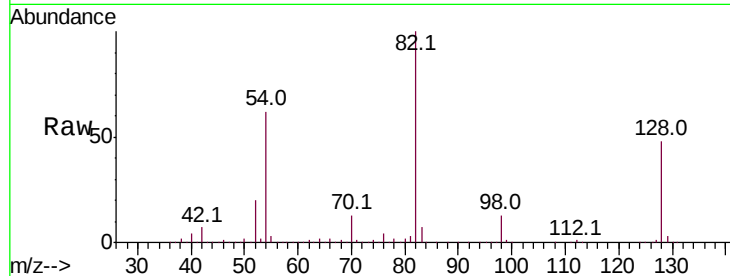


#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.87 min Scan# 1324
 Delta R.T. -0.01 min
 Lab File: BF119583.D
 Acq: 27 Mar 2020 22:44

Tgt Ion:164 Resp: 581323

Ion	Ratio	Lower	Upper
164	100		
162	103.0	80.6	121.0
160	46.8	35.7	53.5

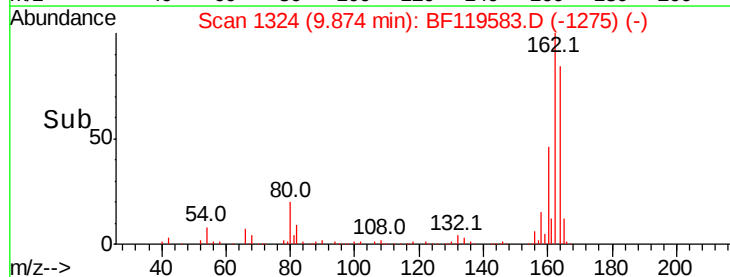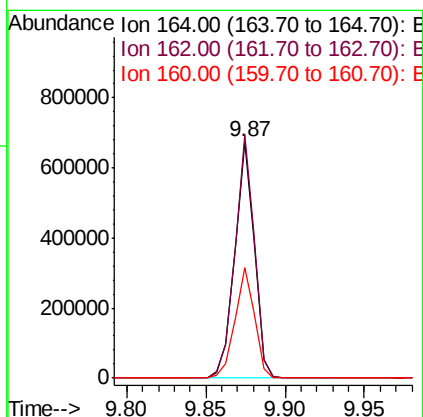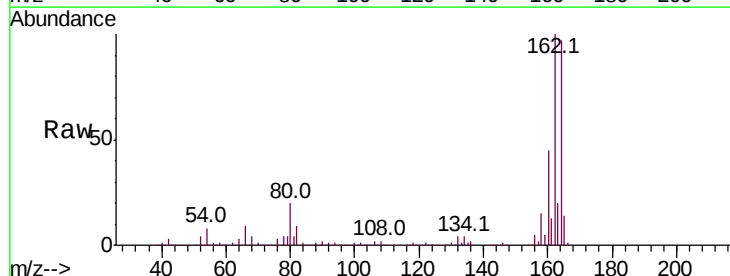



#42

2,4,6-Tribromophenol

Concen: 152.075 ng

RT: 10.67 min Scan# 1459

Delta R.T. -0.01 min

Lab File: BF119583.D

Acq: 27 Mar 2020 22:44

Instrument :

BNA_F

ClientSampleId :

GW-1


Tot Ion:330 Resp: 912043

Ion Ratio Lower Upper

330 100

332 95.9 75.7 113.5




141 31.5 25.4 38.0

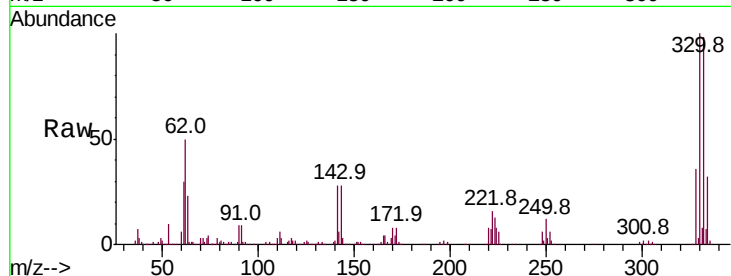

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

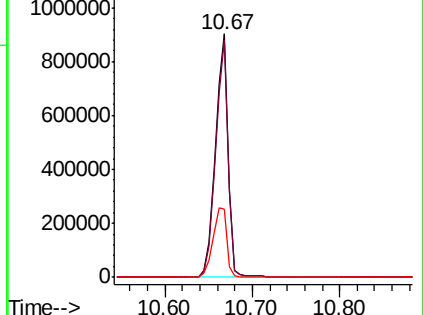

#45

2-Fluorobiphenyl

Concen: 90.247 ng

RT: 9.20 min Scan# 1209

Delta R.T. -0.01 min

Lab File: BF119583.D

Acq: 27 Mar 2020 22:44


Tgt Ion:172 Resp: 3541259

Ion Ratio Lower Upper

172 100

171 38.3 29.6 44.4



170 25.9 20.2 30.2




Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

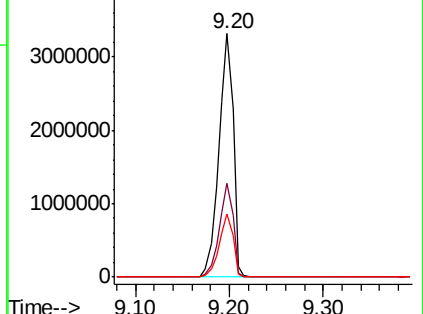







#50
Dimethylphthalate
Concen: 21.478 ng
RT: 9.59 min Scan# 1276
Delta R.T. -0.02 min
Lab File: BF119583.D
Acq: 27 Mar 2020 22:44

Instrument :
BNA_F
ClientSampleId :
GW-1

Tot Ion:163 Resp: 886854
Ion Ratio Lower Upper
163 100
194 4.2 3.1 4.7
164 9.8 8.2 12.2

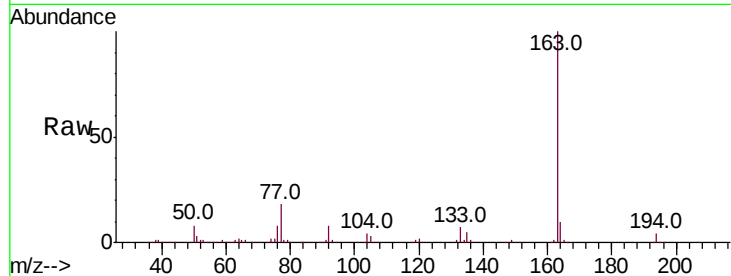


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

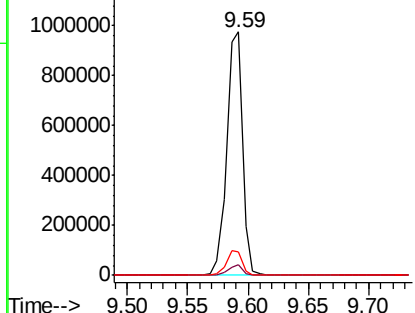
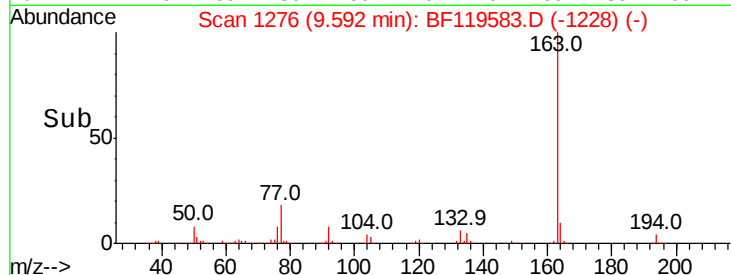



#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.36 min Scan# 1577
Delta R.T. -0.01 min
Lab File: BF119583.D
Acq: 27 Mar 2020 22:44

Tgt Ion:188 Resp: 1029492
Ion Ratio Lower Upper
188 100
94 9.1 7.5 11.3
80 9.4 9.0 13.4



Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

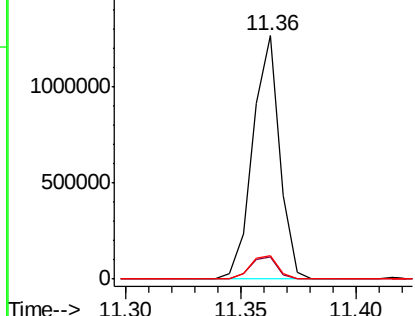



#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.00 min Scan# 2026

Delta R.T. -0.01 min

Lab File: BF119583.D

Acq: 27 Mar 2020 22:44

Instrument :

BNA_F

ClientSampleID :

GW-1


Tot Ion:240 Resp: 744148

Ion Ratio Lower Upper

240 100

120 10.4 10.6 15.8#




236 25.9 20.2 30.2



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

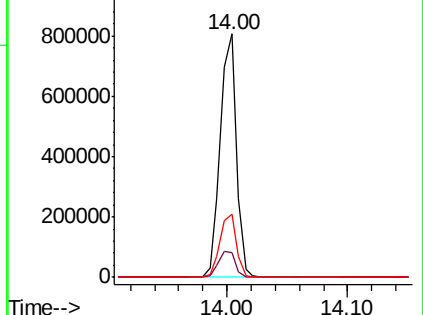

#79

Terphenyl-d14

Concen: 93.354 ng

RT: 12.96 min Scan# 1848

Delta R.T. -0.01 min

Lab File: BF119583.D

Acq: 27 Mar 2020 22:44


Tgt Ion:244 Resp: 3545789

Ion Ratio Lower Upper

244 100

212 7.1 5.8 8.8



122 13.1 10.3 15.5




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

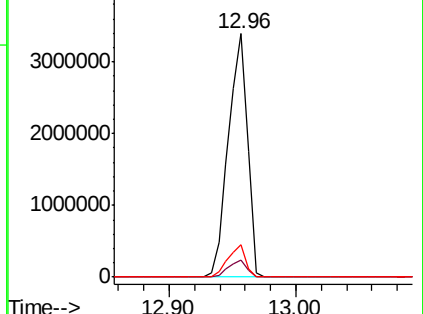

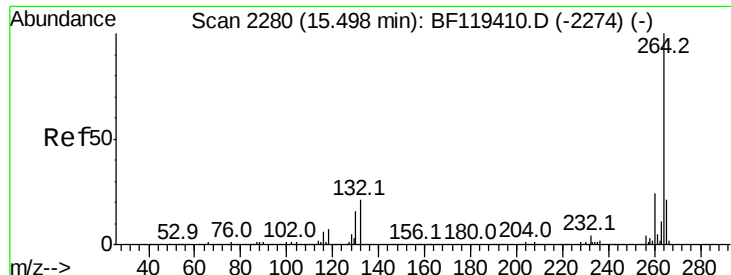

#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.46 min Scan# 2274
 Delta R.T. -0.02 min
 Lab File: BF119583.D
 Acq: 27 Mar 2020 22:44

Instrument :
 BNA_F
 ClientSampleId :
 GW-1

Tot Ion:	264	Resp:	757067
Ion	Ratio	Lower	Upper
264	100		
260	22.7	18.7	28.1
265	21.2	17.7	26.5

