


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032720\
 Data File : BF119569.D
 Acq On : 27 Mar 2020 16:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 27 07:52:09 2020

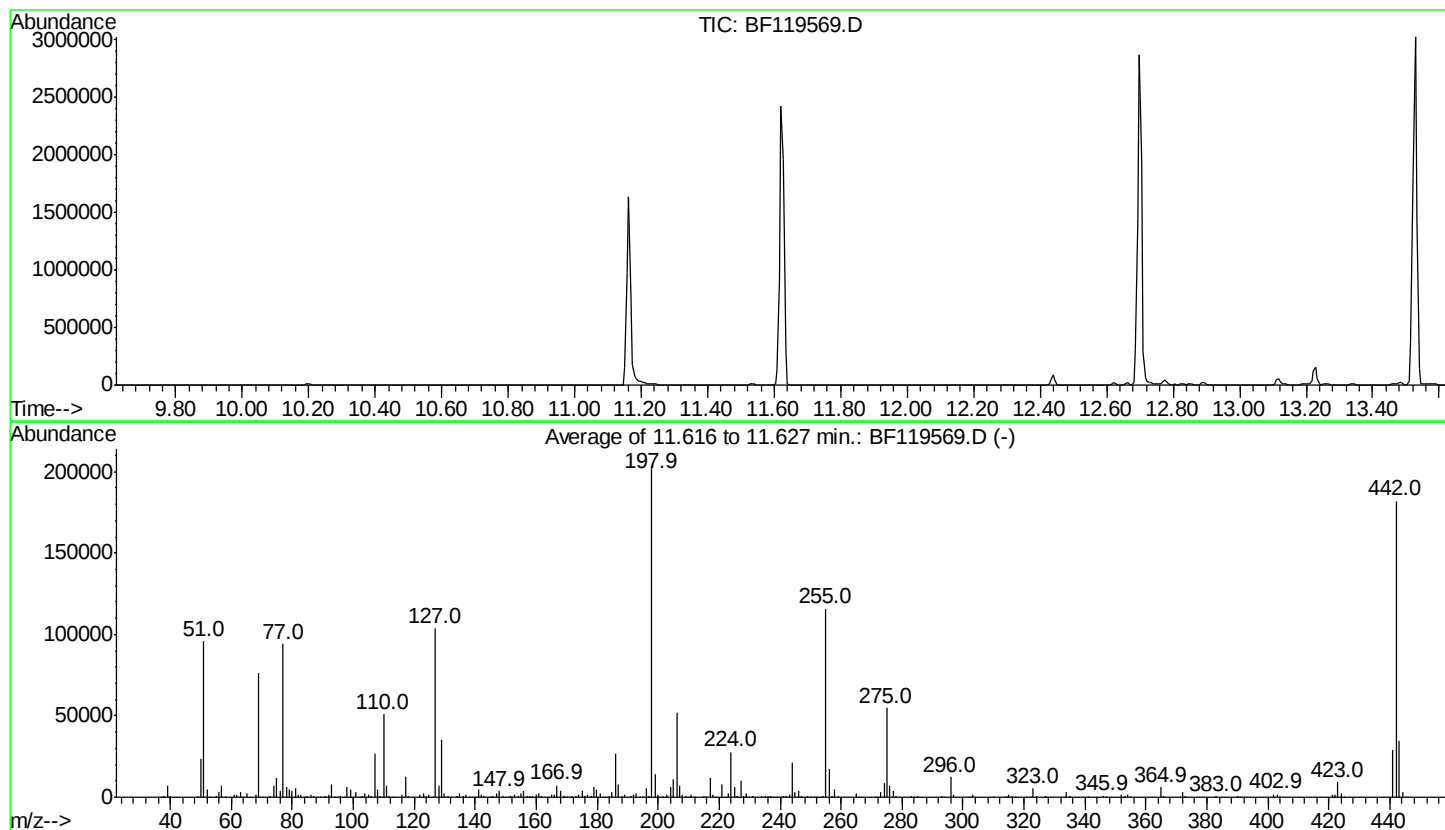

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.0	95805	PASS
68	69	0.00	2	1.8	1374	PASS
69	198	0.00	100	37.6	76560	PASS
70	69	0.00	2	0.4	282	PASS
127	198	10	80	50.8	103533	PASS
197	198	0.00	2	0.5	983	PASS
198	198	100	100	100.0	203677	PASS
199	198	5	9	6.9	14050	PASS
275	198	10	60	26.9	54885	PASS
365	198	1	100	3.0	6093	PASS
441	198	0.01	100	14.3	29211	PASS
442	198	50	100	89.3	181914	PASS
443	442	15	24	18.9	34356	PASS