


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032720\
 Data File : BF119590.D
 Acq On : 28 Mar 2020 1:59
 Operator : CG/JU
 Sample : DFTTP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTTP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 27 07:52:09 2020

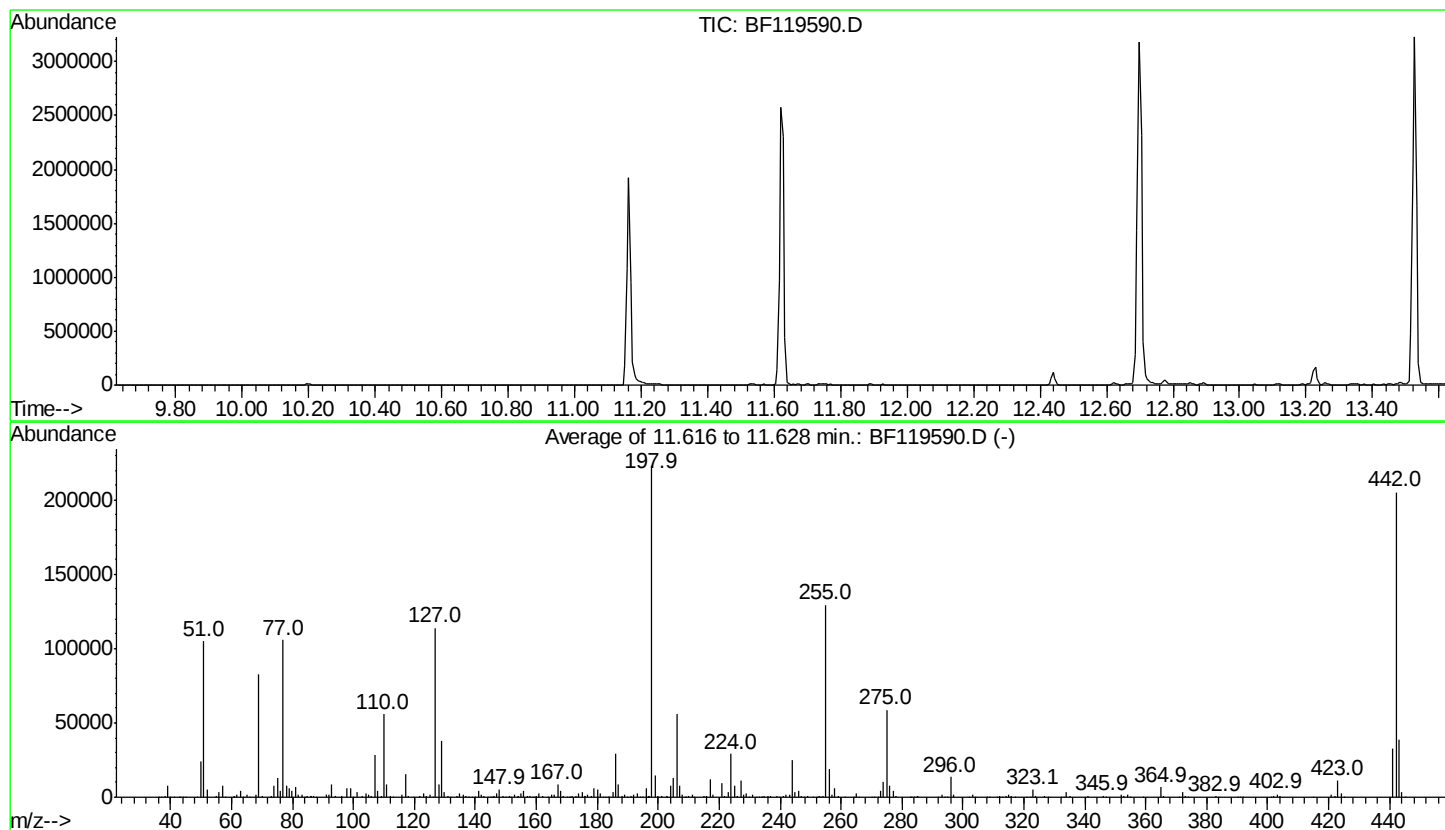

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.0	104869	PASS
68	69	0.00	2	1.7	1376	PASS
69	198	0.00	100	37.0	82613	PASS
70	69	0.00	2	0.7	585	PASS
127	198	10	80	51.1	114040	PASS
197	198	0.00	2	0.3	699	PASS
198	198	100	100	100.0	223101	PASS
199	198	5	9	6.4	14286	PASS
275	198	10	60	26.3	58584	PASS
365	198	1	100	3.0	6745	PASS
441	198	0.01	100	14.5	32370	PASS
442	198	50	100	91.9	205018	PASS
443	442	15	24	18.9	38731	PASS