


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032720\
 Data File : BF119609.D
 Acq On : 28 Mar 2020 11:22
 Operator : CG/JU
 Sample : DFTTP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTTP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 27 07:52:09 2020

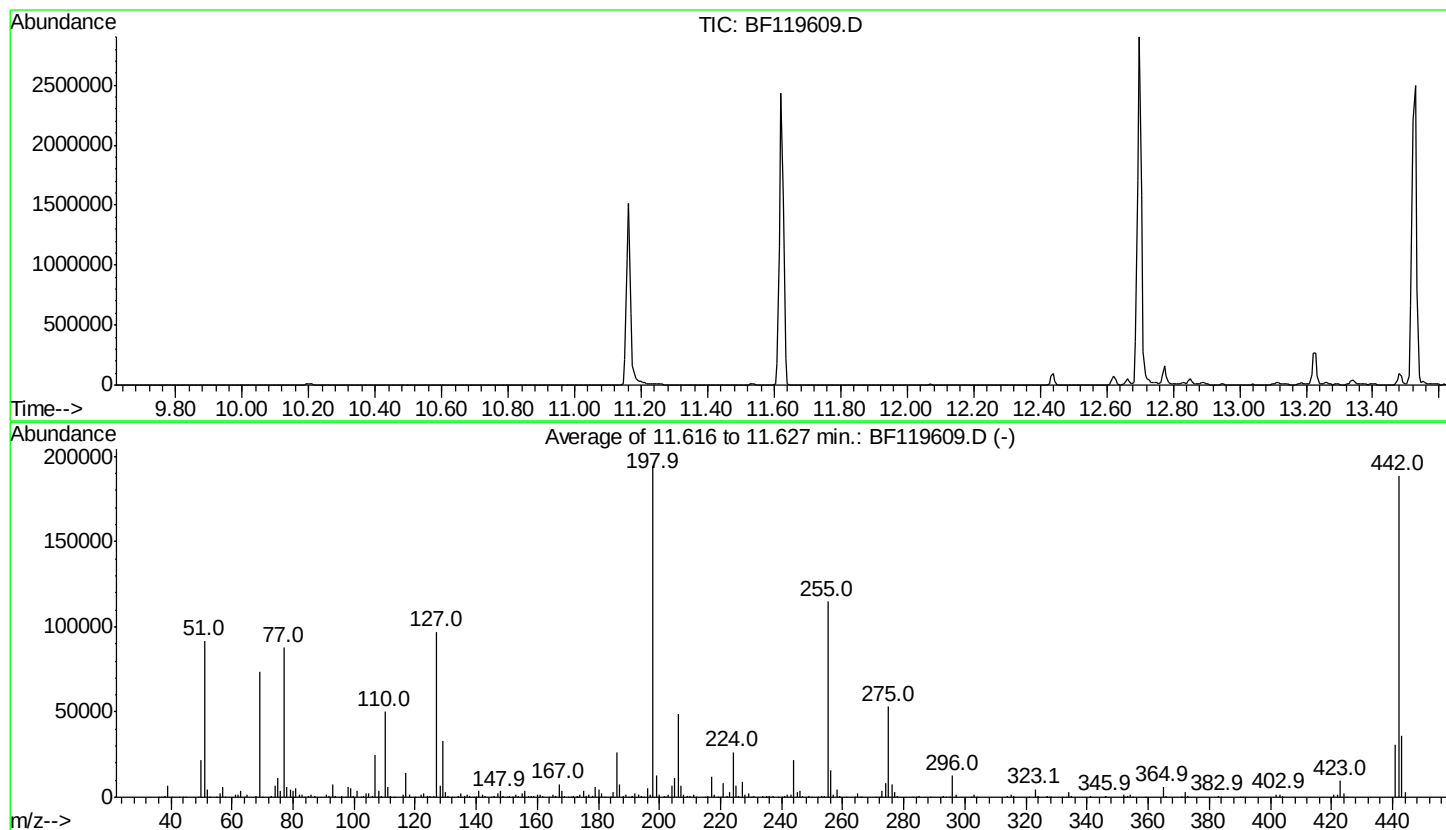

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.2	91813	PASS
68	69	0.00	2	1.5	1066	PASS
69	198	0.00	100	37.7	73298	PASS
70	69	0.00	2	0.4	299	PASS
127	198	10	80	49.9	97058	PASS
197	198	0.00	2	0.7	1318	PASS
198	198	100	100	100.0	194618	PASS
199	198	5	9	6.4	12539	PASS
275	198	10	60	27.3	53045	PASS
365	198	1	100	3.3	6403	PASS
441	198	0.01	100	15.7	30516	PASS
442	198	50	100	97.0	188768	PASS
443	442	15	24	19.1	36105	PASS