


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032819\
Data File : BF113369.D
Acq On : 28 Mar 2019 12:11
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032519.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Mar 26 03:32:08 2019

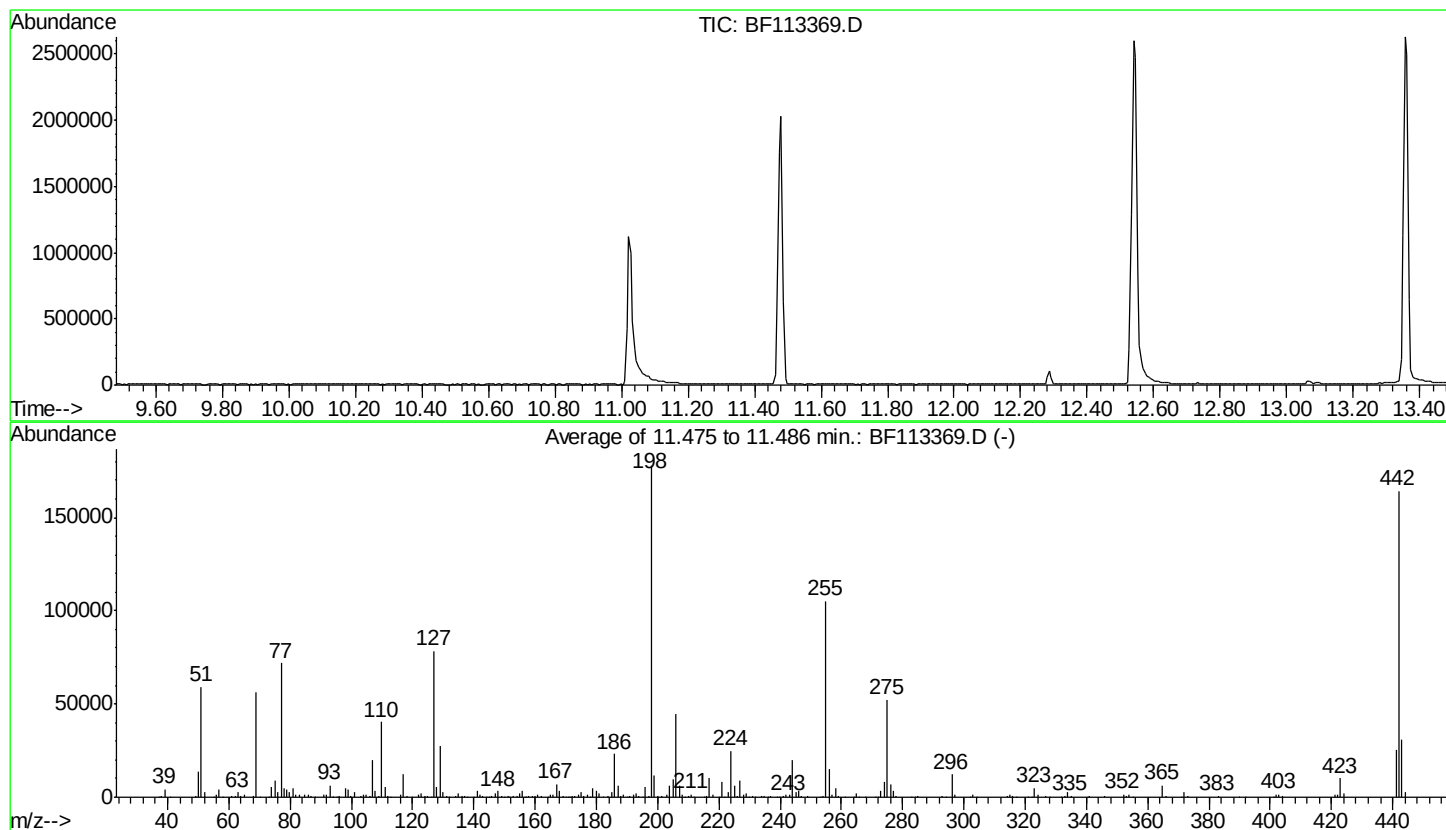

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.4	59355	PASS
68	69	0.00	2	1.6	922	PASS
69	198	0.00	100	31.6	56273	PASS
70	69	0.00	2	0.5	268	PASS
127	198	10	80	44.2	78600	PASS
197	198	0.00	2	0.6	1009	PASS
198	198	100	100	100.0	177832	PASS
199	198	5	9	6.7	11981	PASS
275	198	10	60	29.5	52538	PASS
365	198	1	100	3.5	6229	PASS
441	198	0.01	100	14.3	25448	PASS
442	198	50	100	92.3	164138	PASS
443	442	15	24	18.7	30682	PASS