


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032819\
 Data File : BF113393.D
 Acq On : 29 Mar 2019 1:17
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 26 03:32:08 2019

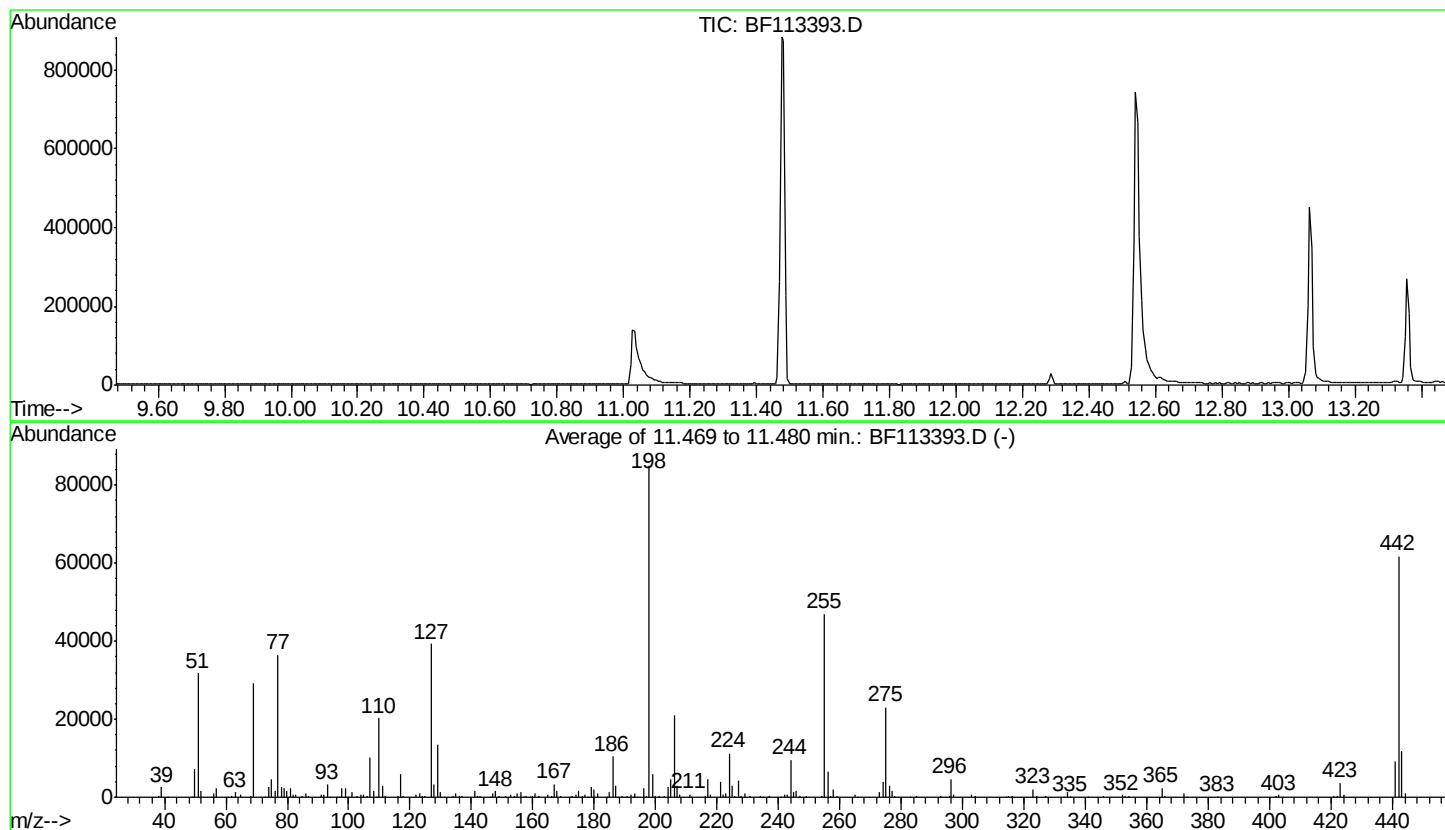

AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	31784	PASS
68	69	0.00	2	1.4	418	PASS
69	198	0.00	100	34.2	29085	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.3	39378	PASS
197	198	0.00	2	0.5	392	PASS
198	198	100	100	100.0	85026	PASS
199	198	5	9	6.8	5800	PASS
275	198	10	60	27.2	23096	PASS
365	198	1	100	2.8	2406	PASS
441	198	0.01	100	11.0	9329	PASS
442	198	50	100	72.7	61844	PASS
443	442	15	24	19.3	11928	PASS