

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032919\
 Data File : BF113440.D
 Acq On : 30 Mar 2019 4:59
 Operator : JU/SJ
 Sample : K2138-02
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 S6A(2-10)COMP

Quant Time: Mar 30 05:28:05 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 26 03:32:08 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.70	152	141283	20.00	ng	0.00
21) Naphthalene-d8	7.99	136	520341	20.00	ng	0.00
39) Acenaphthene-d10	9.73	164	230140	20.00	ng	0.00
64) Phenanthrene-d10	11.22	188	403580	20.00	ng	0.00
76) Chrysene-d12	13.85	240	421920	20.00	ng	0.00
87) Perylene-d12	15.24	264	326362	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.33	112	852066	98.61	ng	0.02
7) Phenol-d6	6.36	99	989932	90.56	ng	0.00
23) Nitrobenzene-d5	7.27	82	712627	81.29	ng	0.00
42) 2,4,6-Tribromophenol	10.52	330	328139	115.43	ng	0.00
45) 2-Fluorobiphenyl	9.06	172	1332323	92.24	ng	0.00
79) Terphenyl-d14	12.79	244	1324113	69.17	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.27	70	91899	13.385	ng	Qvalue # 76
25) Isophorone	7.27	82	709481	41.760	ng	# 64
51) 2,6-Dinitrotoluene	9.73	165	28710	7.462	ng	# 25
57) 2,4-Dinitrotoluene	9.73	165	28710	5.868	ng	# 22
67) 4-Bromophenyl-phenylether	10.52	248	17144	3.898	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032919\
Data File : BF113440.D
Acq On : 30 Mar 2019 4:59
Operator : JU/SJ
Sample : K2138-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S6A(2-10)COMP

Quant Time: Mar 30 05:28:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 26 03:32:08 2019
Response via : Initial Calibration

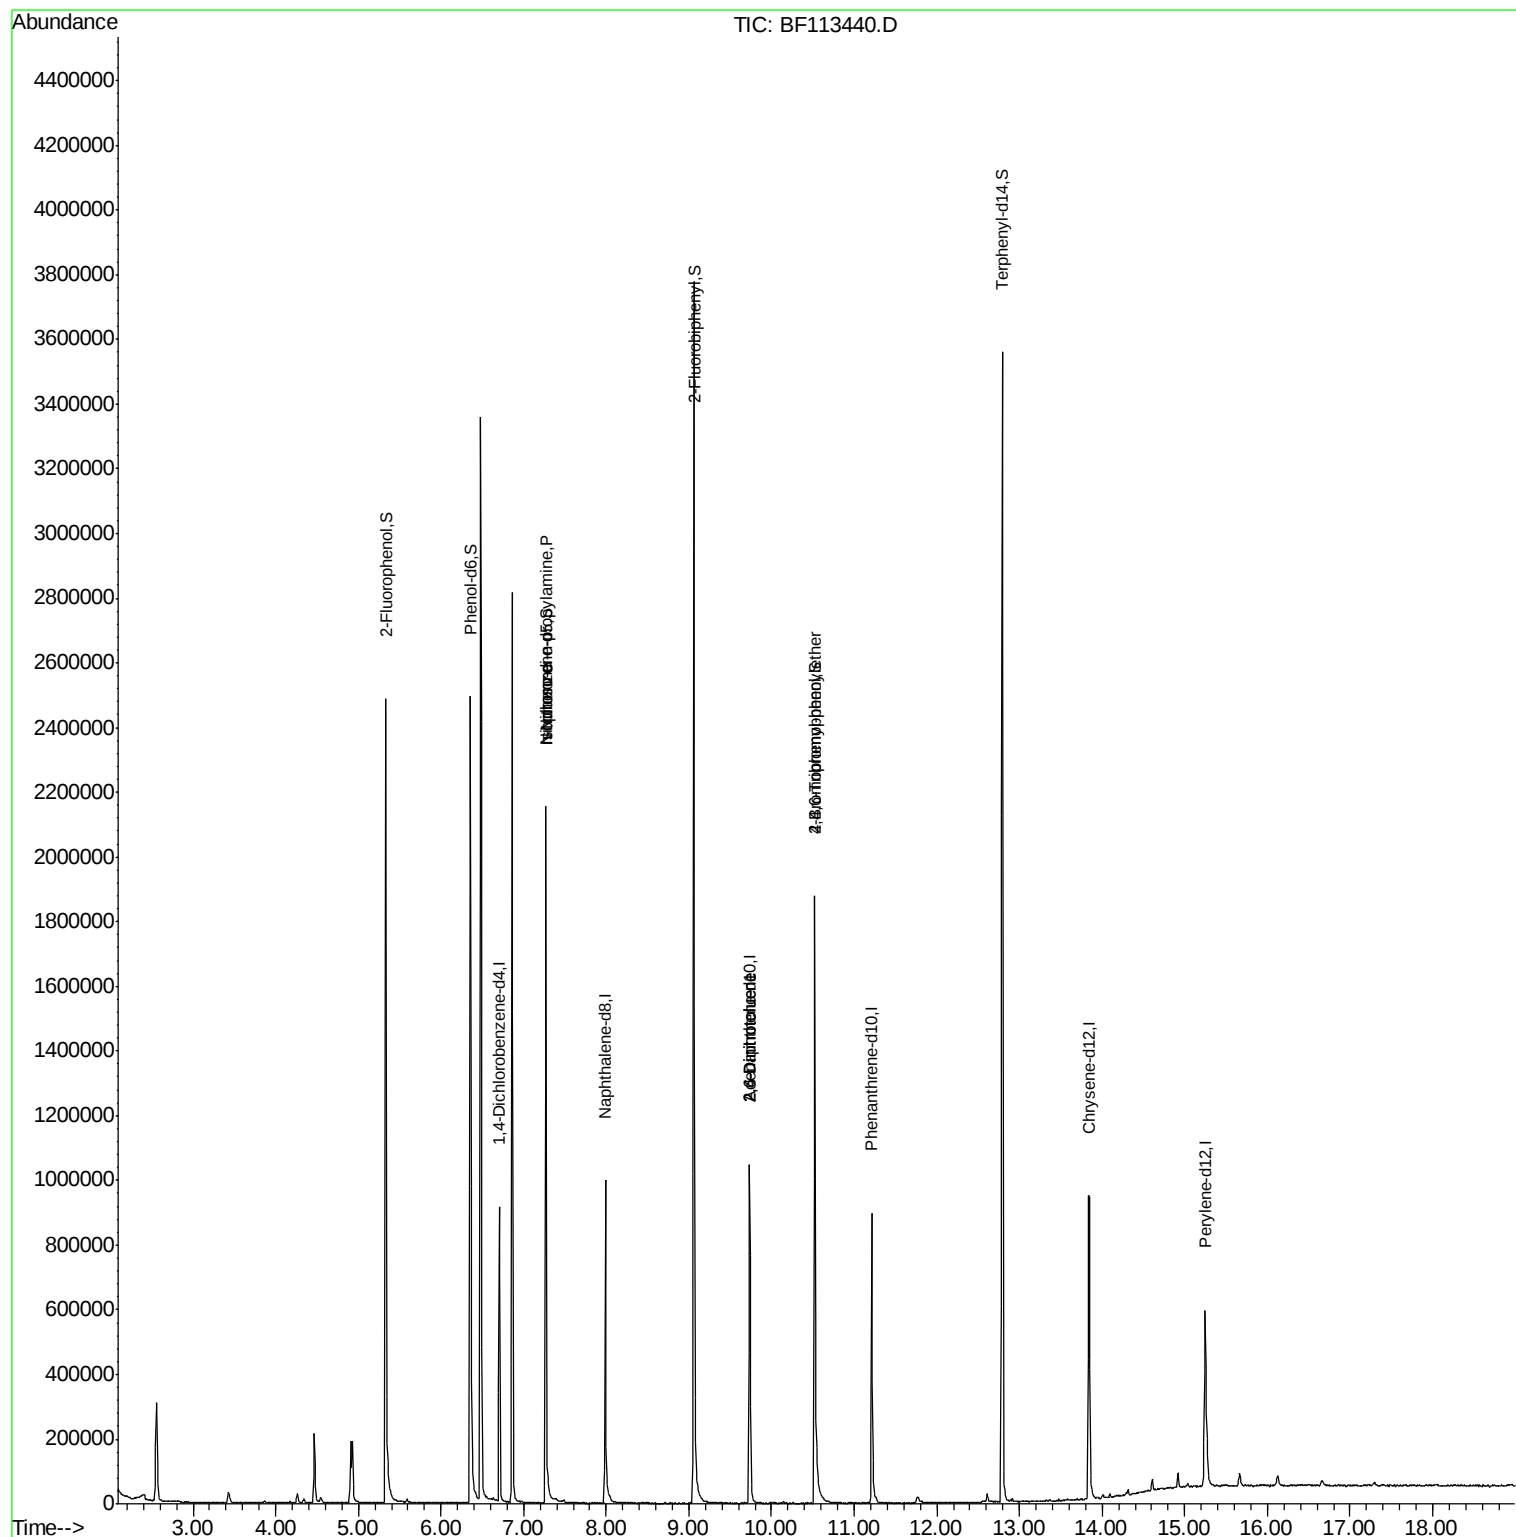

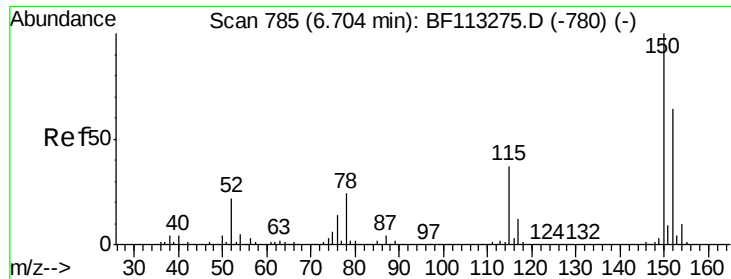

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 6.70 min Scan# 785

Delta R.T. 0.00 min

Lab File: BF113440.D

Acq: 30 Mar 2019 4:59

Instrument :

BNA_F

ClientSampleId :

S6A(2-10)COMP


Tgt Ion:152 Resp: 141283

Ion Ratio Lower Upper

152 100

150 154.5 124.7 187.1




115 58.3 46.0 69.0

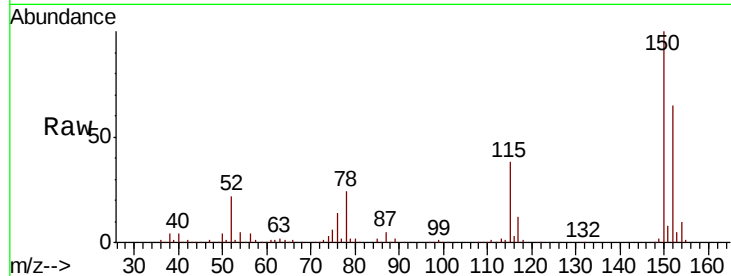

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

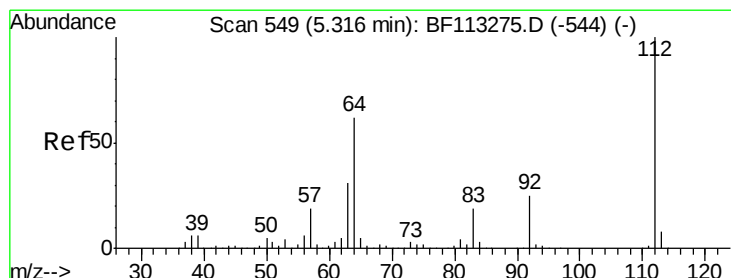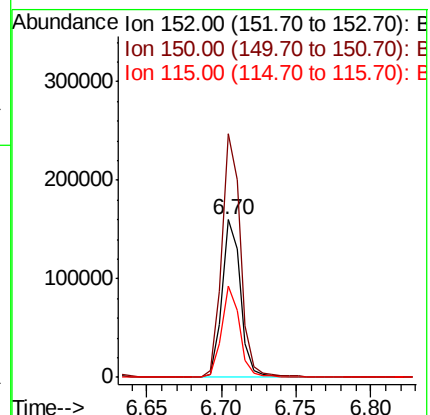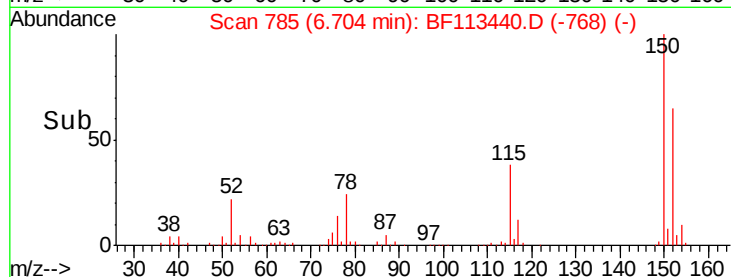

#5

2-Fluorophenol

Concen: 98.613 ng

RT: 5.33 min Scan# 552

Delta R.T. 0.02 min

Lab File: BF113440.D

Acq: 30 Mar 2019 4:59


Tgt Ion:112 Resp: 852066

Ion Ratio Lower Upper

112 100

64 56.1 49.2 73.8



63 28.5 24.9 37.3

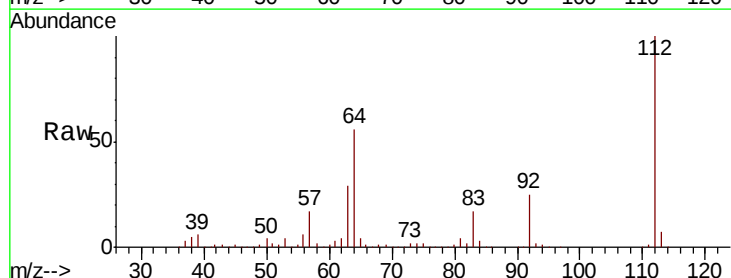

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

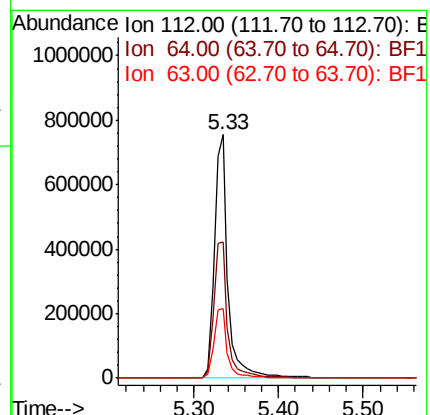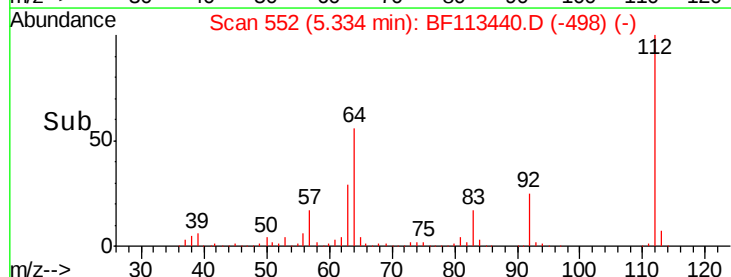



#7

Phenol-d6

Concen: 90.564 ng

RT: 6.36 min Scan# 726

Delta R.T. 0.00 min

Lab File: BF113440.D

Acq: 30 Mar 2019 4:59

Instrument :

BNA_F

ClientSampleId :

S6A(2-10)COMP





Tgt Ion: 99 Resp: 989932

Ion Ratio Lower Upper

99 100

42 17.3 14.8 22.2

71 30.3 24.9 37.3

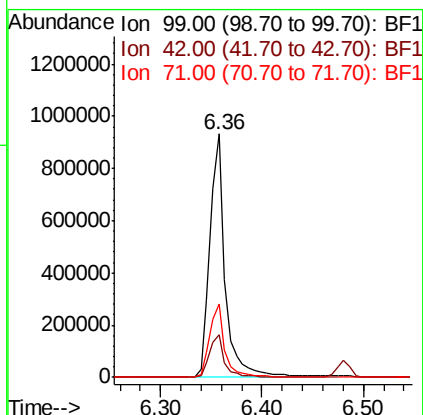

#19

n-Nitroso-di-n-propylamine

Concen: 13.385 ng

RT: 7.27 min Scan# 881

Delta R.T. 0.14 min

Lab File: BF113440.D

Acq: 30 Mar 2019 4:59

Tgt Ion: 70 Resp: 91899




Ion Ratio Lower Upper


70 100

42 47.5 48.4 72.6#

101 0.0 7.8 11.8#

130 2.2 18.2 27.4#

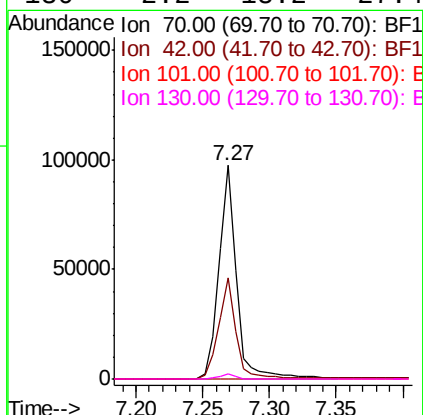







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 7.99 min Scan# 1003
Delta R.T. 0.00 min
Lab File: BF113440.D
Acq: 30 Mar 2019 4:59

Instrument :
BNA_F
ClientSampleId :
S6A(2-10)COMP

Tgt Ion:	136	Resp:	520341
Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.9	13.3
54	8.1	7.0	10.6
68	6.2	4.8	7.2




Abundance Ion 136.00 (135.70 to 136.70): E
800000
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

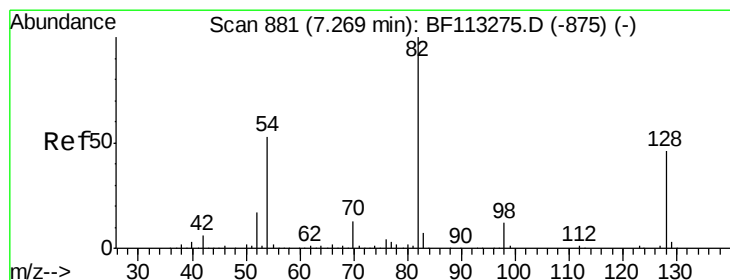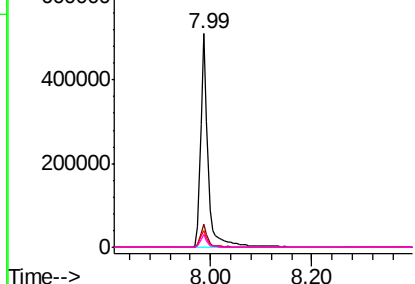




#23
Nitrobenzene-d5
Concen: 81.288 ng
RT: 7.27 min Scan# 881
Delta R.T. 0.00 min
Lab File: BF113440.D
Acq: 30 Mar 2019 4:59

Tgt Ion:	82	Resp:	712627
Ion	Ratio	Lower	Upper
82	100		
128	46.4	36.5	54.7
54	51.4	42.2	63.2



Abundance Ion 82.00 (81.70 to 82.70): BF1
1000000
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

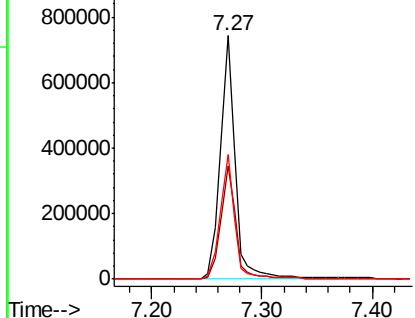

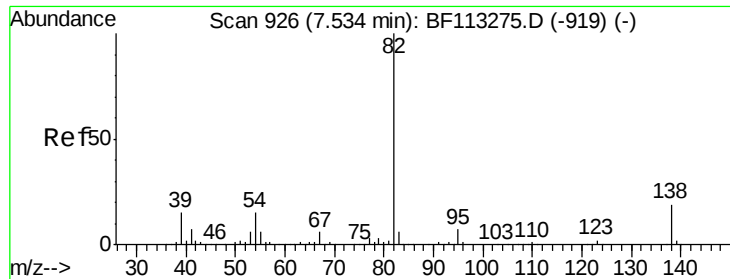

#25

Isophorone

Concen: 41.760 ng

RT: 7.27 min Scan# 881

Delta R.T. -0.26 min

Lab File: BF113440.D

Acq: 30 Mar 2019 4:59

Instrument :

BNA_F

ClientSampleId :

S6A(2-10)COMP


Tgt Ion: 82 Resp: 709481

Ion Ratio Lower Upper

82 100

95 0.0 5.5 8.3#




138 0.0 15.2 22.8#

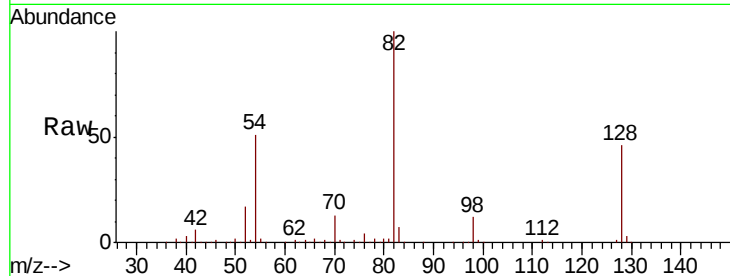

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

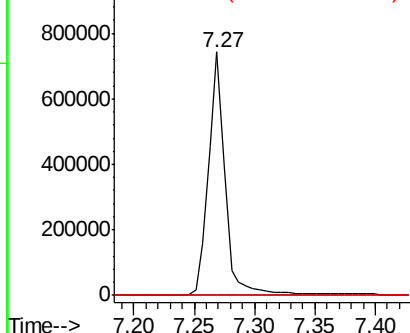

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.73 min Scan# 1300

Delta R.T. -0.01 min

Lab File: BF113440.D

Acq: 30 Mar 2019 4:59


Tgt Ion: 164 Resp: 230140

Ion Ratio Lower Upper

164 100

162 99.2 81.8 122.6



160 43.8 36.4 54.6




Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

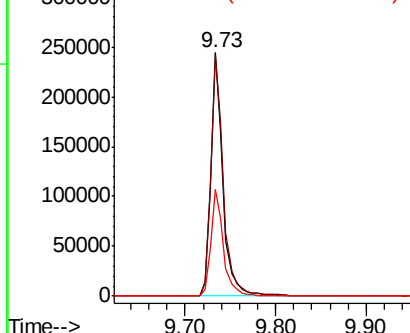



#42

2,4,6-Tribromophenol

Concen: 115.430 ng

RT: 10.52 min Scan# 1434

Delta R.T. -0.01 min

Lab File: BF113440.D

Acq: 30 Mar 2019 4:59

Instrument :

BNA_F

ClientSampleId :

S6A(2-10)COMP


Tgt Ion:330 Resp: 328139

Ion Ratio Lower Upper

330 100

332 94.9 77.8 116.6




141 26.7 22.7 34.1

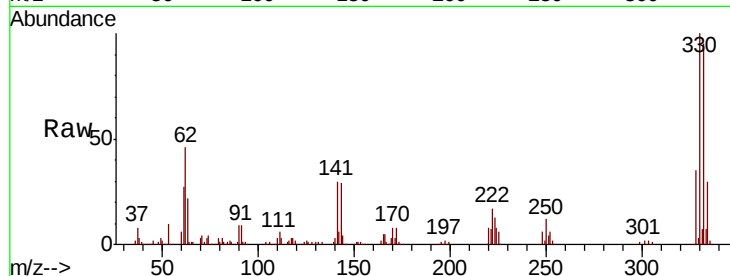

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

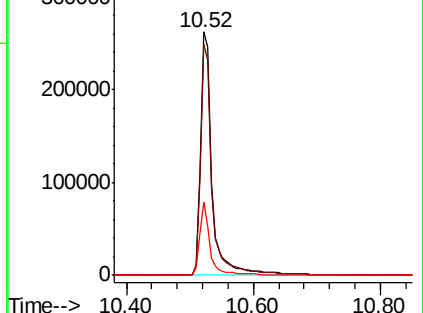

#45

2-Fluorobiphenyl

Concen: 92.239 ng

RT: 9.06 min Scan# 1186

Delta R.T. 0.00 min

Lab File: BF113440.D

Acq: 30 Mar 2019 4:59


Tgt Ion:172 Resp: 1332323

Ion Ratio Lower Upper

172 100

171 35.9 29.0 43.6



170 24.1 19.5 29.3




Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

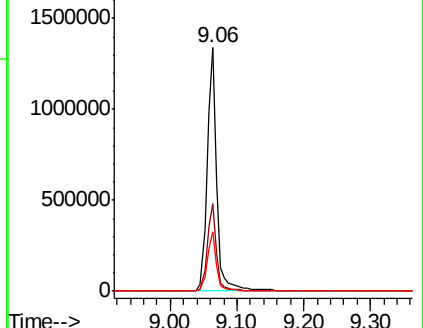



#51

2,6-Dinitrotoluene

Concen: 7.462 ng

RT: 9.73 min Scan# 1300

Delta R.T. 0.21 min

Lab File: BF113440.D

Acq: 30 Mar 2019 4:59

Instrument :

BNA_F

ClientSampleId :

S6A(2-10)COMP


Tgt Ion:165 Resp: 28710

Ion Ratio Lower Upper

165 100

63 0.0 43.4 65.0#




89 1.3 43.1 64.7#

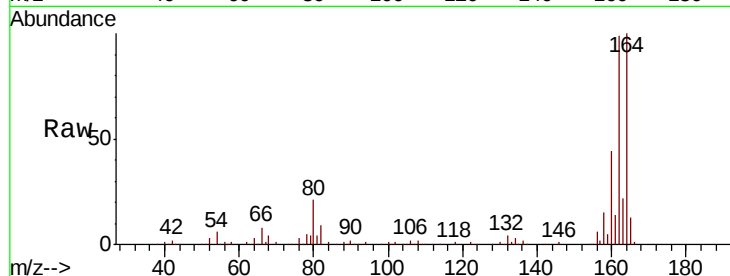

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

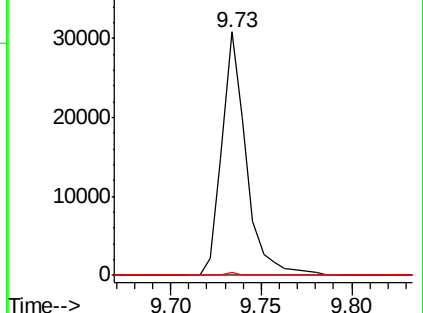

#57

2,4-Dinitrotoluene

Concen: 5.868 ng

RT: 9.73 min Scan# 1300

Delta R.T. -0.20 min

Lab File: BF113440.D

Acq: 30 Mar 2019 4:59

Tgt Ion:165 Resp: 28710


Ion Ratio Lower Upper

165 100

63 0.0 37.5 56.3#

89 1.3 57.4 86.2#

182 0.0 2.0 3.0#






Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

Ion 182.00 (181.70 to 182.70): E

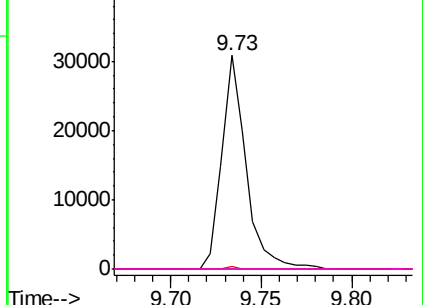

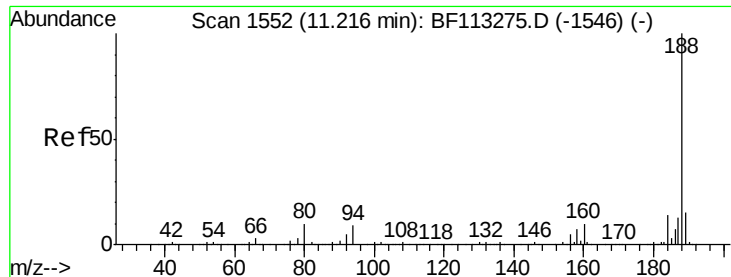

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.22 min Scan# 1552

Delta R.T. 0.00 min

Lab File: BF113440.D

Acq: 30 Mar 2019 4:59

Instrument :

BNA_F

ClientSampleId :

S6A(2-10)COMP


Tgt Ion:188 Resp: 403580

Ion Ratio Lower Upper

188 100

94 8.9 7.0 10.6




80 9.0 7.7 11.5

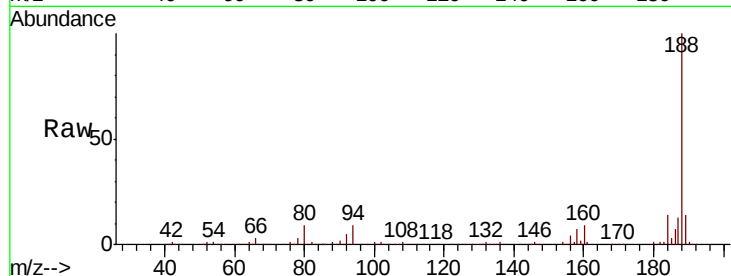

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

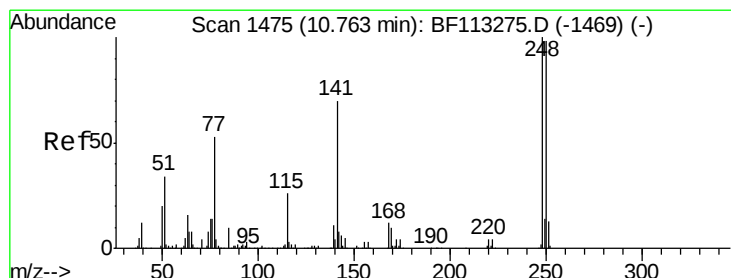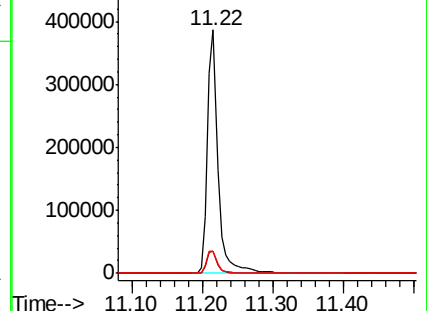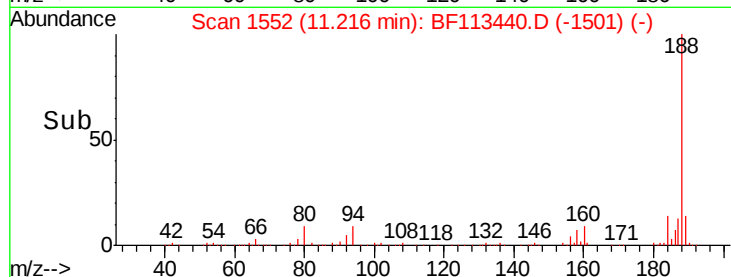

#67

4-Bromophenyl-phenylether

Concen: 3.898 ng

RT: 10.52 min Scan# 1434

Delta R.T. -0.24 min

Lab File: BF113440.D

Acq: 30 Mar 2019 4:59


Tgt Ion:248 Resp: 17144

Ion Ratio Lower Upper

248 100

250 202.4 78.3 117.5#



141 505.4 56.2 84.4#

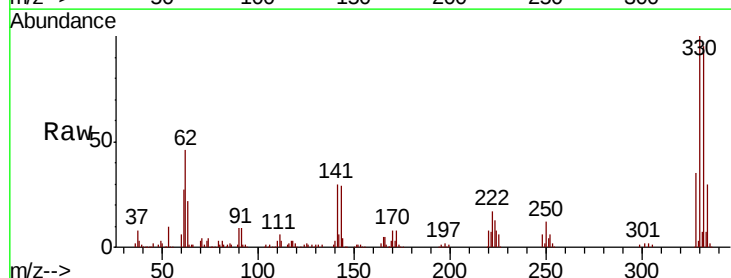


Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

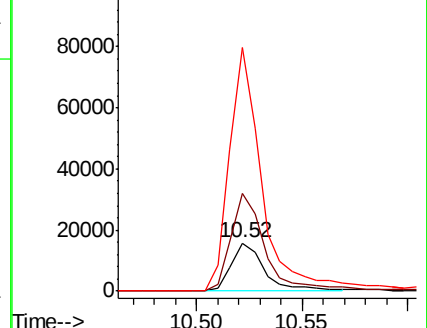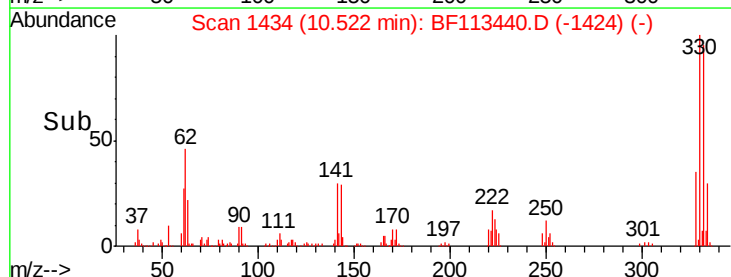



#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.85 min Scan# 1999

Delta R.T. 0.00 min

Lab File: BF113440.D

Acq: 30 Mar 2019 4:59

Instrument :

BNA_F

ClientSampleId :

S6A(2-10)COMP


Tgt Ion:240 Resp: 421920

Ion Ratio Lower Upper

240 100

120 10.2 8.8 13.2




236 25.3 20.9 31.3



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

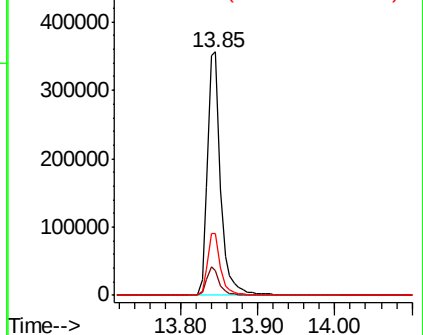

#79

Terphenyl-d14

Concen: 69.173 ng

RT: 12.79 min Scan# 1820

Delta R.T. -0.00 min

Lab File: BF113440.D

Acq: 30 Mar 2019 4:59


Tgt Ion:244 Resp: 1324113

Ion Ratio Lower Upper

244 100

212 6.7 5.5 8.3



122 11.3 8.6 13.0




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

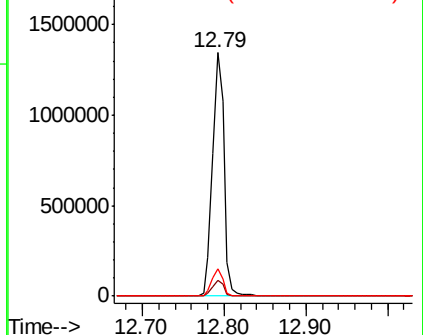


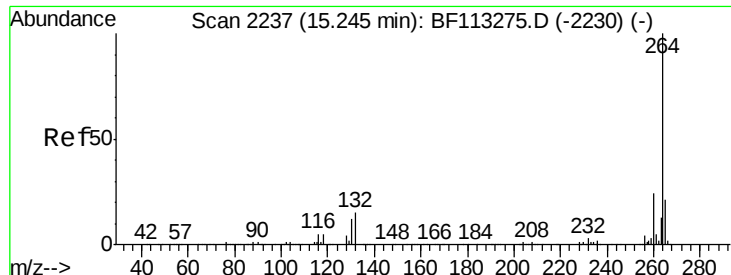

#87
Perylene-d12
Concen: 20.000 ng
RT: 15.24 min Scan# 2237
Delta R.T. 0.00 min
Lab File: BF113440.D
Acq: 30 Mar 2019 4:59

Instrument :
BNA_F
ClientSampleId :
S6A(2-10)COMP

Tgt Ion: 264 Resp: 326362
Ion Ratio Lower Upper
264 100
260 22.9 19.1 28.7
265 21.9 17.1 25.7

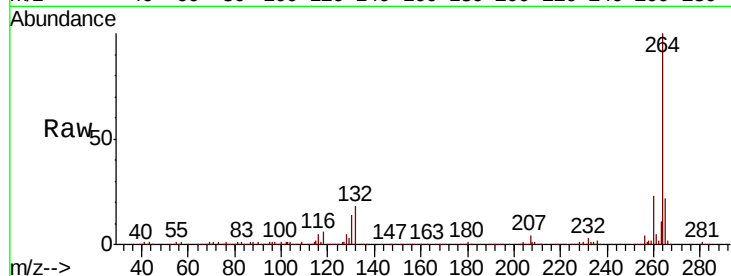

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

