

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032919\
 Data File : BF113457.D
 Acq On : 30 Mar 2019 13:01
 Operator : JU/SJ
 Sample : PB118325TB
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB118325TB

Quant Time: Apr 01 04:14:39 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 26 03:32:08 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.70	152	113938	20.00	ng	0.00
21) Naphthalene-d8	7.99	136	425201	20.00	ng	0.00
39) Acenaphthene-d10	9.74	164	198787	20.00	ng	0.00
64) Phenanthrene-d10	11.22	188	380573	20.00	ng	0.00
76) Chrysene-d12	13.84	240	388564	20.00	ng	0.00
87) Perylene-d12	15.25	264	280265	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.32	112	640378	91.90	ng	0.00
7) Phenol-d6	6.35	99	848674	96.27	ng	0.00
23) Nitrobenzene-d5	7.27	82	501800	70.05	ng	0.00
42) 2,4,6-Tribromophenol	10.53	330	218371	88.93	ng	0.00
45) 2-Fluorobiphenyl	9.06	172	987372	75.98	ng	0.00
79) Terphenyl-d14	12.80	244	1108957	62.91	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.27	70	61110	11.036	ng	# 78
25) Isophorone	7.27	82	501797	36.144	ng	# 64
50) Dimethylphthalate	9.46	163	69166	4.695	ng	# 99
51) 2,6-Dinitrotoluene	9.73	165	24720	7.438	ng	# 26
57) 2,4-Dinitrotoluene	9.73	165	24720	5.849	ng	# 23
67) 4-Bromophenyl-phenylether	10.52	248	11952	2.881	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032919\
Data File : BF113457.D
Acq On : 30 Mar 2019 13:01
Operator : JU/SJ
Sample : PB118325TB
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB118325TB

Quant Time: Apr 01 04:14:39 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 26 03:32:08 2019
Response via : Initial Calibration

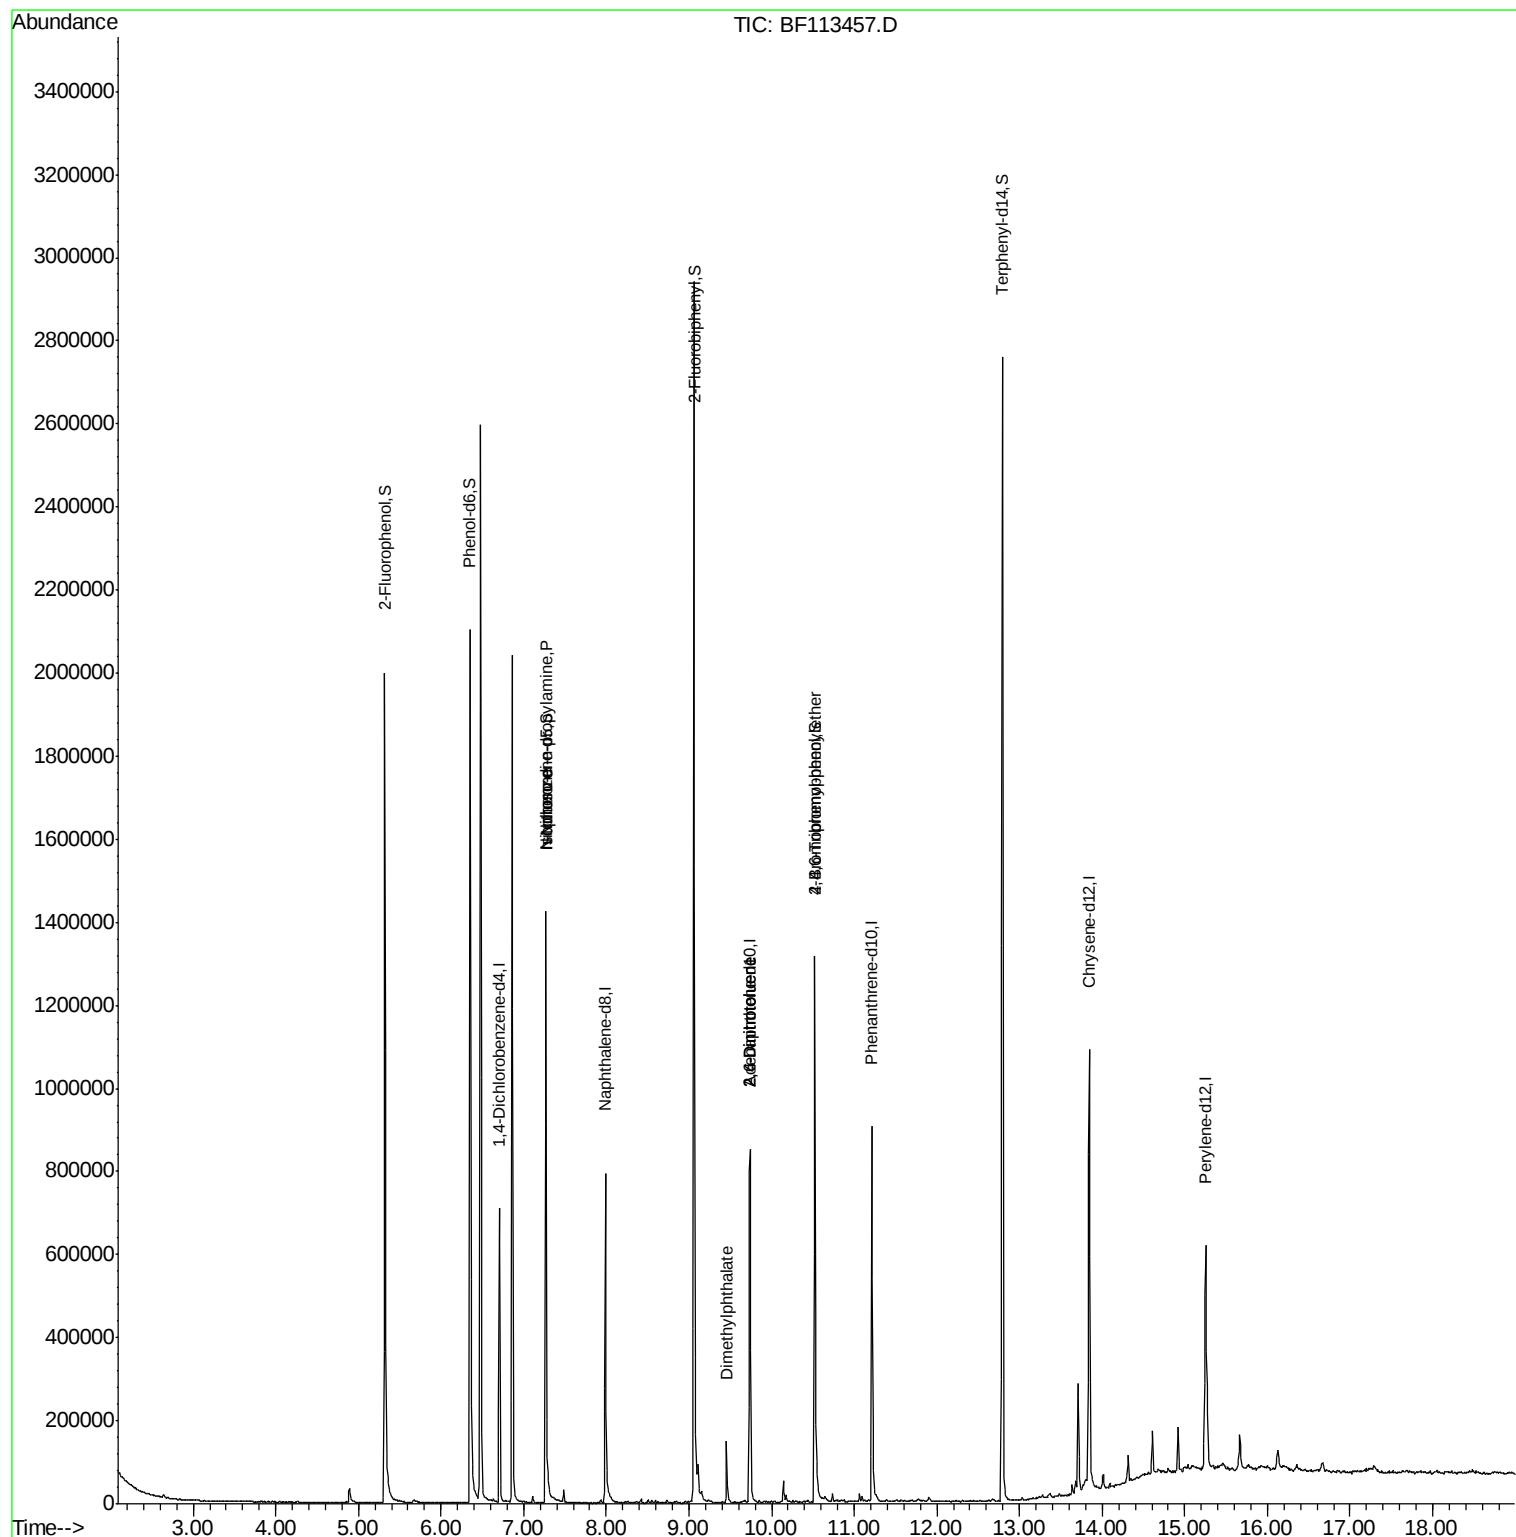




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.70 min Scan# 785
Delta R.T. -0.00 min
Lab File: BF113457.D
Acq: 30 Mar 2019 13:01

Instrument :
BNA_F
ClientSampleId :
PB118325TB

Tgt Ion:152 Resp: 113938
Ion Ratio Lower Upper
152 100
150 159.0 124.7 187.1
115 60.7 46.0 69.0

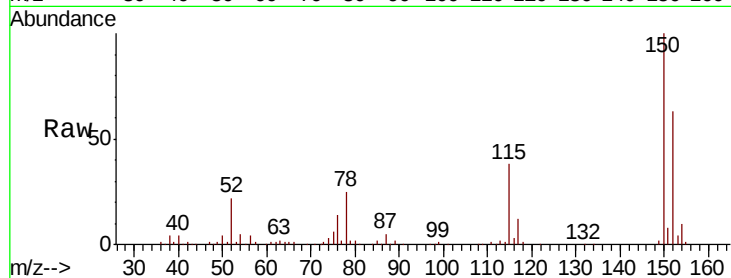


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

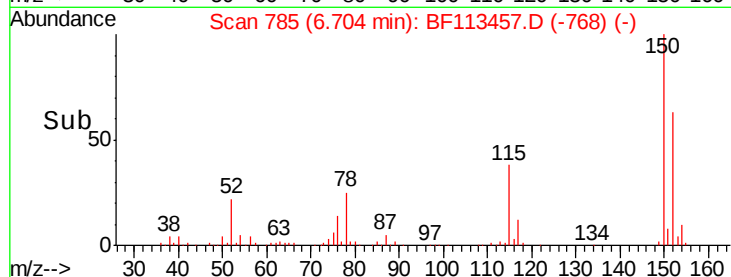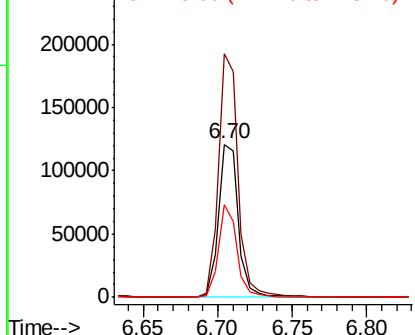



#5


2-Fluorophenol
Concen: 91.900 ng
RT: 5.32 min Scan# 550
Delta R.T. 0.01 min
Lab File: BF113457.D
Acq: 30 Mar 2019 13:01

Tgt Ion:112 Resp: 640378
Ion Ratio Lower Upper
112 100
64 57.4 49.2 73.8
63 29.3 24.9 37.3

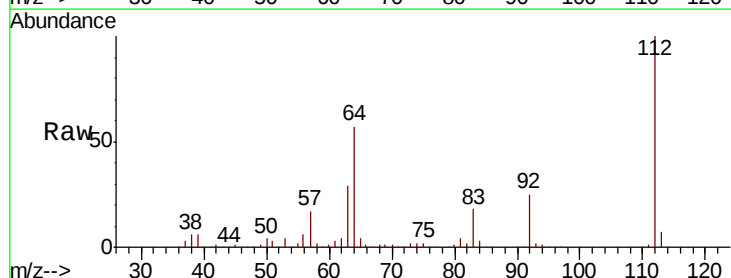

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

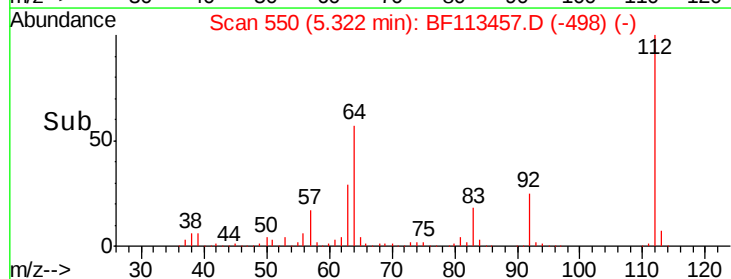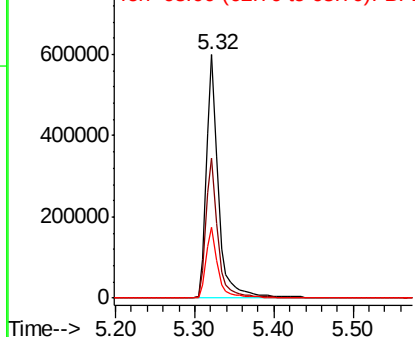

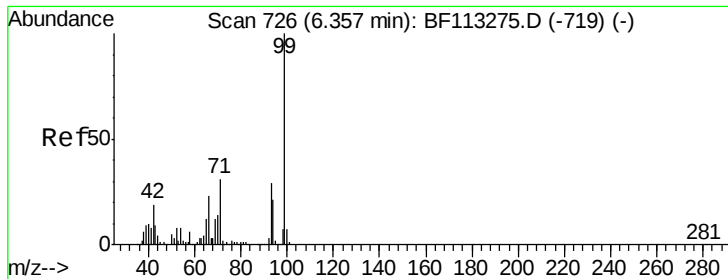

#7

Phenol-d6

Concen: 96.275 ng

RT: 6.35 min Scan# 725

Delta R.T. -0.01 min

Lab File: BF113457.D

Acq: 30 Mar 2019 13:01

Instrument :

BNA_F

ClientSampleId :

PB118325TB


Tgt Ion: 99 Resp: 848674

Ion Ratio Lower Upper

99 100

42 18.0 14.8 22.2

71 31.1 24.9 37.3



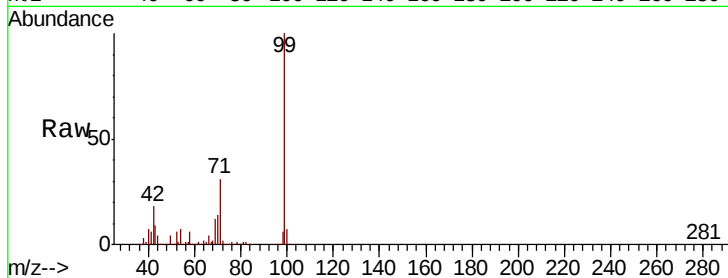


Abundance

Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

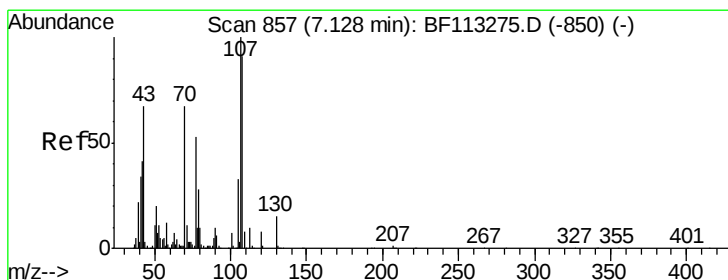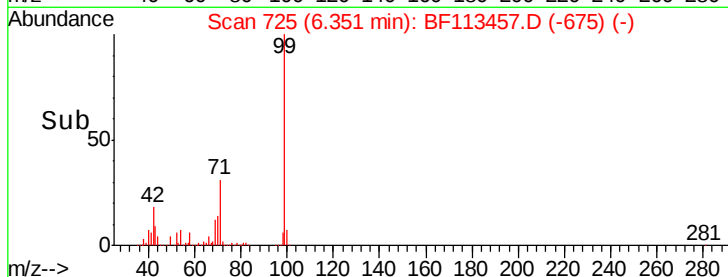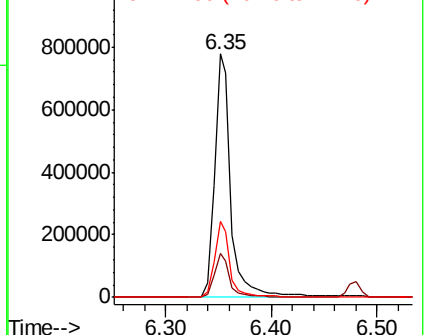

#19

n-Nitroso-di-n-propylamine

Concen: 11.036 ng

RT: 7.27 min Scan# 881

Delta R.T. 0.14 min

Lab File: BF113457.D

Acq: 30 Mar 2019 13:01

Tgt Ion: 70 Resp: 61110


Ion Ratio Lower Upper

70 100

42 49.6 48.4 72.6

101 0.0 7.8 11.8#

130 2.5 18.2 27.4#

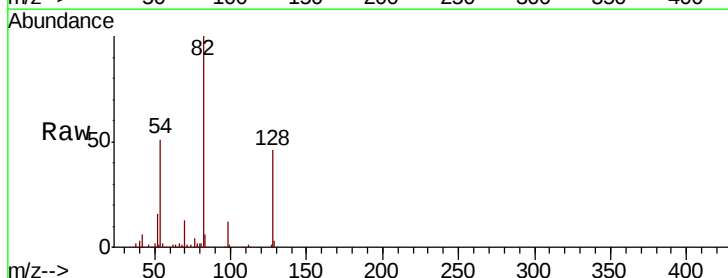



Abundance

Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): BF1

Ion 130.00 (129.70 to 130.70): BF1

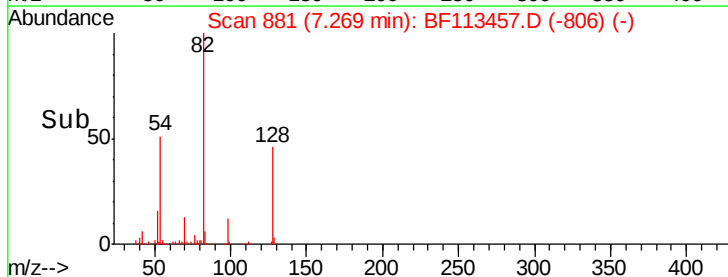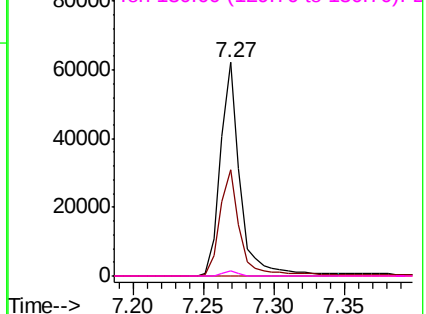







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 7.99 min Scan# 1003
Delta R.T. -0.00 min
Lab File: BF113457.D
Acq: 30 Mar 2019 13:01

Instrument :
BNA_F
ClientSampleId :
PB118325TB

Tgt Ion:	136	Resp:	425201
Ion	Ratio	Lower	Upper
136	100		
137	10.9	8.9	13.3
54	8.4	7.0	10.6
68	6.2	4.8	7.2

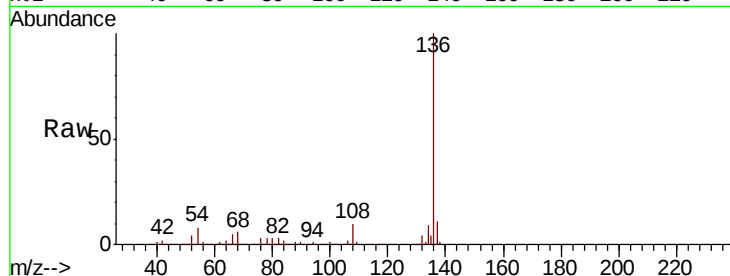


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

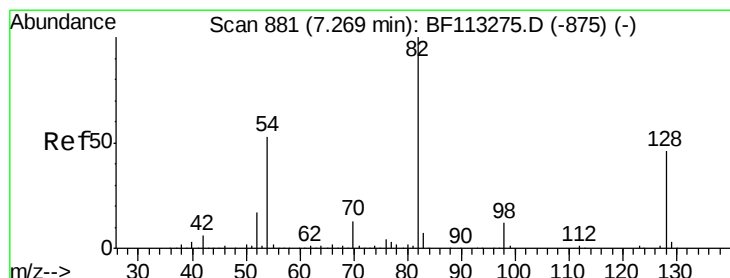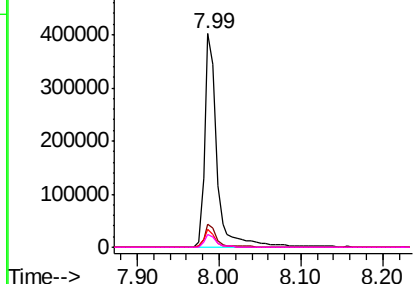
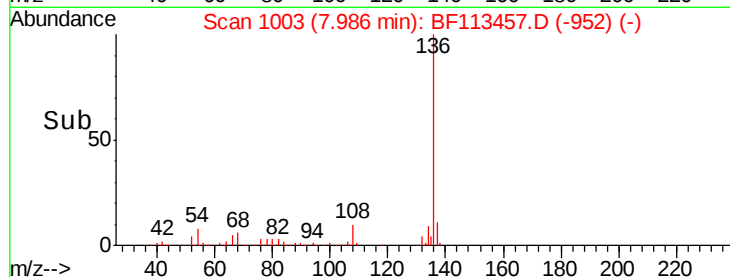



#23
Nitrobenzene-d5
Concen: 70.047 ng
RT: 7.27 min Scan# 881
Delta R.T. 0.00 min
Lab File: BF113457.D
Acq: 30 Mar 2019 13:01

Tgt Ion:	82	Resp:	501800
Ion	Ratio	Lower	Upper
82	100		
128	46.0	36.5	54.7
54	51.2	42.2	63.2

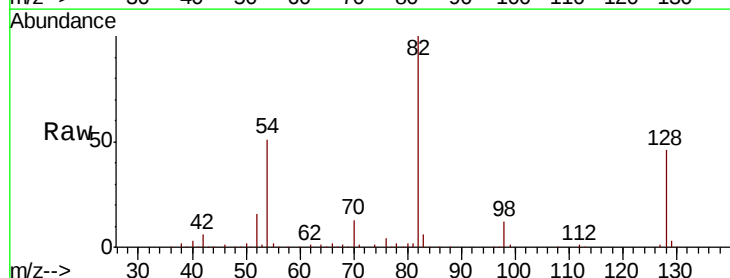

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

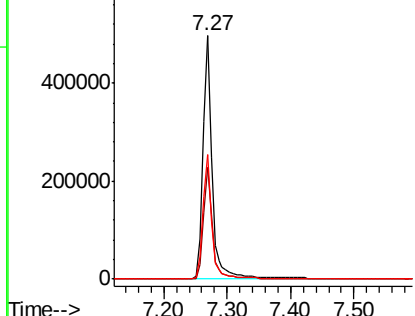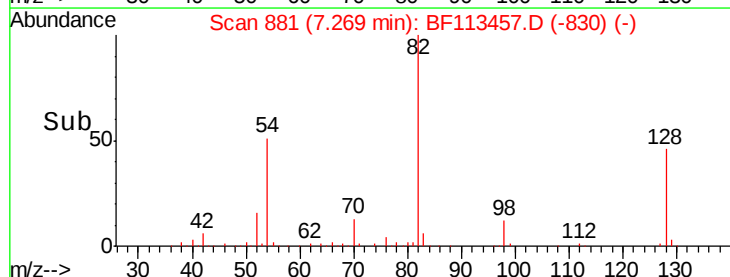

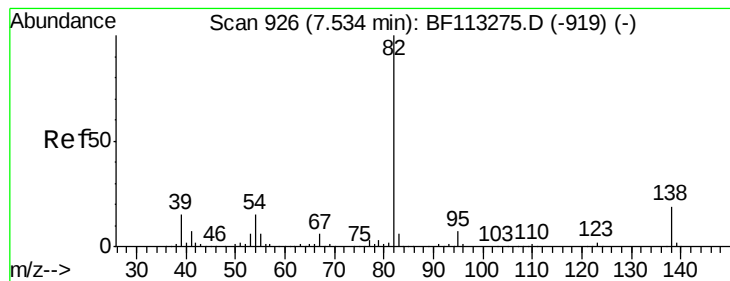

#25

Isophorone

Concen: 36.144 ng

RT: 7.27 min Scan# 881

Delta R.T. -0.26 min

Lab File: BF113457.D

Acq: 30 Mar 2019 13:01

Instrument :

BNA_F

ClientSampleId :

PB118325TB


Tgt Ion: 82 Resp: 501797

Ion Ratio Lower Upper

82 100

95 0.0 5.5 8.3#




138 0.0 15.2 22.8#

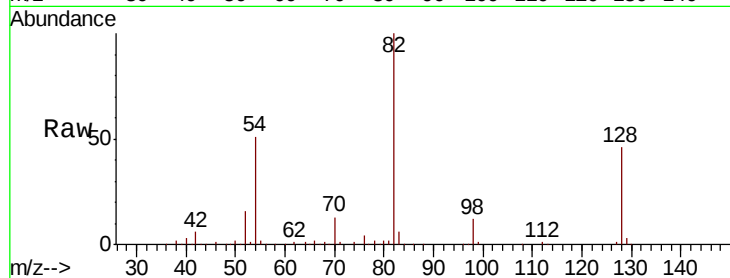

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

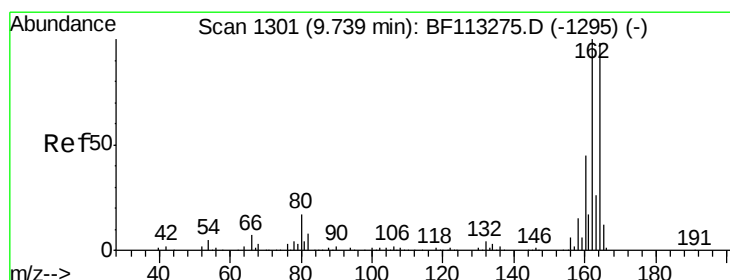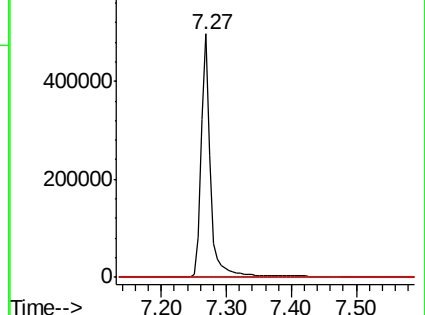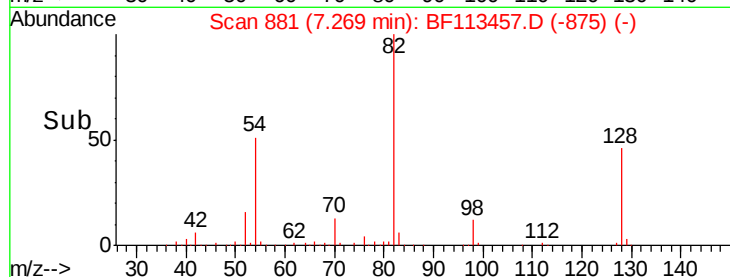

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.74 min Scan# 1301

Delta R.T. -0.00 min

Lab File: BF113457.D

Acq: 30 Mar 2019 13:01


Tgt Ion: 164 Resp: 198787

Ion Ratio Lower Upper

164 100

162 100.4 81.8 122.6



160 44.8 36.4 54.6

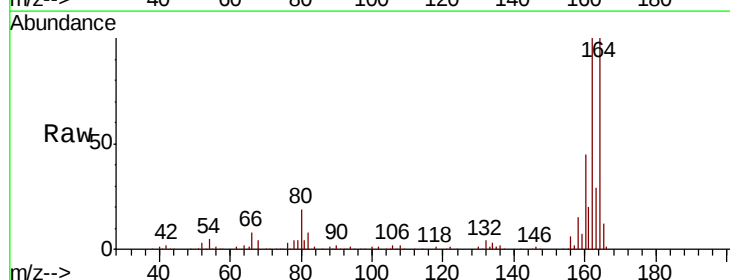


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

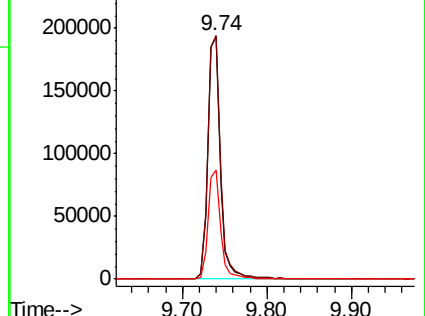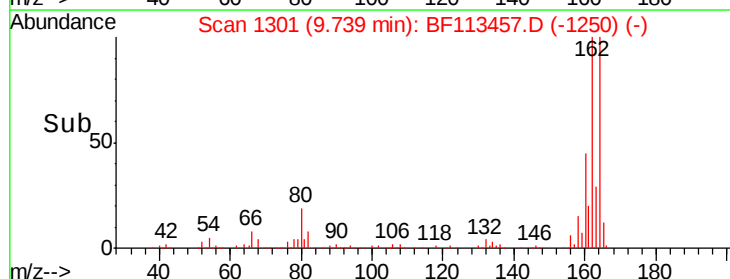


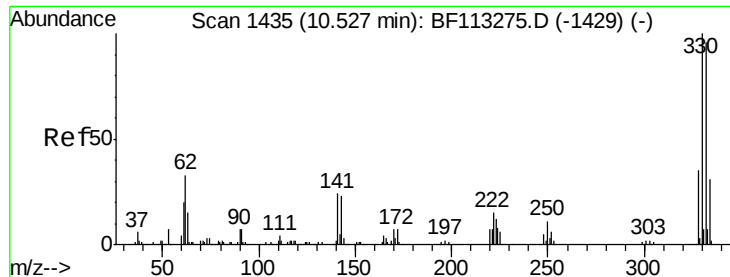



#42
 2,4,6-Tribromophenol
 Concen: 88.932 ng
 RT: 10.53 min Scan# 1435
 Delta R.T. 0.00 min
 Lab File: BF113457.D
 Acq: 30 Mar 2019 13:01

Instrument :
 BNA_F
 ClientSampleId :
 PB118325TB

Tgt Ion:330 Resp: 218371
 Ion Ratio Lower Upper
 330 100
 332 95.4 77.8 116.6
 141 27.1 22.7 34.1

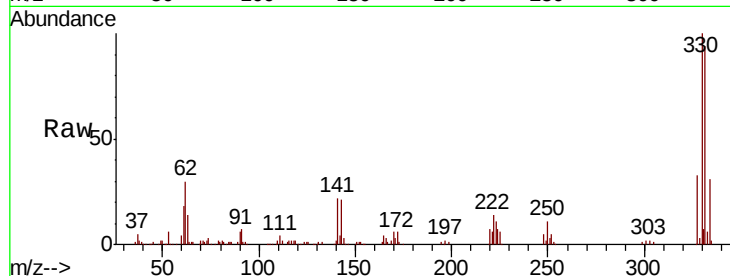


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

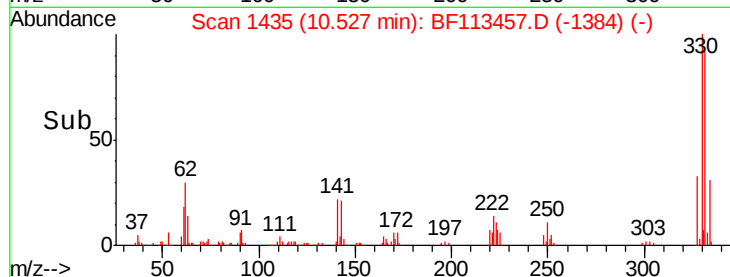
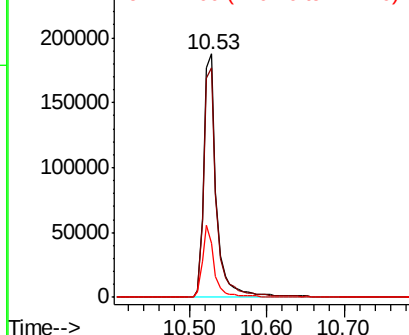



#45
 2-Fluorobiphenyl
 Concen: 75.979 ng
 RT: 9.06 min Scan# 1186
 Delta R.T. 0.00 min
 Lab File: BF113457.D
 Acq: 30 Mar 2019 13:01

Tgt Ion:172 Resp: 987372
 Ion Ratio Lower Upper
 172 100
 171 35.7 29.0 43.6
 170 23.8 19.5 29.3

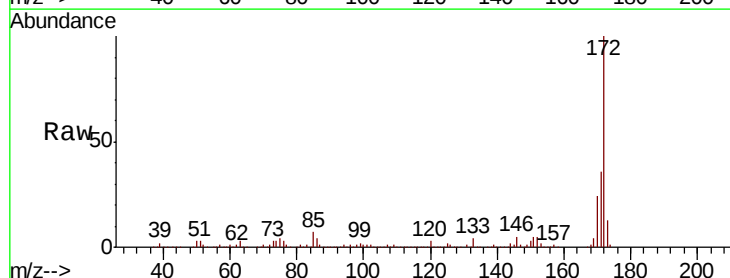

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

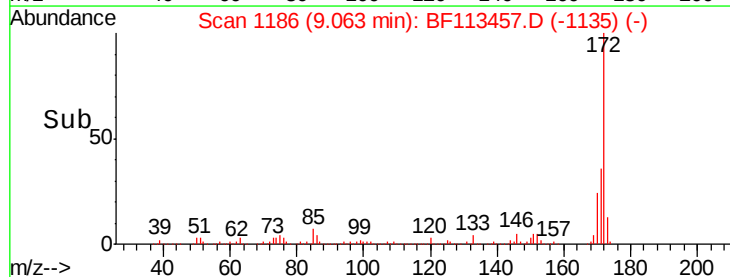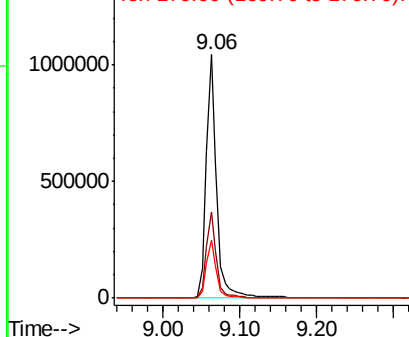

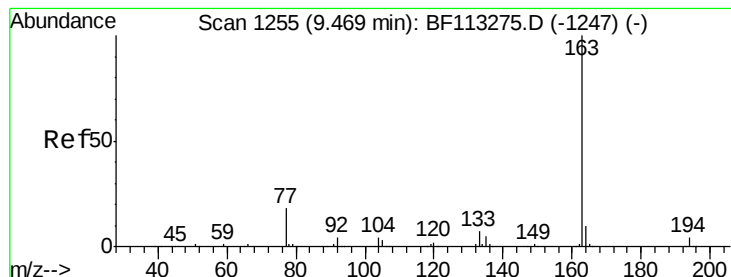

#50

Dimethylphthalate

Concen: 4.695 ng

RT: 9.46 min Scan# 1253

Delta R.T. -0.01 min

Lab File: BF113457.D

Acq: 30 Mar 2019 13:01

Instrument :

BNA_F

ClientSampleId :

PB118325TB


Tgt Ion:163 Resp: 69166

Ion Ratio Lower Upper

163 100

194 4.3 3.0 4.6




164 10.5 8.1 12.1

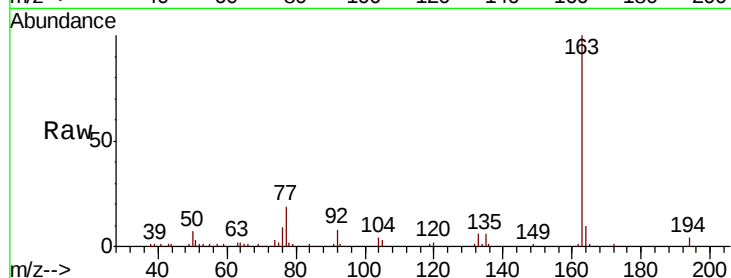

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

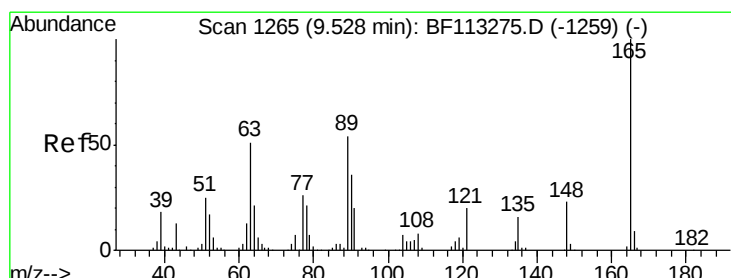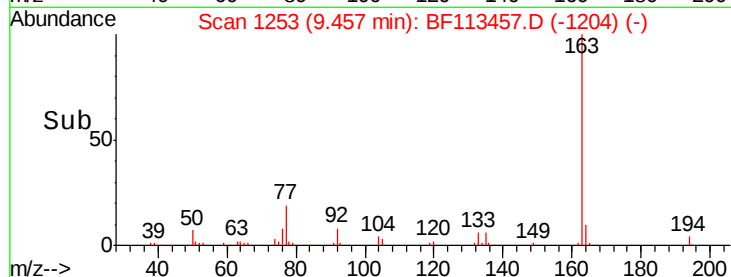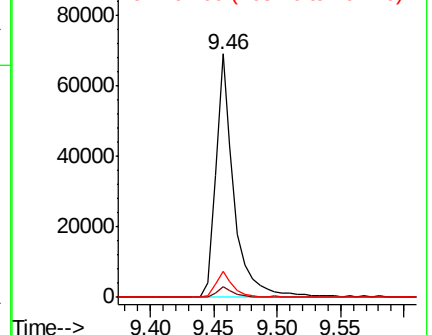

#51

2,6-Dinitrotoluene

Concen: 7.438 ng

RT: 9.73 min Scan# 1300

Delta R.T. 0.21 min

Lab File: BF113457.D

Acq: 30 Mar 2019 13:01


Tgt Ion:165 Resp: 24720

Ion Ratio Lower Upper

165 100

63 1.2 43.4 65.0#



89 1.3 43.1 64.7#

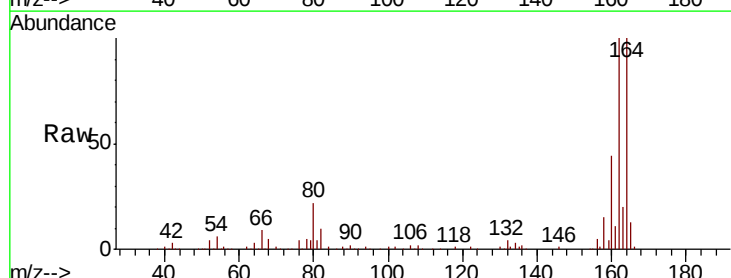


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

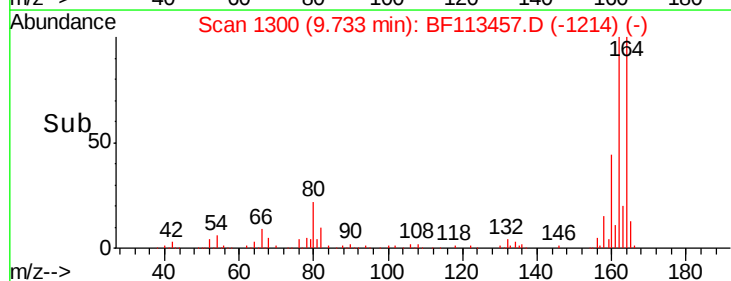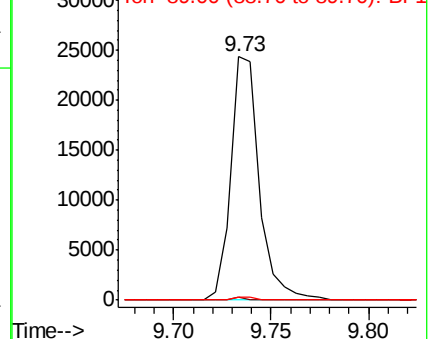


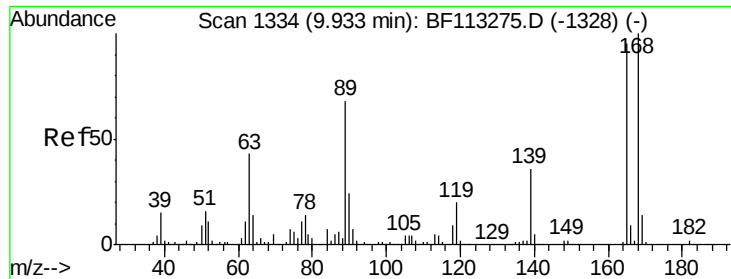




#57
 2,4-Dinitrotoluene
 Concen: 5.849 ng
 RT: 9.73 min Scan# 1300
 Delta R.T. -0.20 min
 Lab File: BF113457.D
 Acq: 30 Mar 2019 13:01

Instrument :
 BNA_F
 ClientSampleId :
 PB118325TB

Tgt Ion:165 Resp: 24720
 Ion Ratio Lower Upper
 165 100
 63 1.2 37.5 56.3#
 89 1.3 57.4 86.2#
 182 0.0 2.0 3.0#

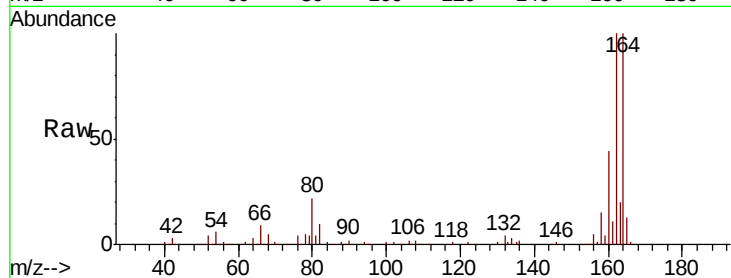


Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF1
 Ion 89.00 (88.70 to 89.70): BF1
 Ion 182.00 (181.70 to 182.70): E

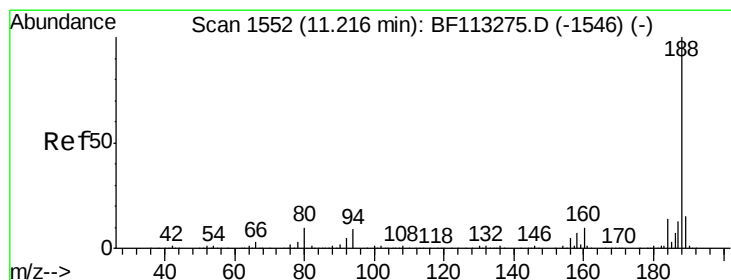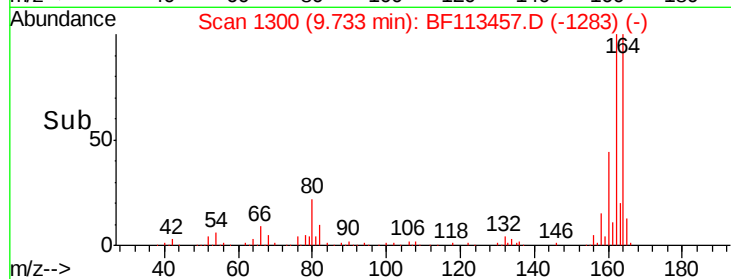
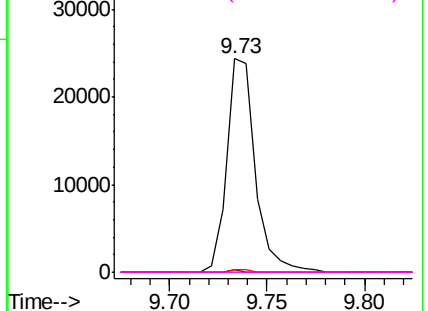



#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.22 min Scan# 1552
 Delta R.T. -0.00 min
 Lab File: BF113457.D
 Acq: 30 Mar 2019 13:01

Tgt Ion:188 Resp: 380573
 Ion Ratio Lower Upper
 188 100
 94 9.6 7.0 10.6
 80 10.1 7.7 11.5

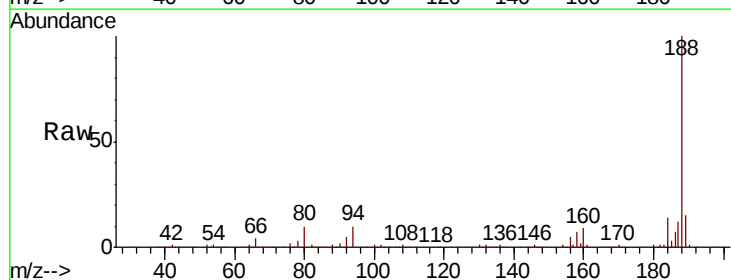

Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF1
 Ion 80.00 (79.70 to 80.70): BF1

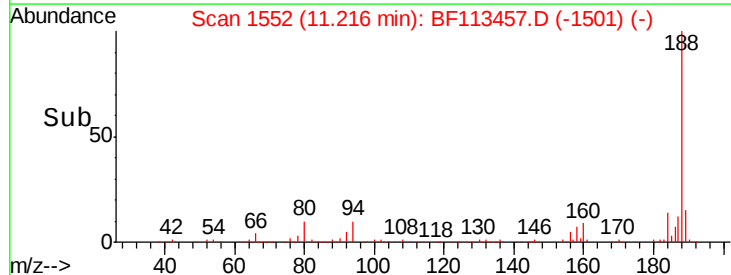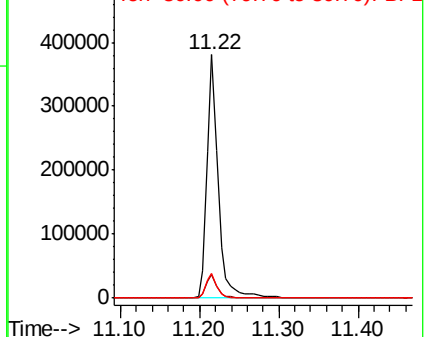


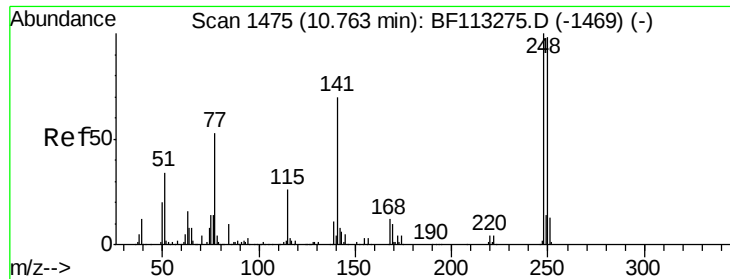




#67
 4-Bromophenyl-phenylether
 Concen: 2.881 ng
 RT: 10.52 min Scan# 1434
 Delta R.T. -0.24 min
 Lab File: BF113457.D
 Acq: 30 Mar 2019 13:01

Instrument :
 BNA_F
 ClientSampleId :
 PB118325TB

Tgt Ion:248 Resp: 11952
 Ion Ratio Lower Upper
 248 100
 250 204.6 78.3 117.5#
 141 511.4 56.2 84.4#

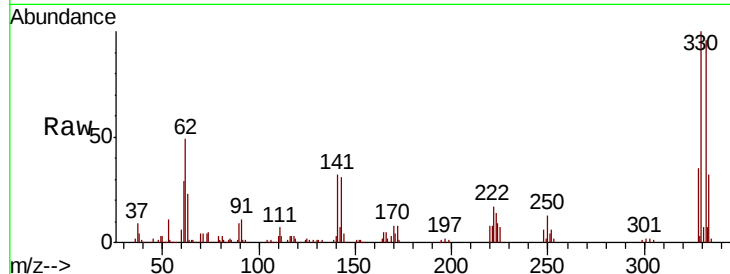


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

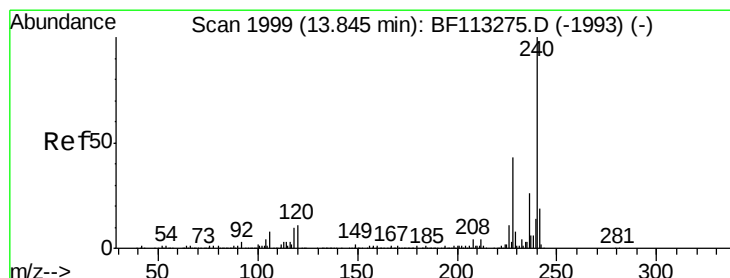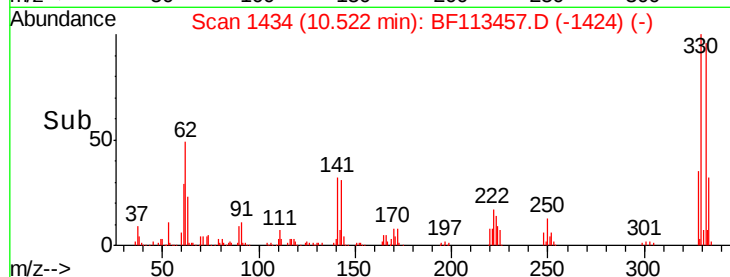
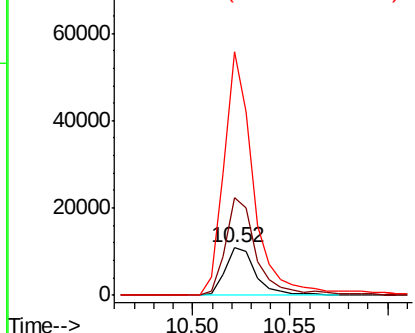



#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 13.84 min Scan# 1999
 Delta R.T. -0.00 min
 Lab File: BF113457.D
 Acq: 30 Mar 2019 13:01

Tgt Ion:240 Resp: 388564
 Ion Ratio Lower Upper
 240 100
 120 11.1 8.8 13.2
 236 26.6 20.9 31.3

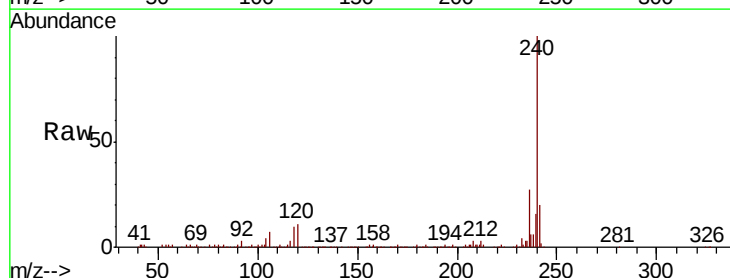

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E



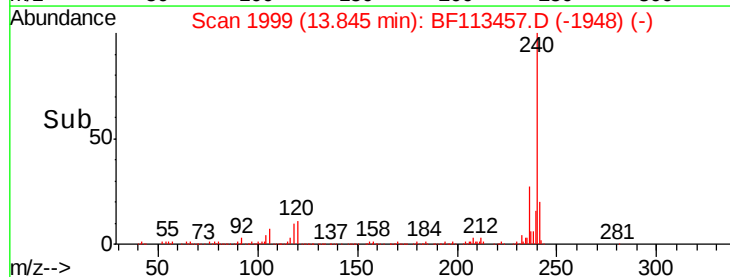
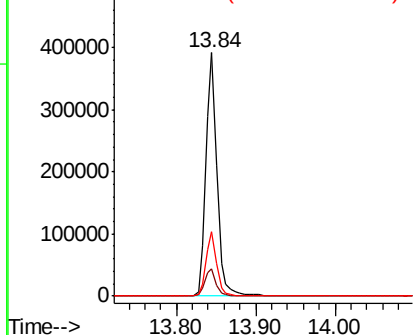


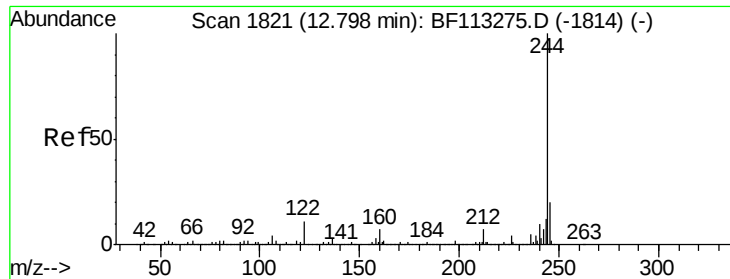

#79
 Terphenyl-d14
 Concen: 62.907 ng
 RT: 12.80 min Scan# 1821
 Delta R.T. 0.00 min
 Lab File: BF113457.D
 Acq: 30 Mar 2019 13:01

Instrument :
 BNA_F
 ClientSampleId :
 PB118325TB

Tgt Ion:244 Resp: 1108957
 Ion Ratio Lower Upper
 244 100
 212 6.3 5.5 8.3
 122 9.5 8.6 13.0

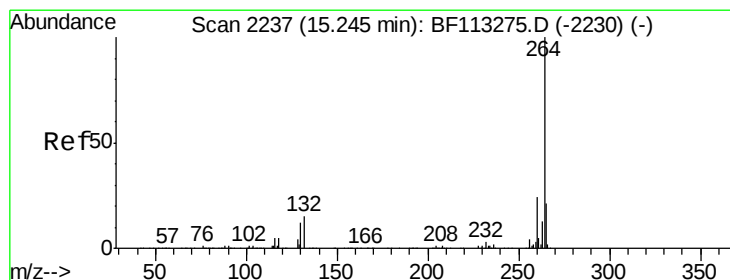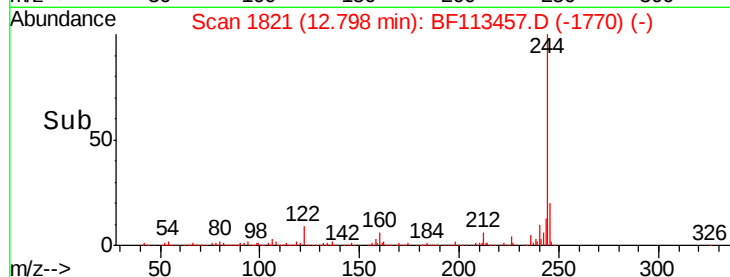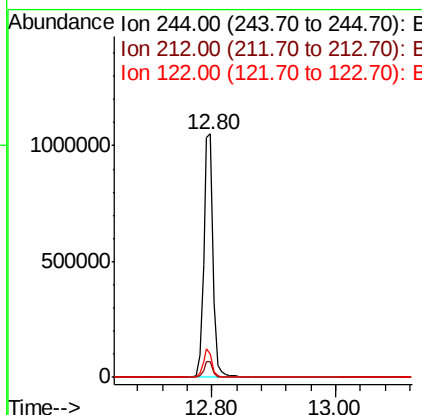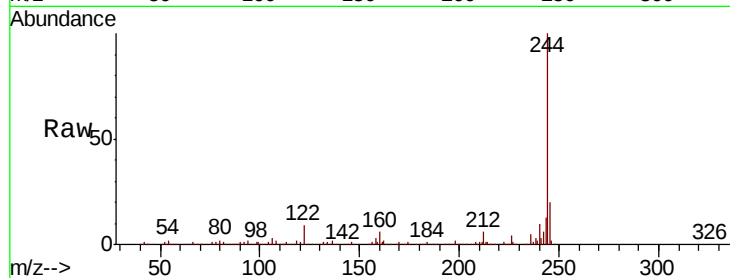

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.25 min Scan# 2238
 Delta R.T. 0.01 min
 Lab File: BF113457.D
 Acq: 30 Mar 2019 13:01

Tgt Ion:264 Resp: 280265
 Ion Ratio Lower Upper
 264 100
 260 23.4 19.1 28.7
 265 21.0 17.1 25.7

