

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032919\
 Data File : BF113456.D
 Acq On : 30 Mar 2019 12:33
 Operator : JU/SJ
 Sample : PB118325BL
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB118325BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.322	546	550	572	rBV	2204753	2383396	78.22%	10.125%
2	6.357	721	726	743	rBV	2277923	2526889	82.93%	10.734%
3	6.481	743	747	762	rVB	2762723	2505368	82.22%	10.643%
4	6.704	782	785	795	rVB	724692	635616	20.86%	2.700%
5	6.863	808	812	829	rBV	2304575	1998447	65.58%	8.489%
6	7.269	877	881	910	rBV	1620018	1543357	50.65%	6.556%
7	7.987	1000	1003	1021	rBV	797446	789897	25.92%	3.355%
8	9.063	1182	1186	1201	rBV	3188313	2911084	95.53%	12.366%
9	9.739	1297	1301	1318	rBV	878918	871487	28.60%	3.702%
10	10.522	1431	1434	1450	rBV	1439837	1601456	52.56%	6.803%
11	11.216	1548	1552	1576	rBV	873352	873269	28.66%	3.710%
12	12.798	1816	1821	1824	rBV	2981497	3047162	100.00%	12.944%
13	13.845	1995	1999	2010	rBV	1012915	1060608	34.81%	4.505%
14	15.251	2233	2238	2249	rVB	536453	792548	26.01%	3.367%


Sum of corrected areas: 23540584

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF032919\
Data File : BF113456.D
Acq On : 30 Mar 2019 12:33
Operator : JU/SJ
Sample : PB118325BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB118325BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF032519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

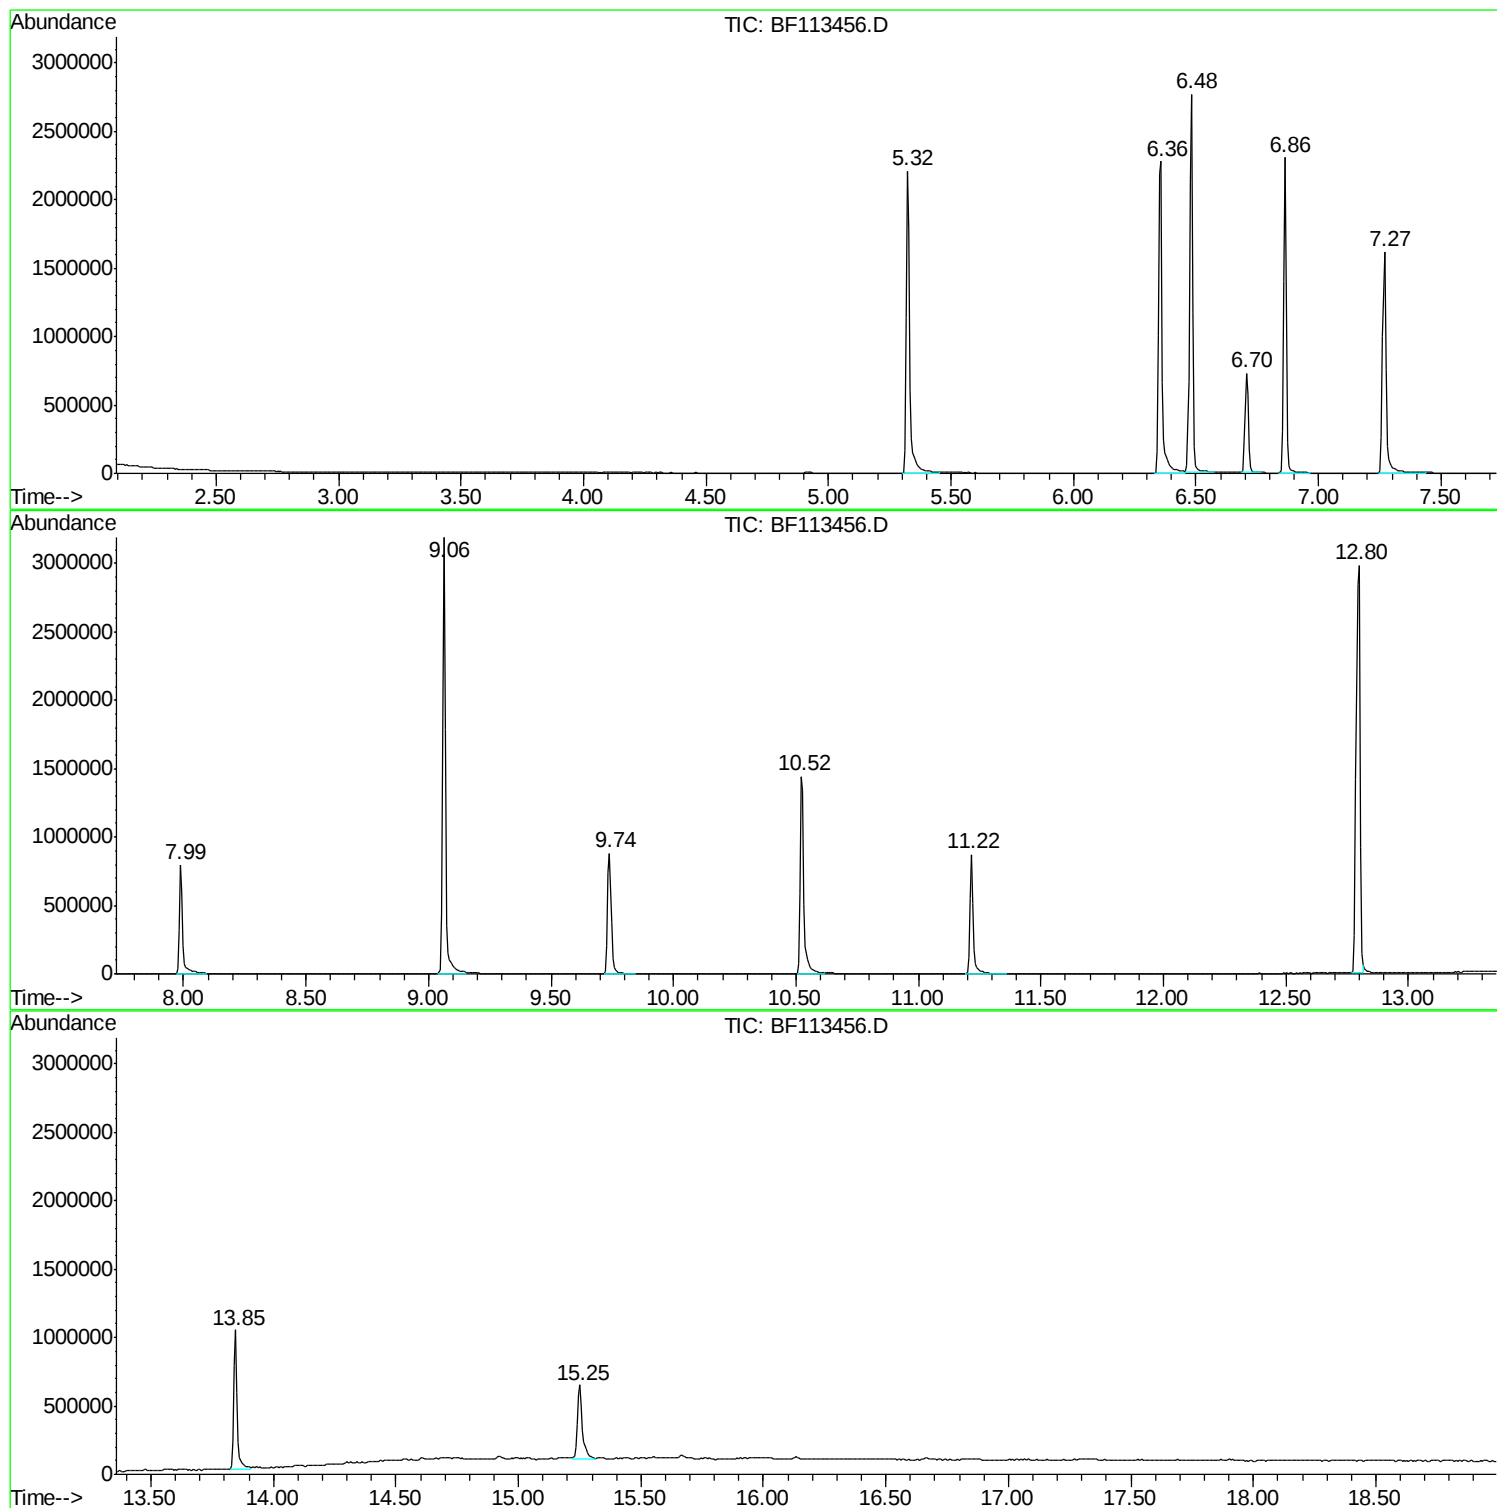

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF032919\
Data File : BF113456.D
Acq On : 30 Mar 2019 12:33
Operator : JU/SJ
Sample : PB118325BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB118325BL









Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF032519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.48 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.48	78.83 ng	2505370	1,4-Dichlorobenzene-d4	6.70

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	12
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
5		Xenon	132	Xe	007440-63-3	9

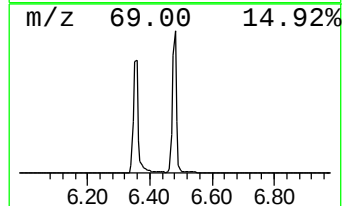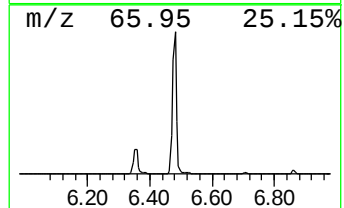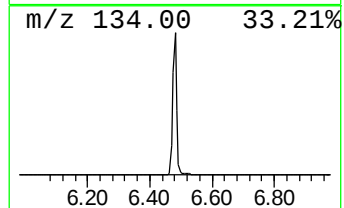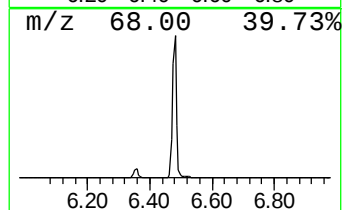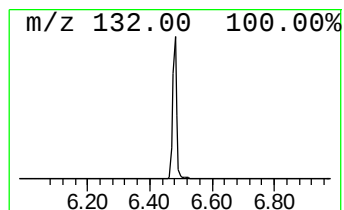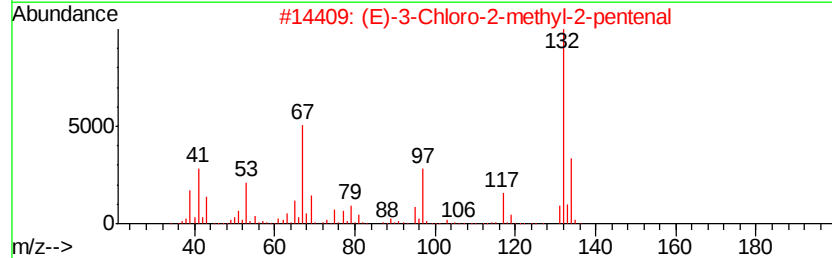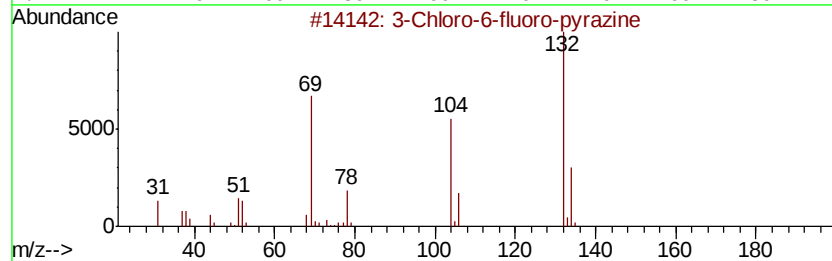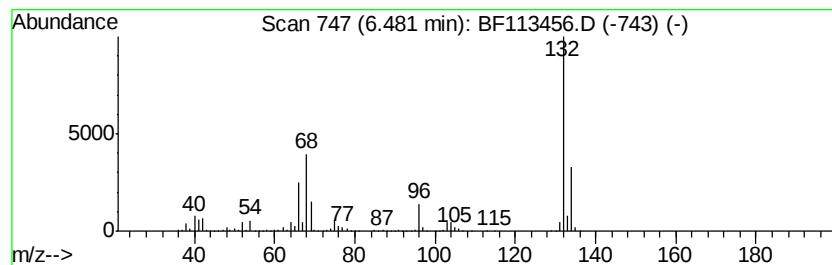

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032919\
Data File : BF113456.D
Acq On : 30 Mar 2019 12:33
Operator : JU/SJ
Sample : PB118325BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB118325BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.48	6.48	78.8	ng	2505370	1	6.70	635616	20.0