


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF032919\  
 Data File : BF113411.D  
 Acq On : 29 Mar 2019 13:59  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF032519.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Mar 26 03:32:08 2019

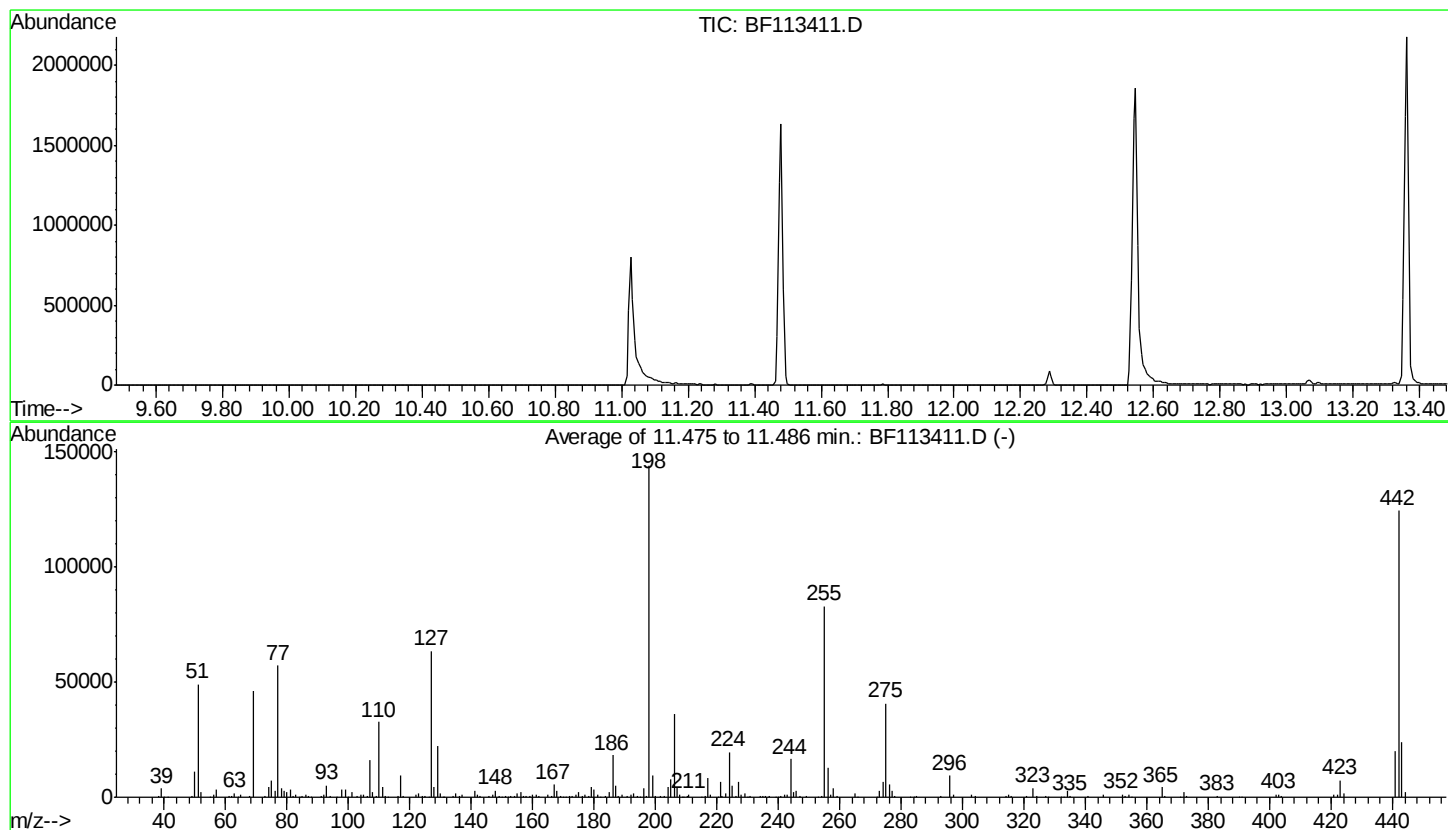

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1591

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 34.2         | 49146      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.2          | 549        | PASS                |
| 69             | 198             | 0.00            | 100             | 31.9         | 45945      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 127            | 198             | 10              | 80              | 44.2         | 63549      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.5          | 776        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 143861     | PASS                |
| 199            | 198             | 5               | 9               | 6.5          | 9369       | PASS                |
| 275            | 198             | 10              | 60              | 28.3         | 40672      | PASS                |
| 365            | 198             | 1               | 100             | 3.1          | 4391       | PASS                |
| 441            | 198             | 0.01            | 100             | 13.8         | 19889      | PASS                |
| 442            | 198             | 50              | 100             | 86.4         | 124248     | PASS                |
| 443            | 442             | 15              | 24              | 19.5         | 24173      | PASS                |