


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032919\
 Data File : BF113436.D
 Acq On : 30 Mar 2019 3:02
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 26 03:32:08 2019

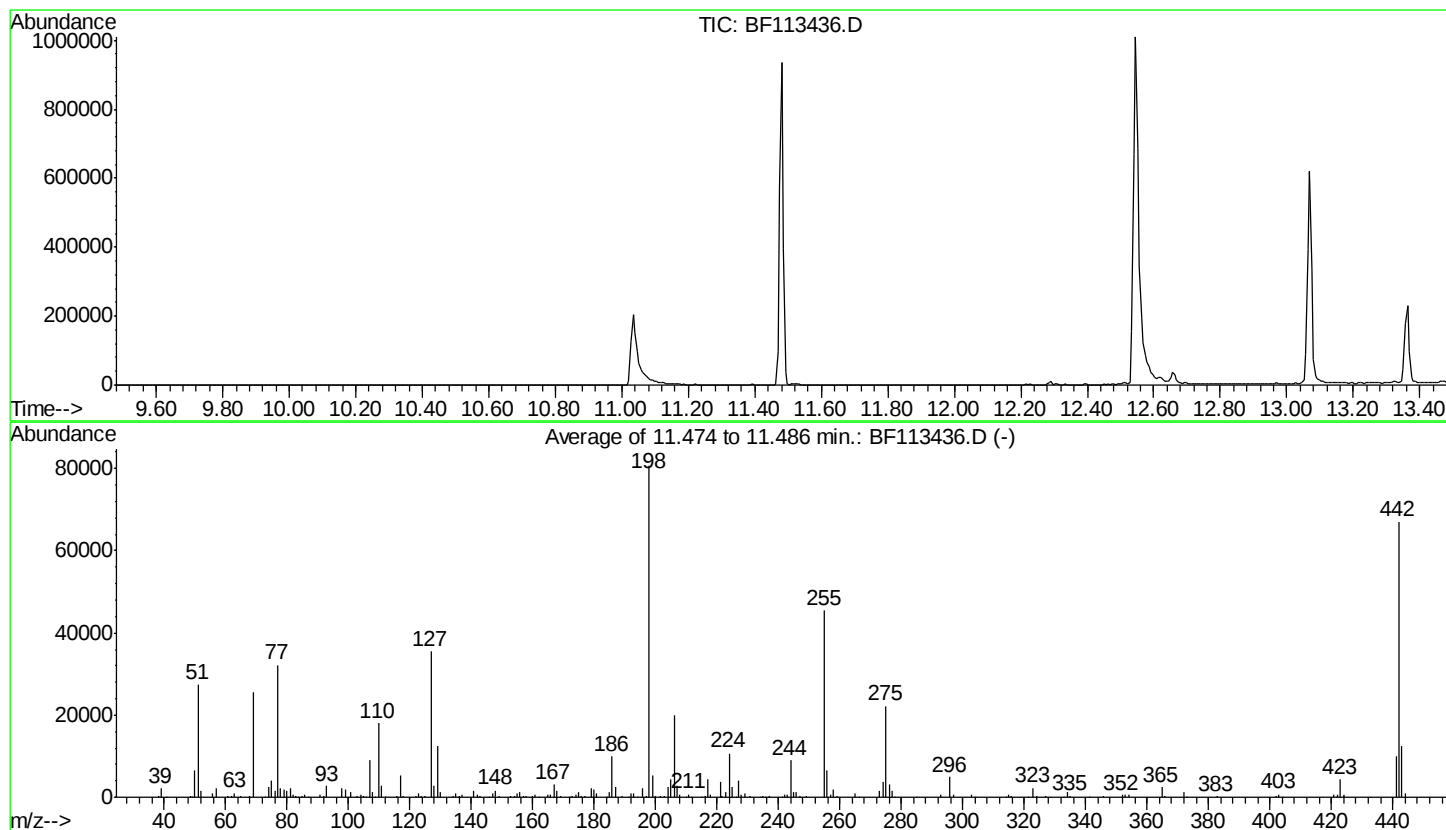

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1591

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	27406	PASS
68	69	0.00	2	1.4	351	PASS
69	198	0.00	100	31.8	25648	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.9	35421	PASS
197	198	0.00	2	0.3	238	PASS
198	198	100	100	100.0	80728	PASS
199	198	5	9	6.5	5228	PASS
275	198	10	60	27.6	22265	PASS
365	198	1	100	3.0	2453	PASS
441	198	0.01	100	12.3	9913	PASS
442	198	50	100	83.0	67005	PASS
443	442	15	24	18.6	12445	PASS