
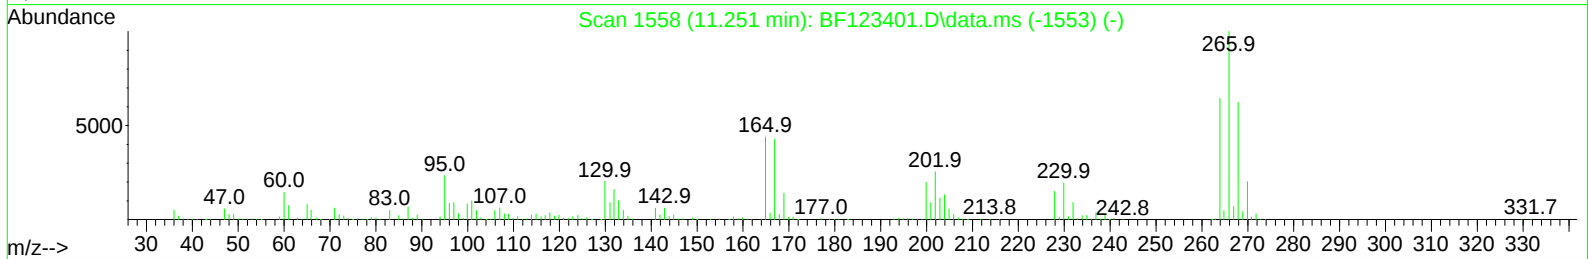
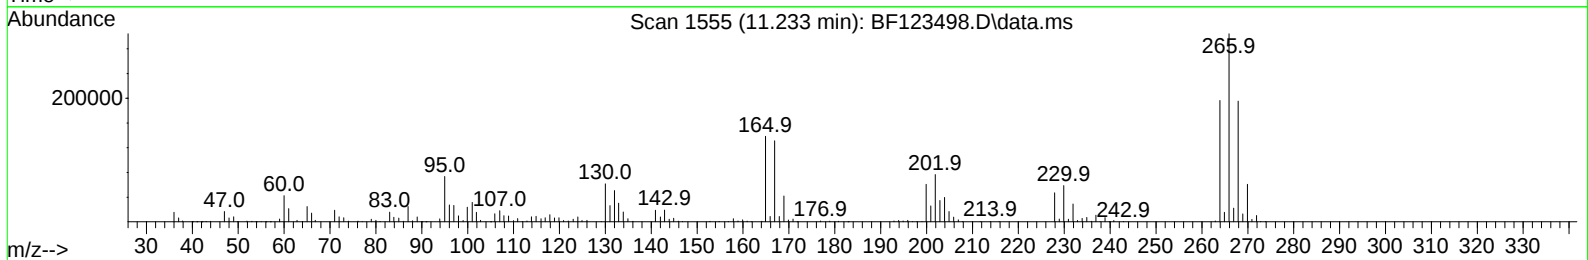


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032921\
Data File : BF123498.D
Acq On : 29 Mar 2021 14:30
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 15:52:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 26 12:51:59 2021
Response via : Initial Calibration

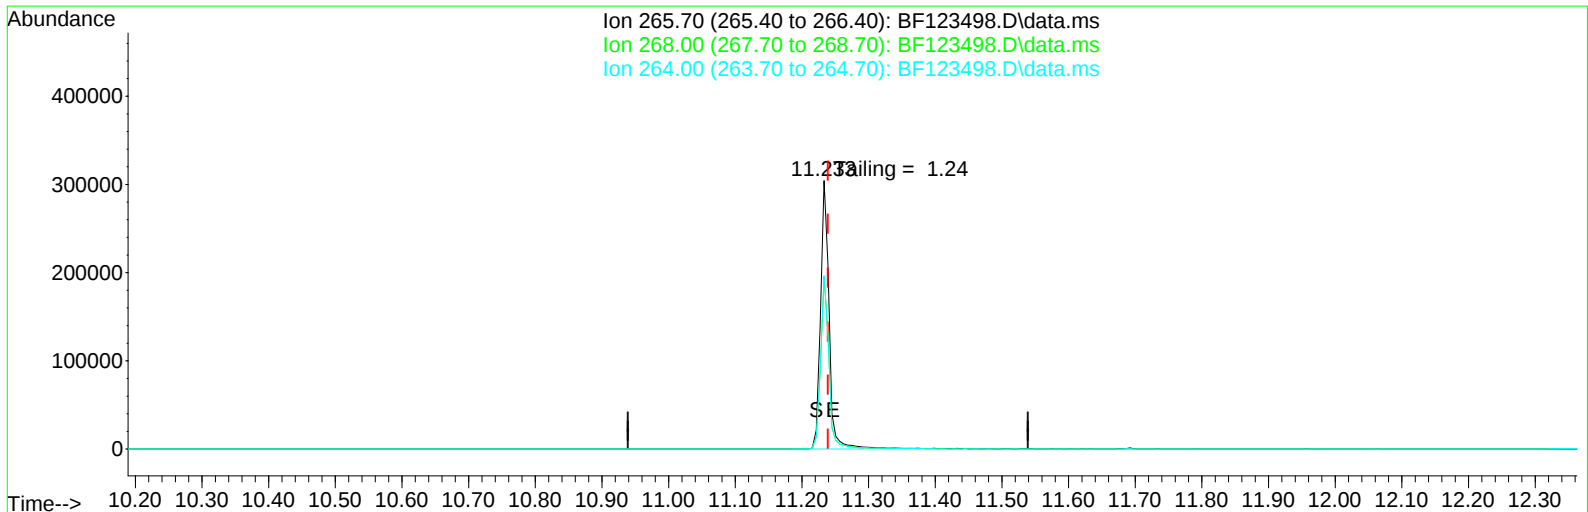

TIC: BF123498.D\data.ms

(70) Pentachlorophenol (C)




11.233min (-0.006) 30676.65 ng

response 273559

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.19
264.00	62.30	64.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032921\
Data File : BF123498.D
Acq On : 29 Mar 2021 14:30
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 15:52:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 26 12:51:59 2021
Response via : Initial Calibration

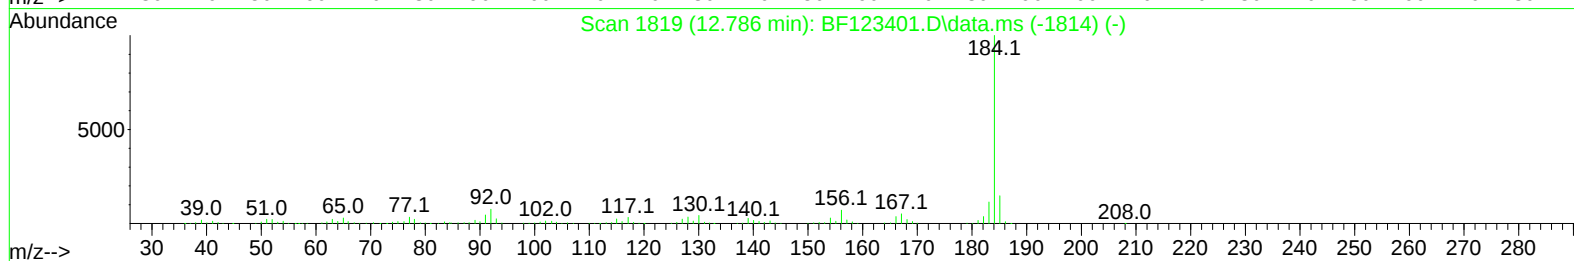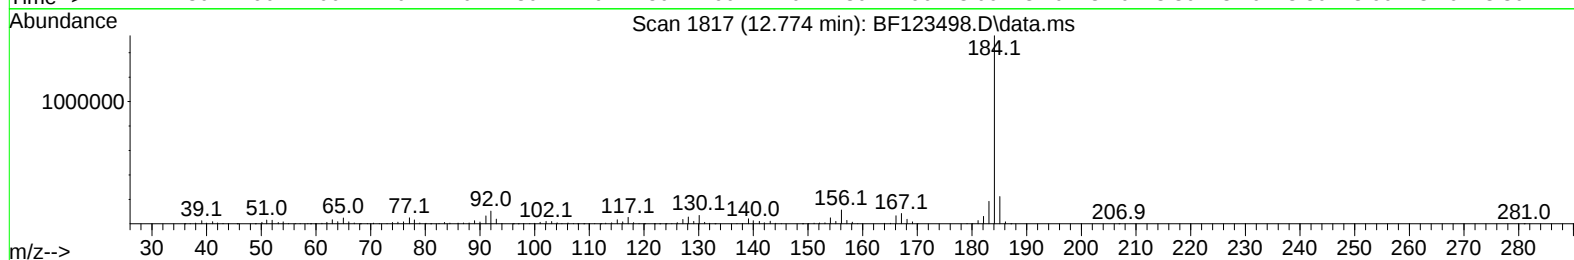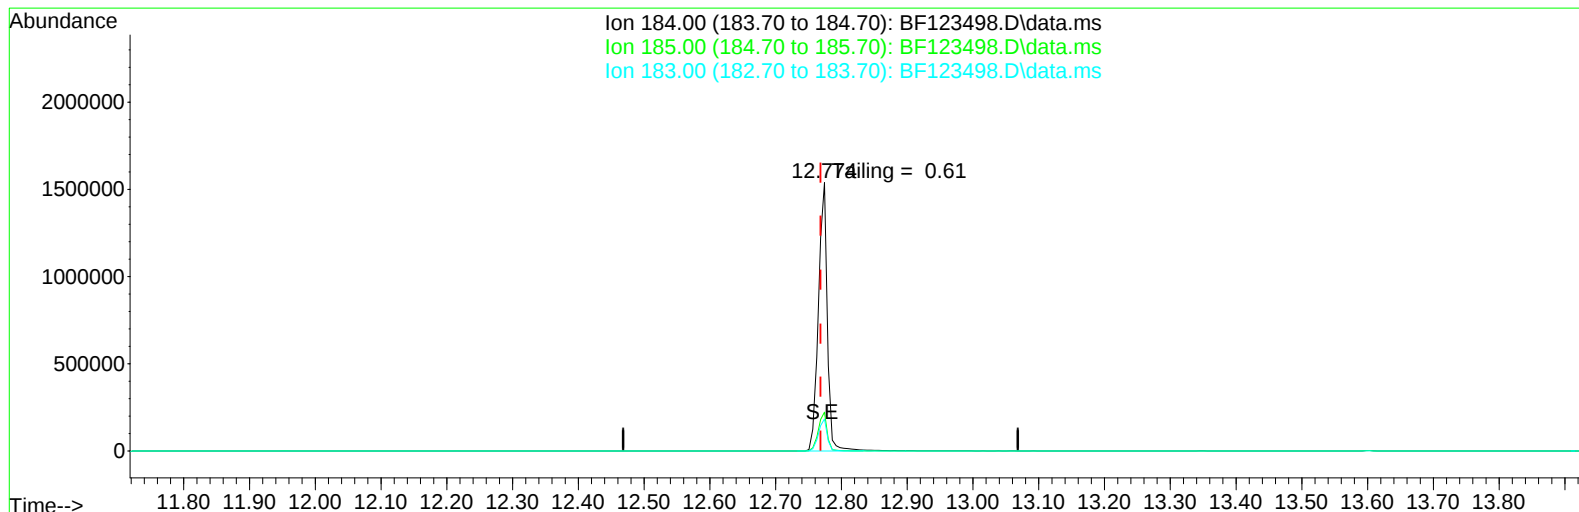

TIC: BF123498.D\data.ms

(77) Benzidine

12.774min (+ 0.006) 0.00 ng

response 1462208

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.49
183.00	12.10	11.92
0.00	0.00	0.00