
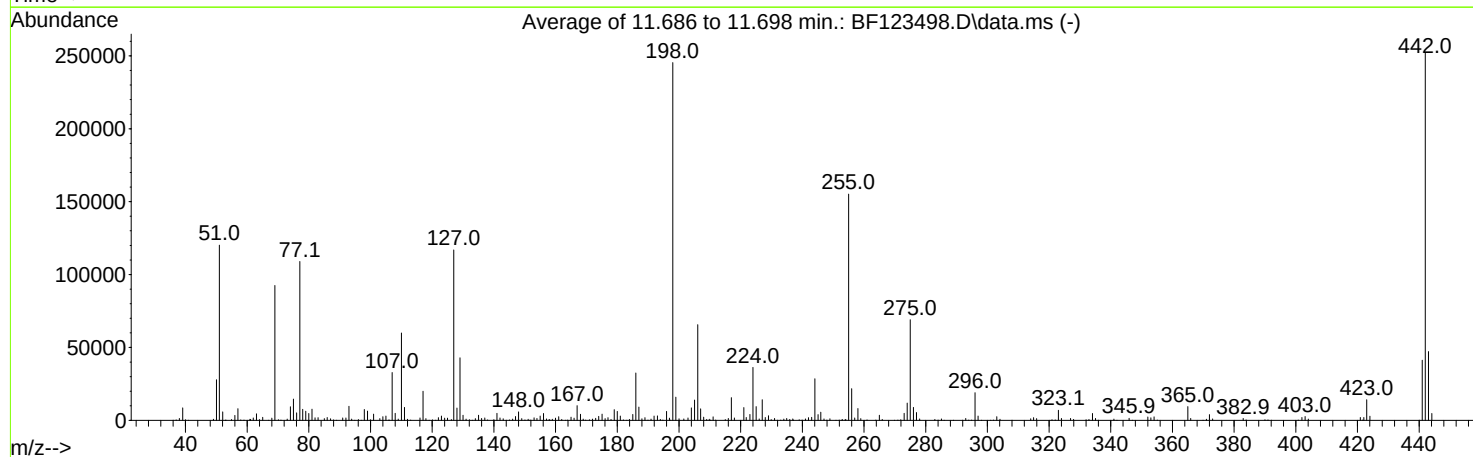


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032921\
 Data File : BF123498.D
 Acq On : 29 Mar 2021 14:30
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 26 12:51:59 2021

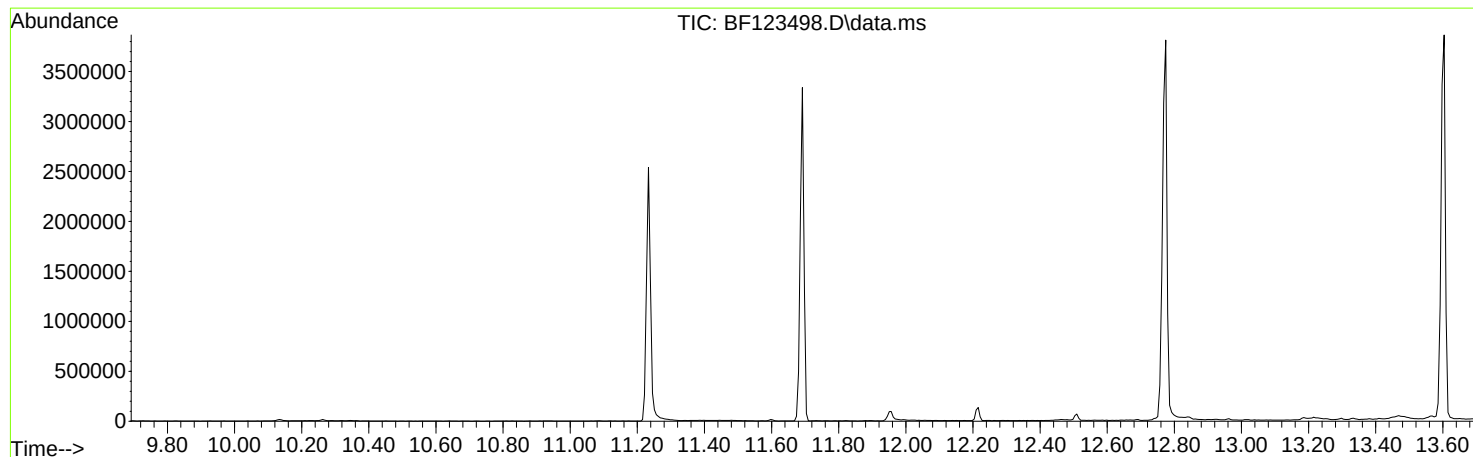

AutoFind: Scans 1632, 1633, 1634; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.0	120155	PASS
68	69	0.00	2	1.6	1524	PASS
69	198	0.00	100	37.7	92493	PASS
70	69	0.00	2	0.5	479	PASS
127	198	10	80	47.6	116896	PASS
197	198	0.00	2	0.6	1508	PASS
198	198	100	100	100.0	245355	PASS
199	198	5	9	6.5	15947	PASS
275	198	10	60	28.2	69077	PASS
365	198	1	100	3.8	9423	PASS
441	198	0.01	100	16.8	41307	PASS
442	442	50	100	100.0	252317	PASS
443	442	15	24	18.7	47224	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/29/2021	BNA_F	<u>BF123498.D</u>
Compound Name	Response	Retention Time
DDT	665728	13.6
DDD	3192	13.29
DDE	1802	12.96
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4994	670722	0.74

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032921\
 Data File : BF123498.D
 Acq On : 29 Mar 2021 14:30
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 29 15:52:22 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 26 12:51:59 2021
 Response via : Initial Calibration

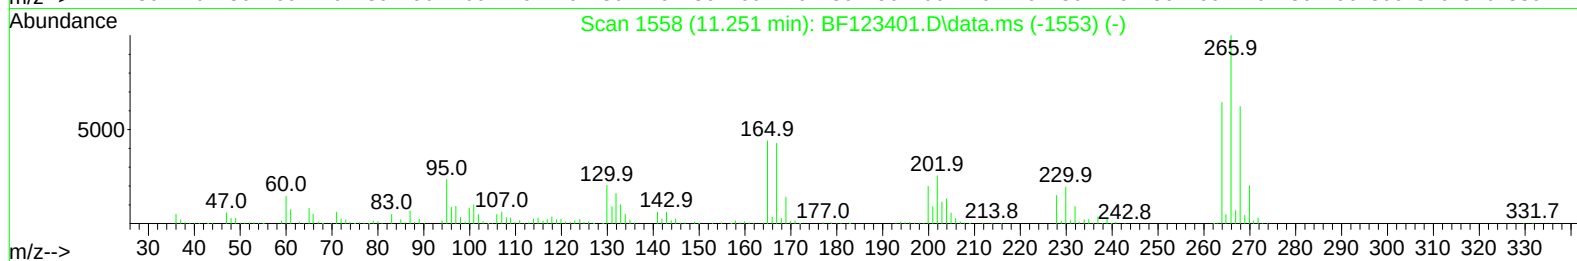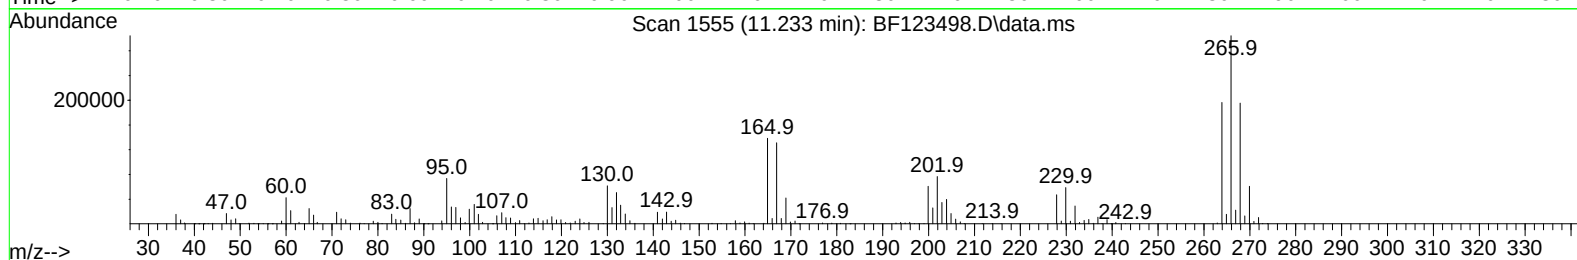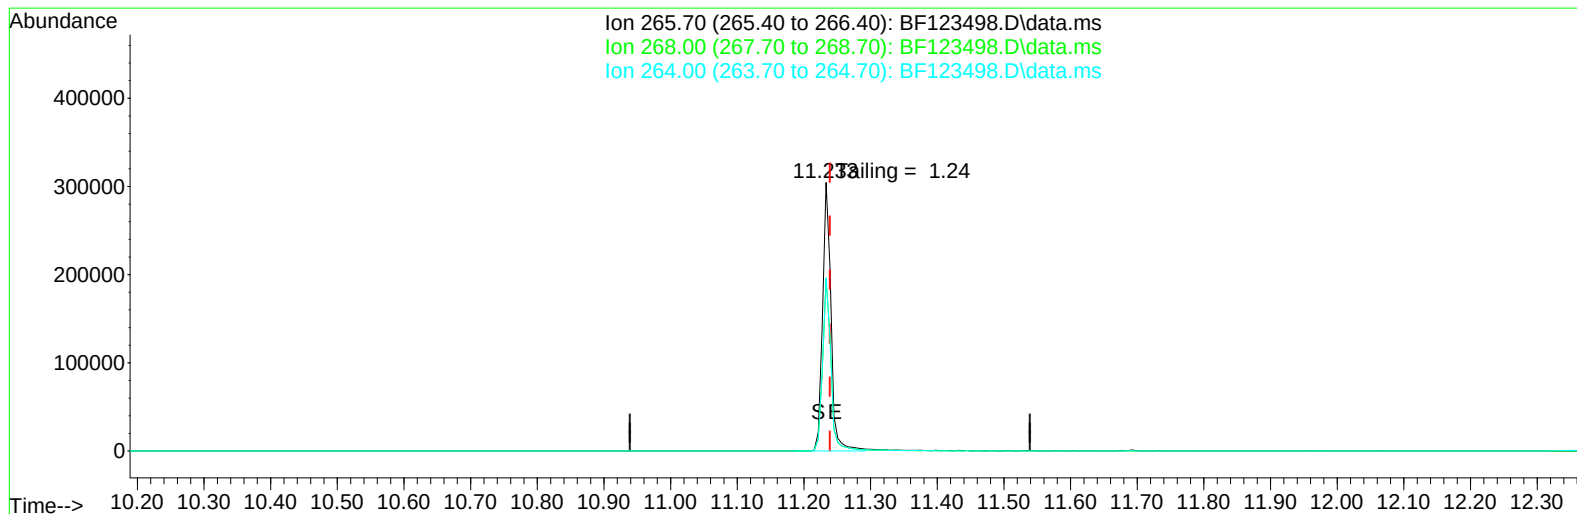

TIC: BF123498.D\data.ms

(70) Pentachlorophenol (C)

11.233min (-0.006) 30676.65 ng




response 273559

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.19
264.00	62.30	64.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032921\
Data File : BF123498.D
Acq On : 29 Mar 2021 14:30
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 29 15:52:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 26 12:51:59 2021
Response via : Initial Calibration

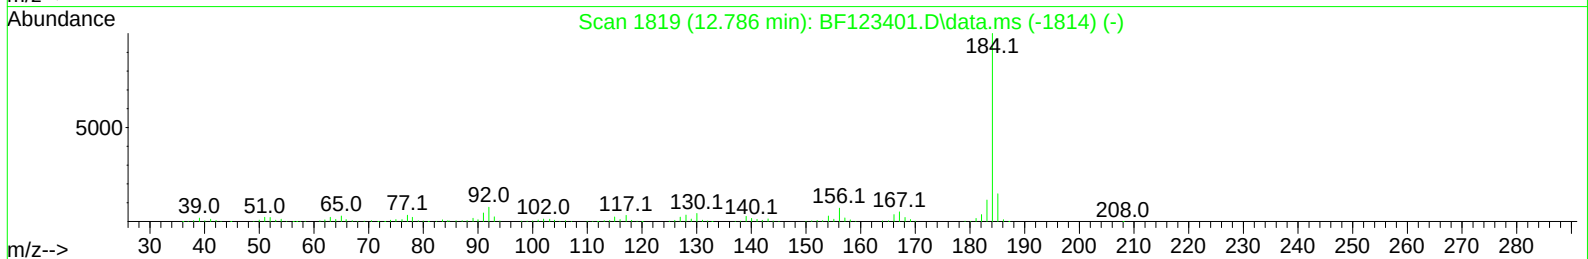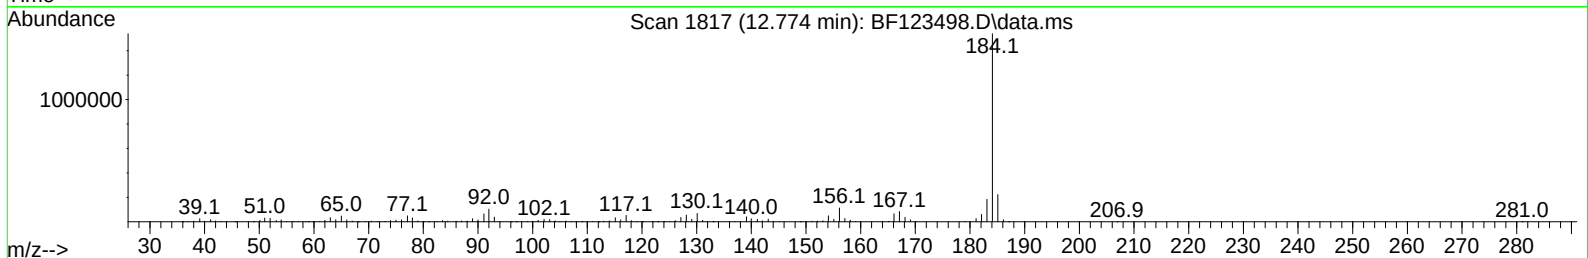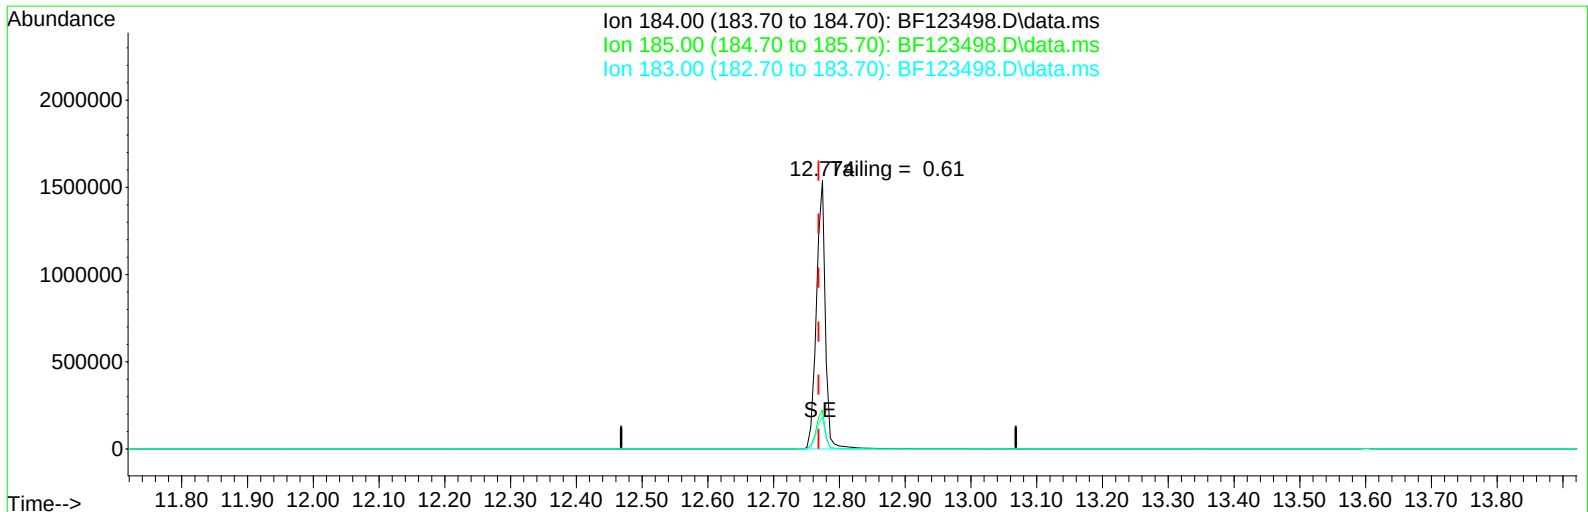

TIC: BF123498.D\data.ms

(77) Benzidine

12.774min (+ 0.006) 0.00 ng

response 1462208

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.49
183.00	12.10	11.92
0.00	0.00	0.00