


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF033020\
 Data File : BF119628.D
 Acq On : 30 Mar 2020 12:00
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 31 14:11:44 2020

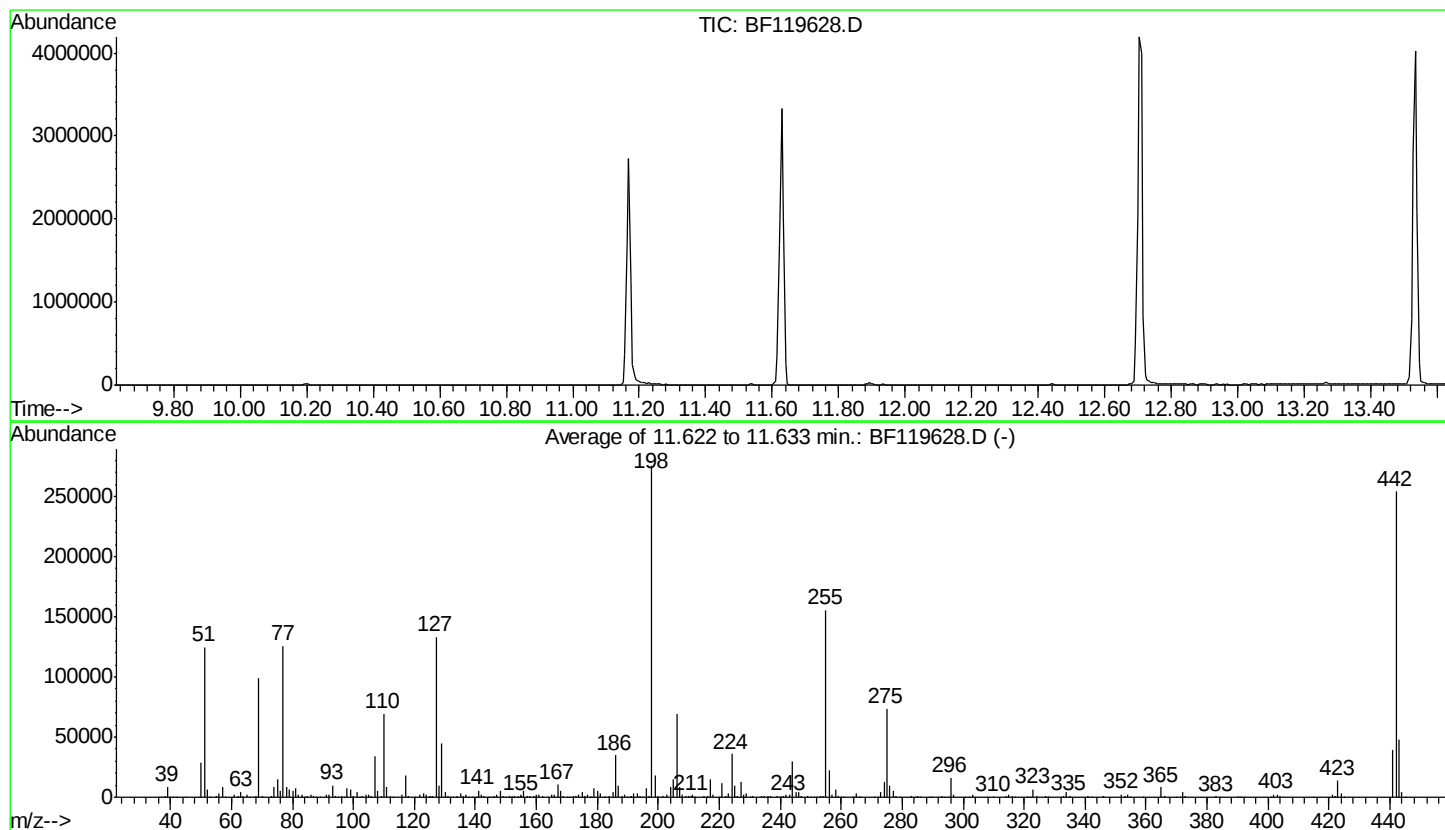

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.2	124530	PASS
68	69	0.00	2	1.6	1601	PASS
69	198	0.00	100	36.0	99298	PASS
70	69	0.00	2	0.7	654	PASS
127	198	10	80	48.4	133258	PASS
197	198	0.00	2	0.3	758	PASS
198	198	100	100	100.0	275498	PASS
199	198	5	9	6.6	18173	PASS
275	198	10	60	26.7	73589	PASS
365	198	1	100	3.0	8164	PASS
441	198	0.01	100	14.4	39792	PASS
442	198	50	100	92.1	253762	PASS
443	442	15	24	18.7	47464	PASS