
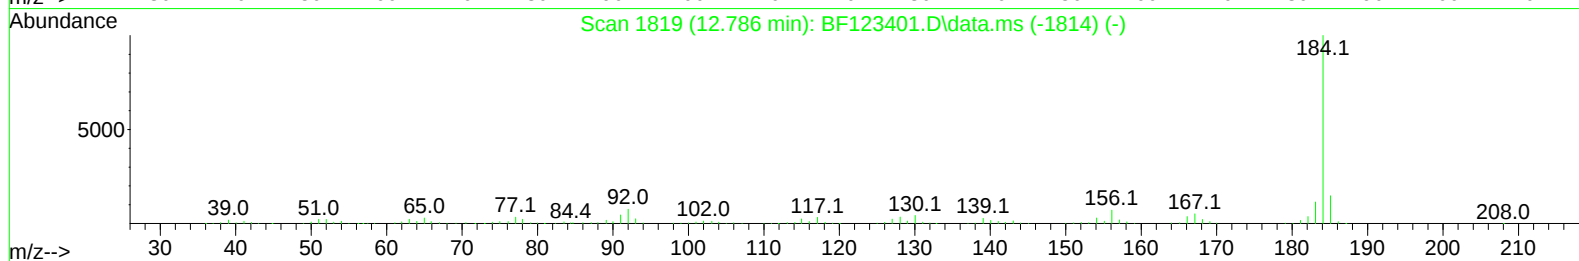
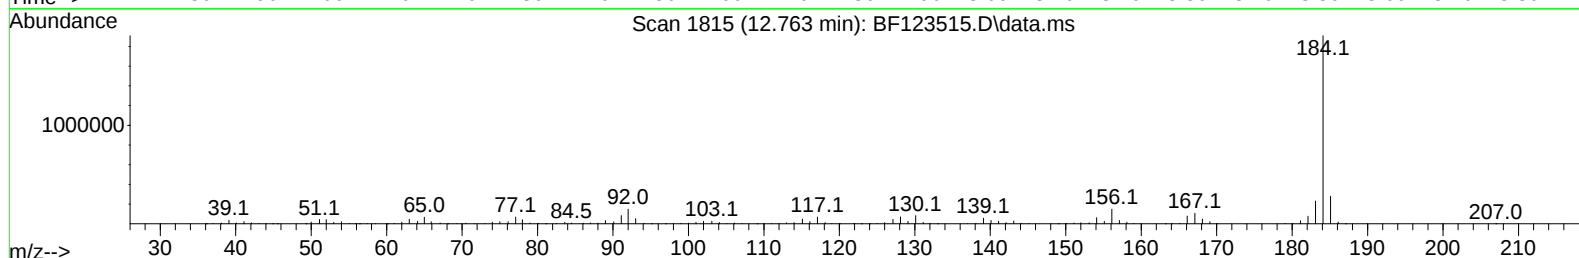


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF033021\
 Data File : BF123515.D
 Acq On : 30 Mar 2021 10:17
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 30 11:42:22 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 26 12:51:59 2021
 Response via : Initial Calibration

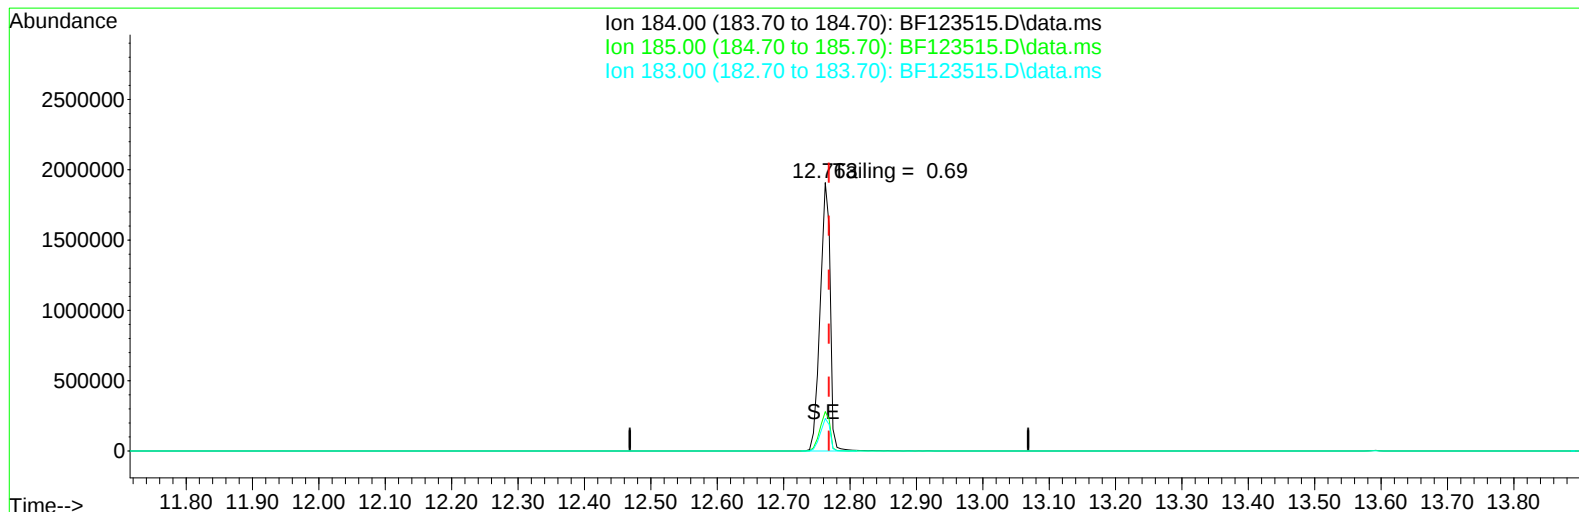

TIC: BF123515.D\data.ms

(77) Benzidine




12.763min (-0.006) 0.00 ng

response 2004020

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.69
183.00	12.10	12.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF033021\
 Data File : BF123515.D
 Acq On : 30 Mar 2021 10:17
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 30 11:42:22 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 26 12:51:59 2021
 Response via : Initial Calibration

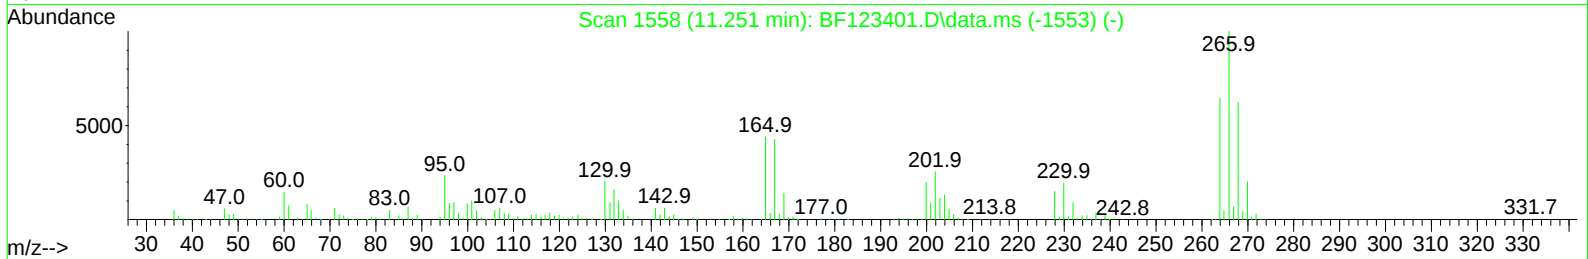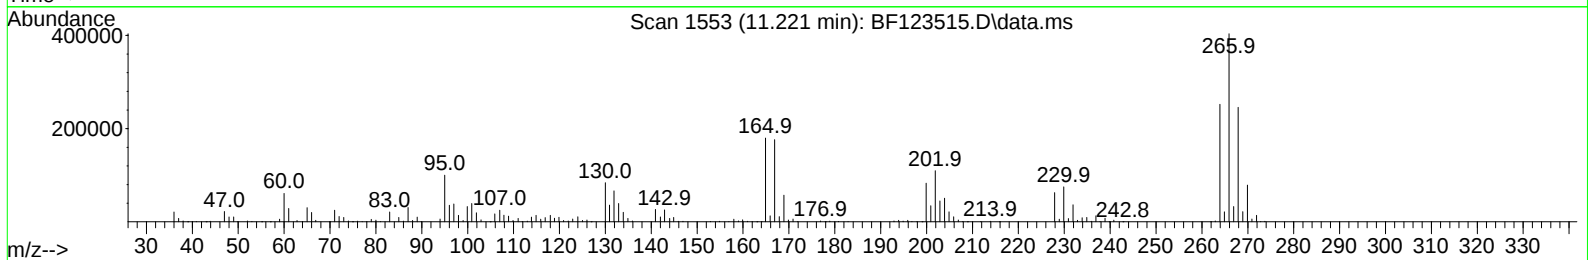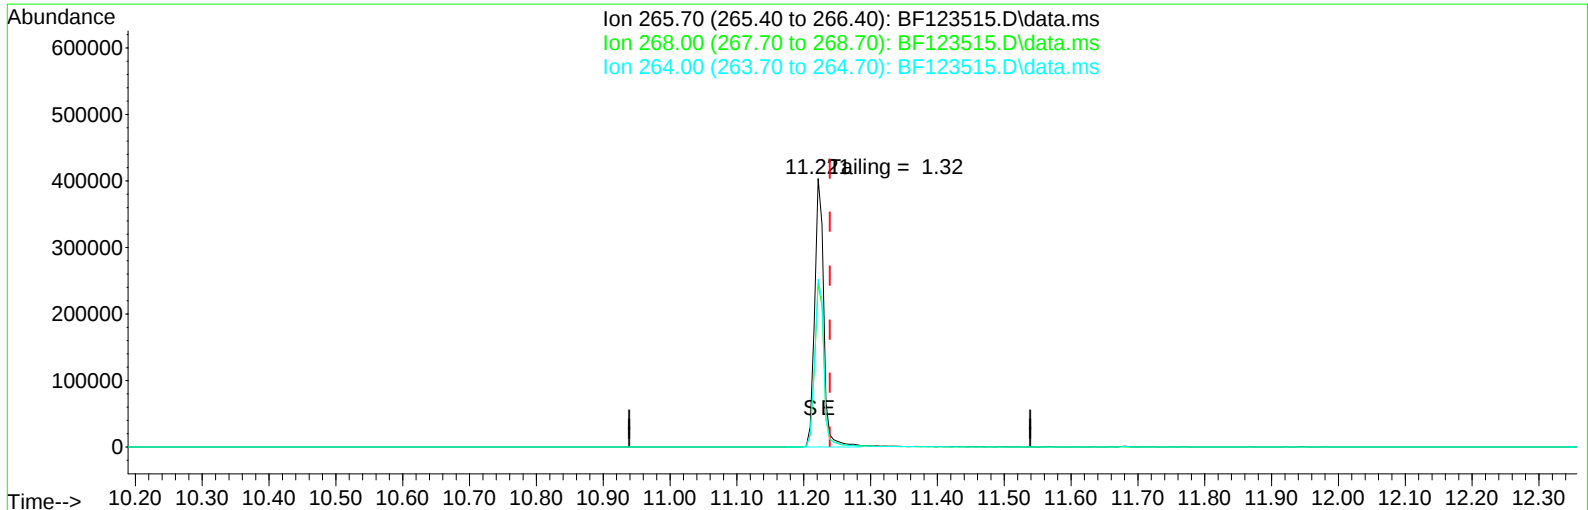

TIC: BF123515.D\data.ms

(70) Pentachlorophenol (C)

11.221min (-0.018) 29269.51 ng

response 386843

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	60.86
264.00	62.30	62.49
0.00	0.00	0.00