
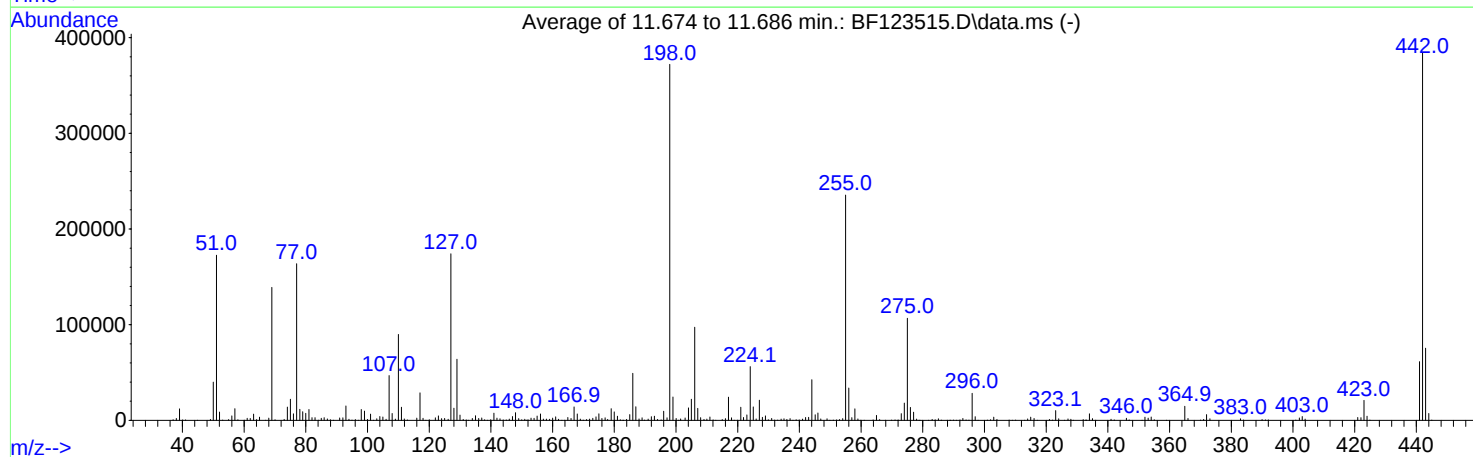


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF033021\
 Data File : BF123515.D
 Acq On : 30 Mar 2021 10:17
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 30 11:51:25 2021

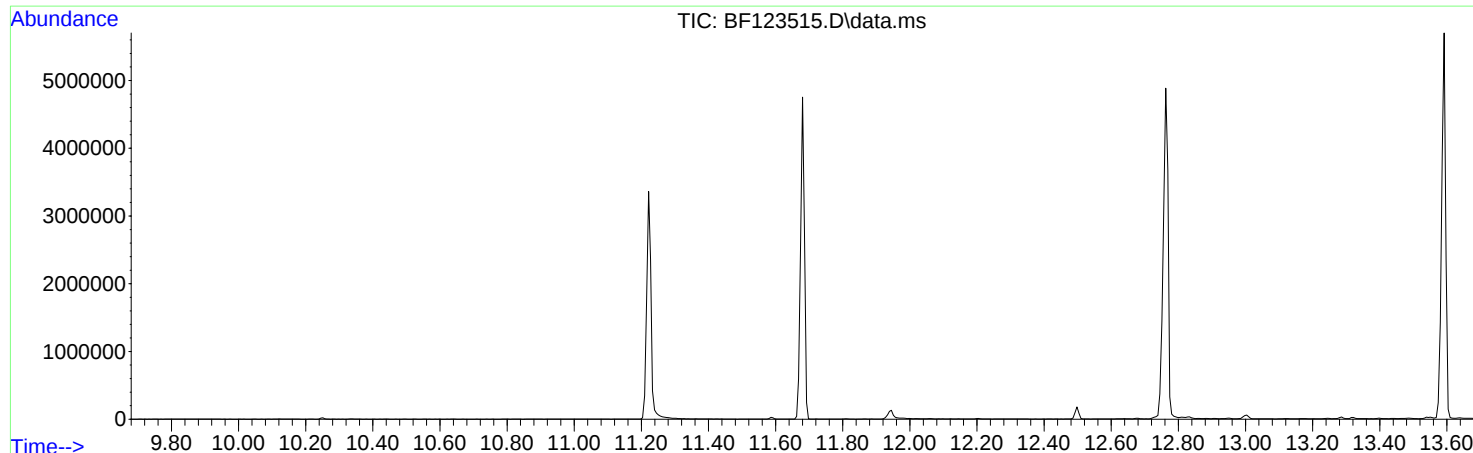




AutoFind: Scans 1630, 1631, 1632; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.4	172632	PASS
68	69	0.00	2	1.7	2298	PASS
69	198	0.00	100	37.4	139000	PASS
70	69	0.00	2	0.5	750	PASS
127	198	10	80	46.8	174123	PASS
197	198	0.00	2	0.7	2720	PASS
198	198	100	100	100.0	371989	PASS
199	198	5	9	6.6	24491	PASS
275	198	10	60	28.7	106723	PASS
365	198	1	100	4.0	14775	PASS
441	198	0.01	100	16.5	61333	PASS
442	442	50	100	100.0	384448	PASS
443	442	15	24	19.6	75400	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF033021\
Data File : BF123515.D
Acq On : 30 Mar 2021 10:17
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 30 11:42:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 26 12:51:59 2021
Response via : Initial Calibration

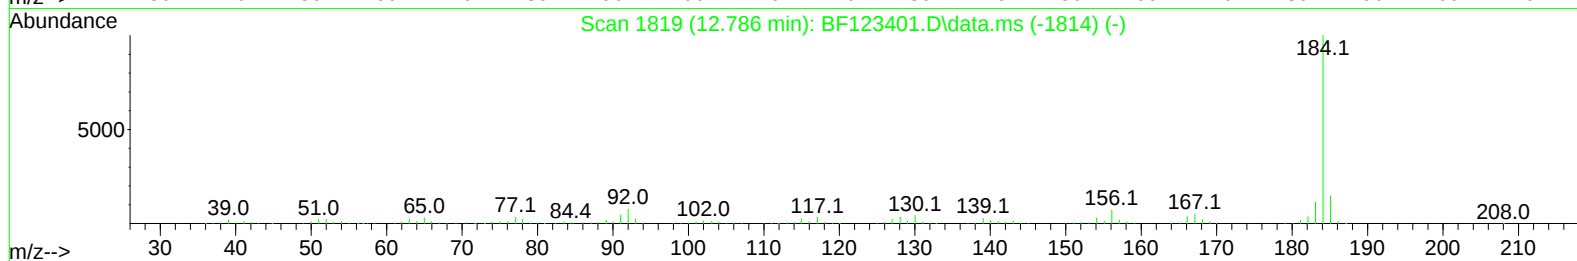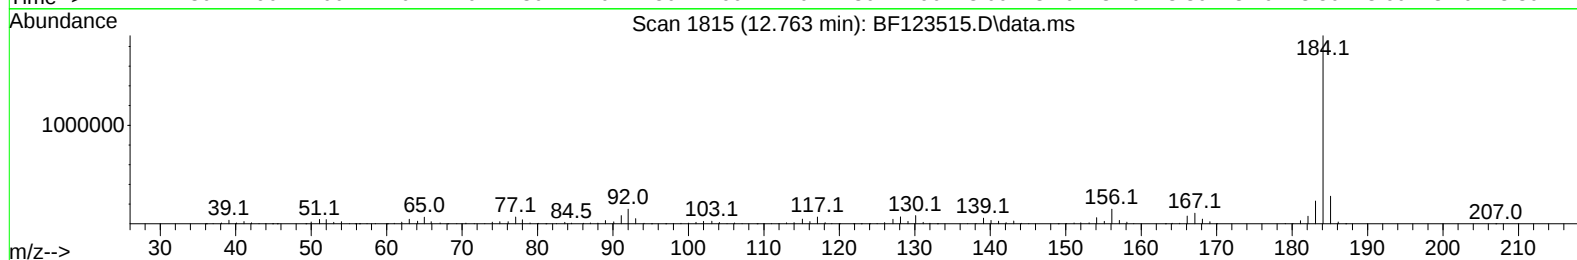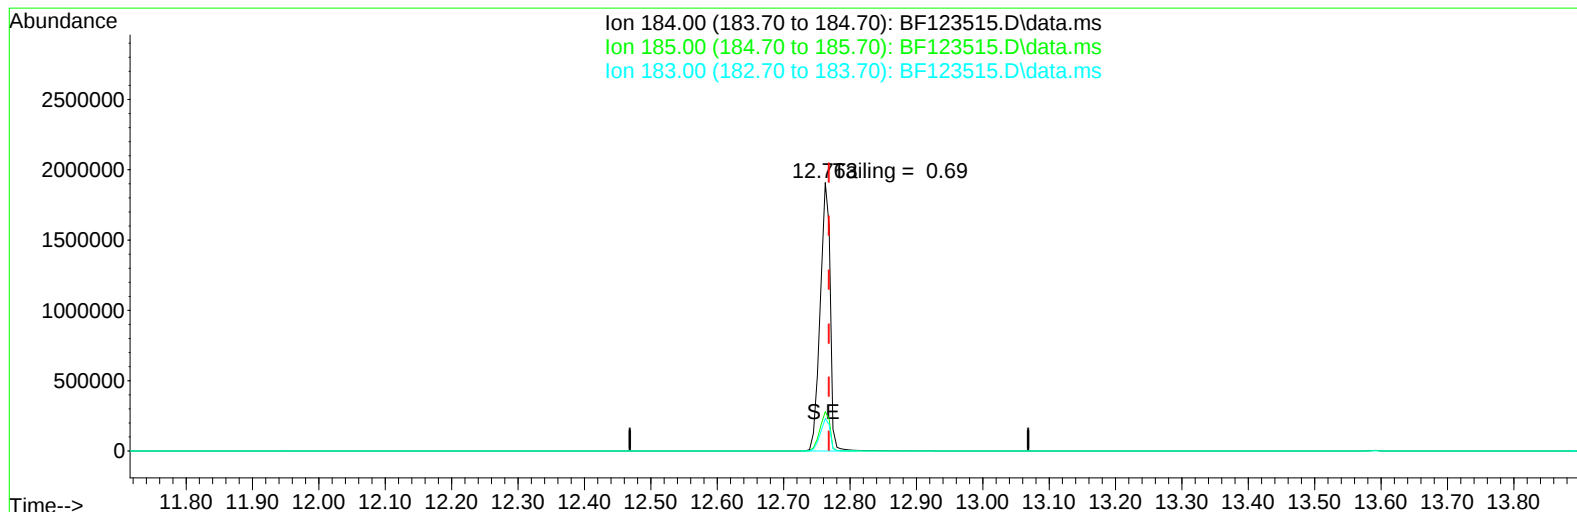

TIC: BF123515.D\data.ms

(77) Benzidine

12.763min (-0.006) 0.00 ng




response 2004020

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.69
183.00	12.10	12.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF033021\
Data File : BF123515.D
Acq On : 30 Mar 2021 10:17
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 30 11:42:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 26 12:51:59 2021
Response via : Initial Calibration

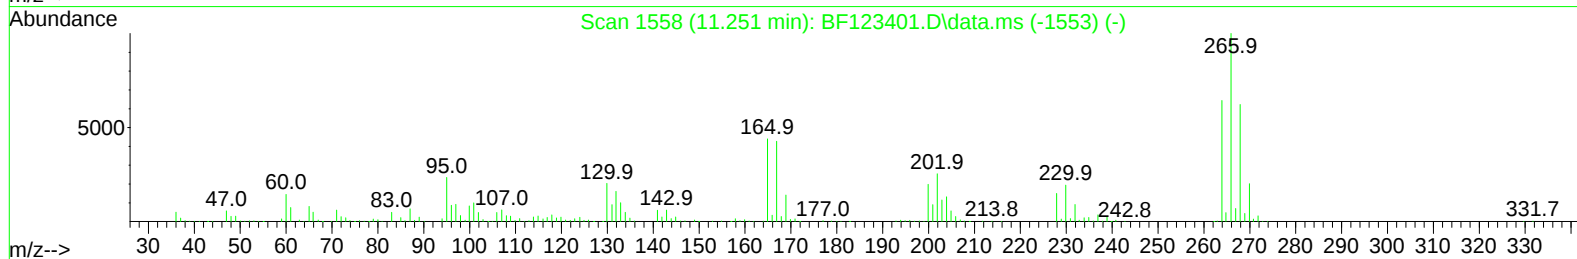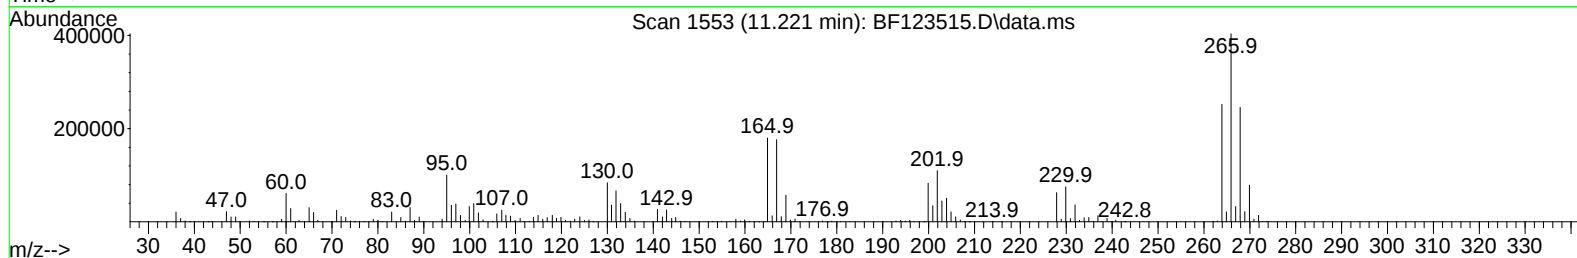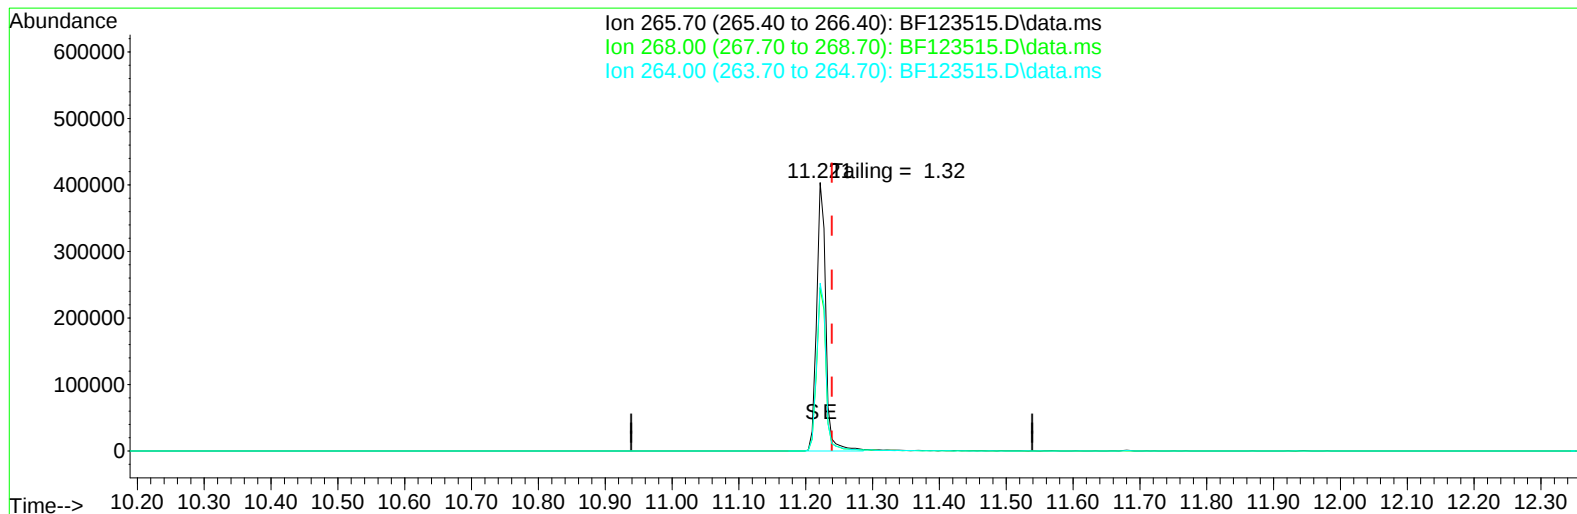

TIC: BF123515.D\data.ms

(70) Pentachlorophenol (C)

11.221min (-0.018) 29269.51 ng

response 386843

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	60.86
264.00	62.30	62.49
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/30/2021	BNA_F	<u>BF123515.D</u>
Compound Name	Response	Retention Time
DDT	950260	13.59
DDD	4789	13.28
DDE	1758	12.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6547	956807	0.68