
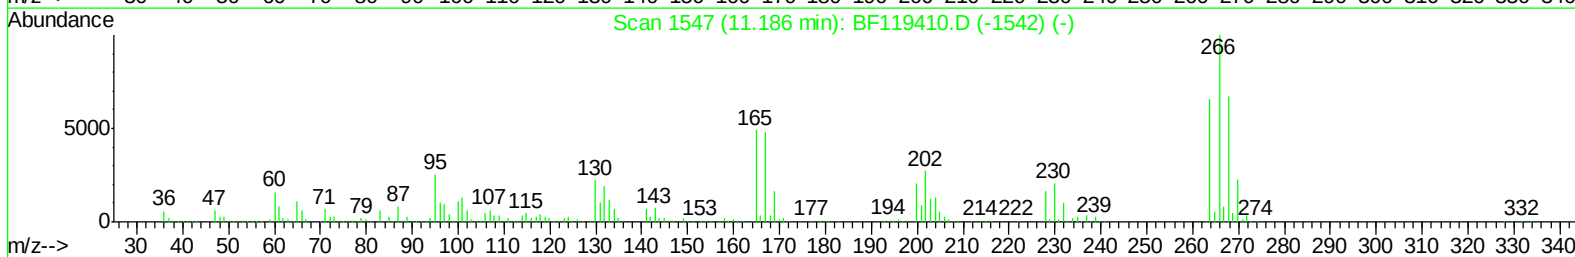
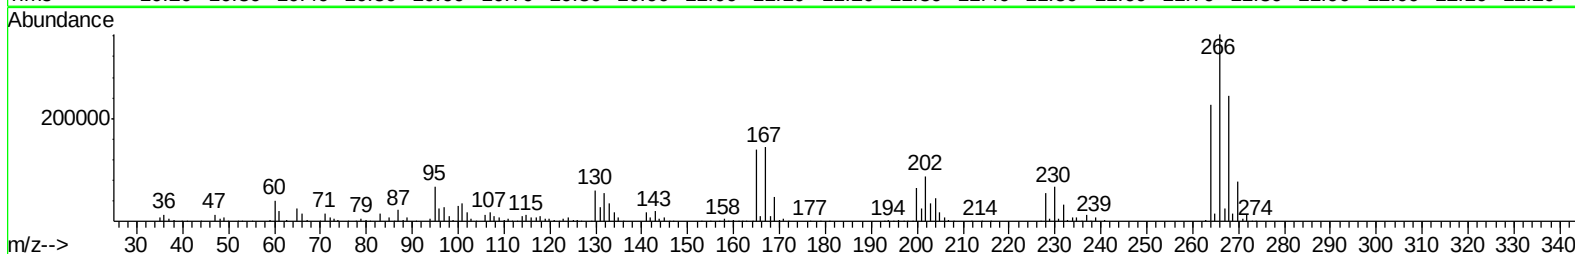


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF033120\
Data File : BF119647.D
Acq On : 31 Mar 2020 12:44
Operator : MA/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 31 23:52:00 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 31 14:11:44 2020
Response via : Initial Calibration

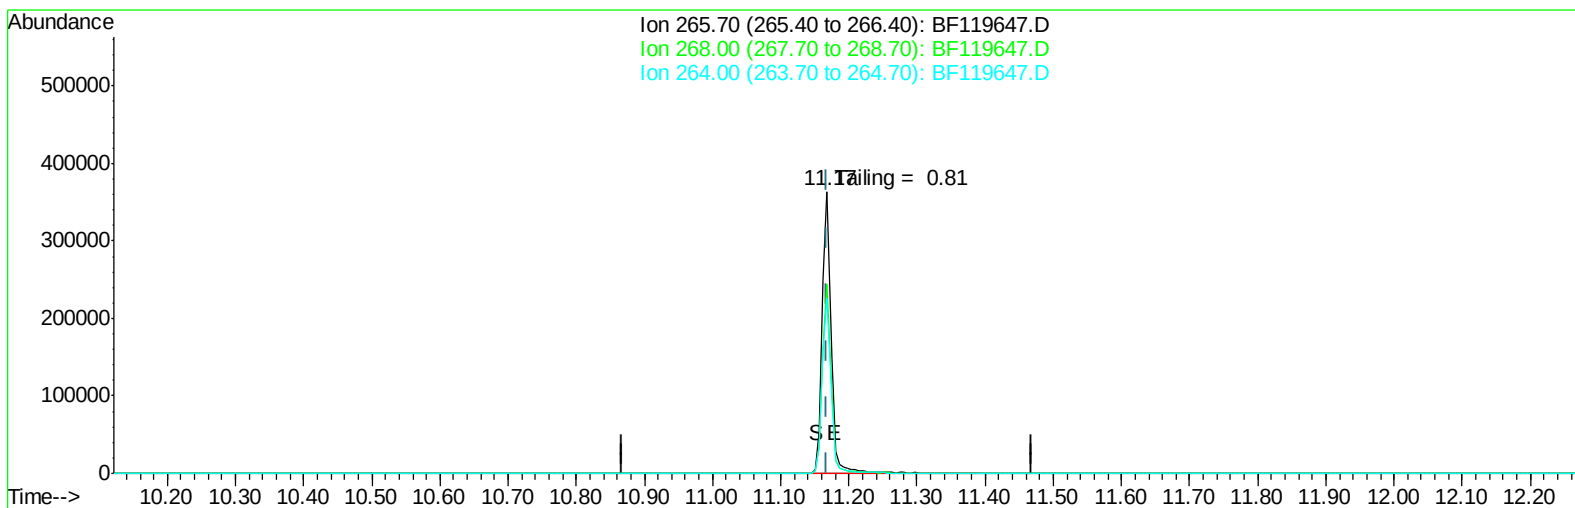

TIC: BF119647.D

(70) Pentachlorophenol (C)




11.168min (-0.000) 44309.25ng

response 318281

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	67.29
264.00	61.20	62.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF033120\
 Data File : BF119647.D
 Acq On : 31 Mar 2020 12:44
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 31 23:52:00 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 31 14:11:44 2020
 Response via : Initial Calibration

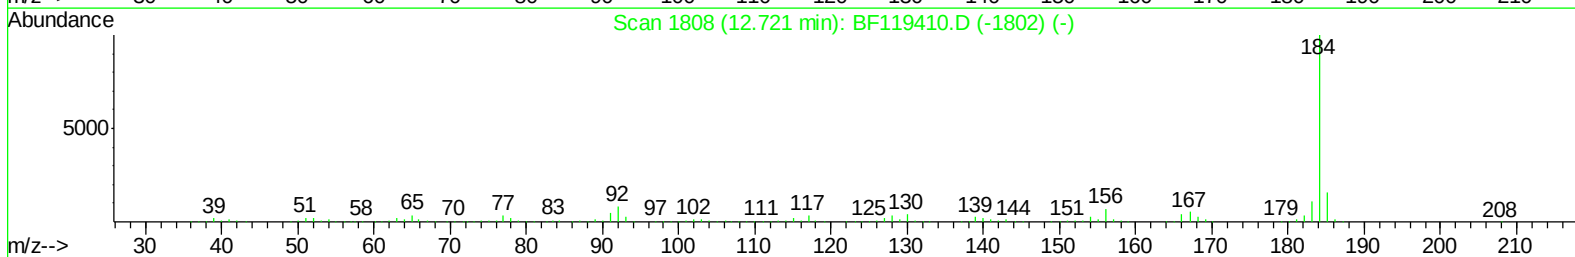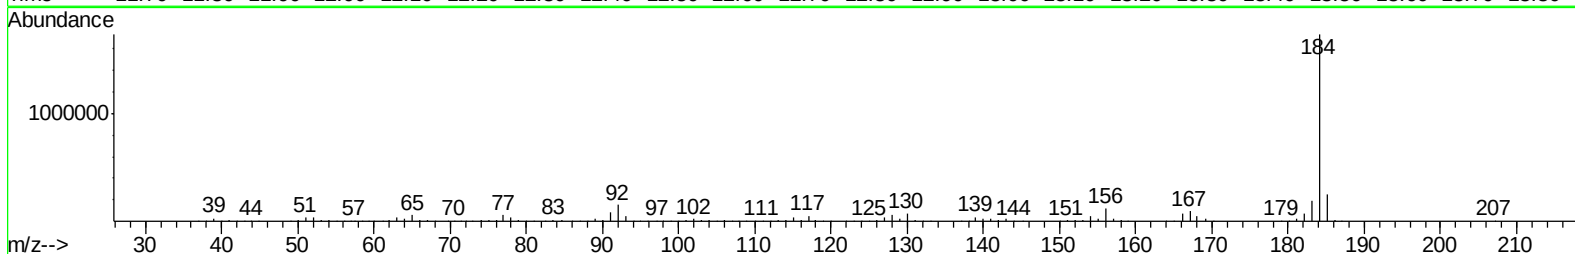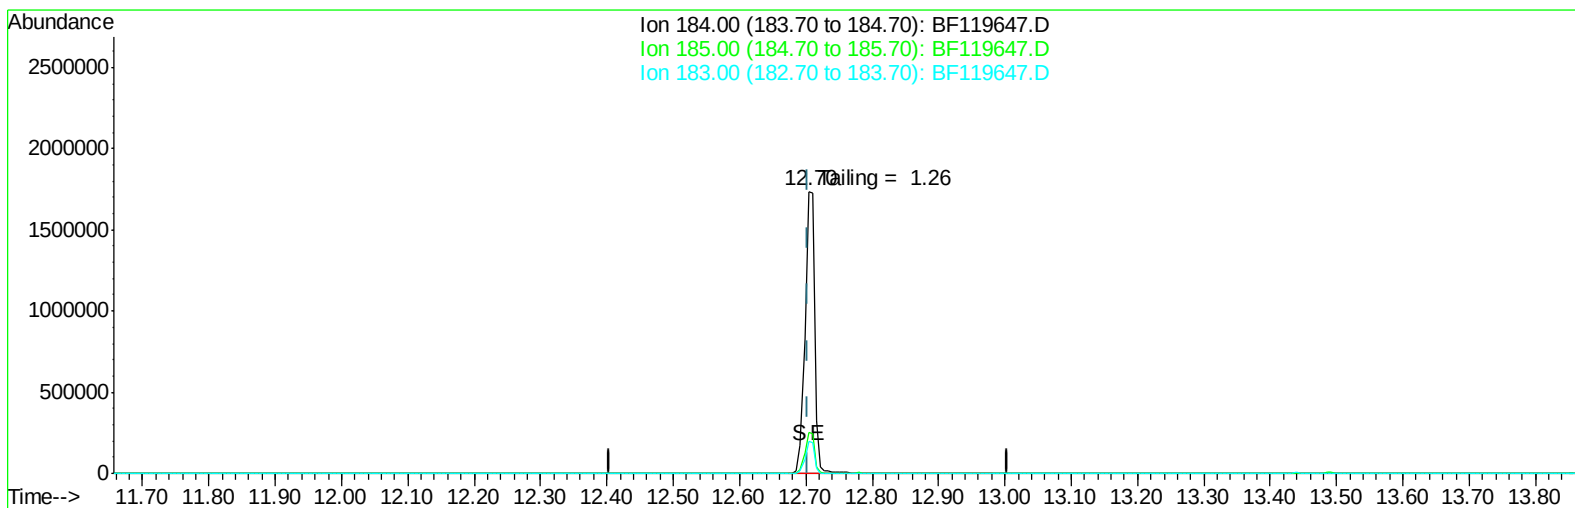

TIC: BF119647.D

(77) Benzidine

12.704min (-0.000) 0.00ng

response 1738665

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	14.34
183.00	11.30	11.22
0.00	0.00	0.00