


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF033120\
 Data File : BF119647.D
 Acq On : 31 Mar 2020 12:44
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 31 14:11:44 2020

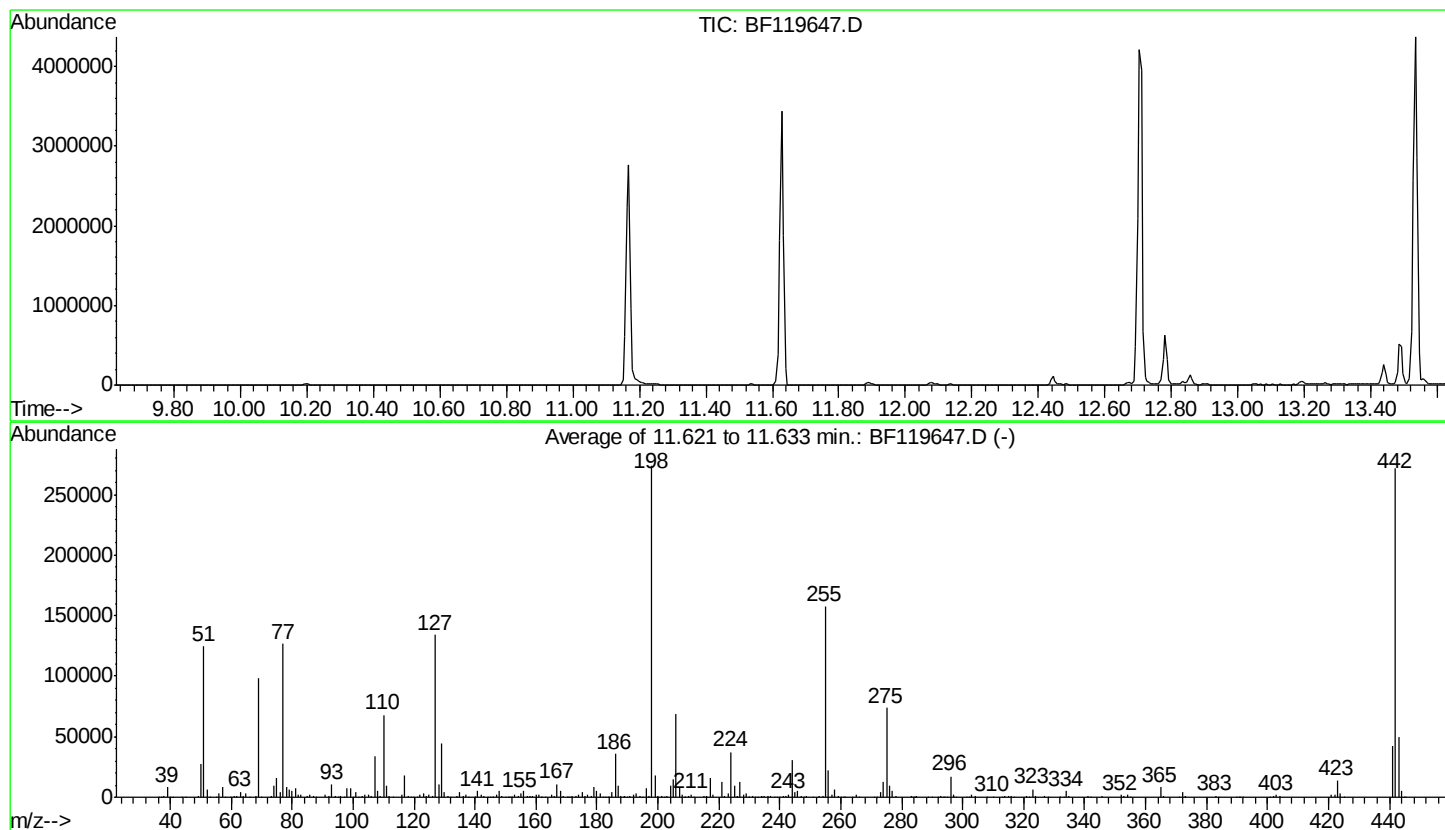

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.5	124648	PASS
68	69	0.00	2	1.5	1450	PASS
69	198	0.00	100	35.8	98082	PASS
70	69	0.00	2	0.5	462	PASS
127	198	10	80	49.0	134165	PASS
197	198	0.00	2	0.3	809	PASS
198	198	100	100	100.0	273920	PASS
199	198	5	9	6.5	17858	PASS
275	198	10	60	26.9	73597	PASS
365	198	1	100	3.0	8177	PASS
441	198	0.01	100	15.5	42594	PASS
442	198	50	100	99.1	271496	PASS
443	442	15	24	18.4	50058	PASS