

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF033122\
 Data File : BF127597.D
 Acq On : 31 Mar 2022 11:02
 Operator : CG\JU
 Sample : PB143744BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB143744BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127597.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.475	538	542	569	rBV	3407130	3909127	84.31%	13.690%
2	6.481	708	713	716	rBV	3221625	3912533	84.38%	13.701%
3	6.828	769	772	782	rBV	834221	809065	17.45%	2.833%
4	7.404	864	870	873	rBV	2373866	2778704	59.93%	9.731%
5	8.116	986	991	1006	rBV	1068829	1087134	23.45%	3.807%
6	9.192	1167	1174	1177	rBV	4221955	4636573	100.00%	16.237%
7	9.869	1284	1289	1304	rBV	1316977	1273138	27.46%	4.458%
8	10.669	1420	1425	1444	rBV	2644147	2778081	59.92%	9.729%
9	11.363	1540	1543	1552	rBV	1405041	1258594	27.14%	4.408%
10	12.951	1808	1813	1816	rBV	4071308	4324957	93.28%	15.146%
11	14.016	1990	1994	2005	rBV	927948	915251	19.74%	3.205%
12	15.086	2172	2176	2182	rBV	40458	51639	1.11%	0.181%
13	15.463	2235	2240	2242	rBV	49174	58478	1.26%	0.205%
14	15.498	2242	2246	2255	rBV2	424240	643202	13.87%	2.252%
15	15.892	2308	2313	2319	rBV	38983	59959	1.29%	0.210%
16	16.392	2394	2398	2407	rVB	32974	59080	1.27%	0.207%




Sum of corrected areas: 28555515

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF033122\
Data File : BF127597.D
Acq On : 31 Mar 2022 11:02
Operator : CG\JU
Sample : PB143744BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143744BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

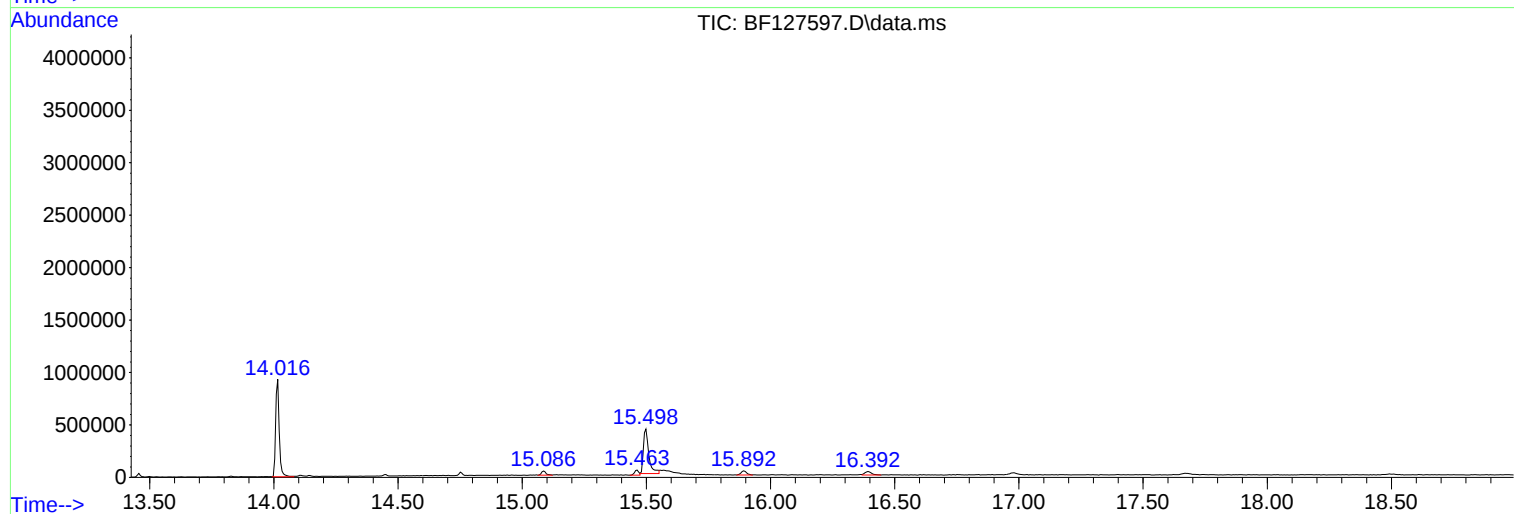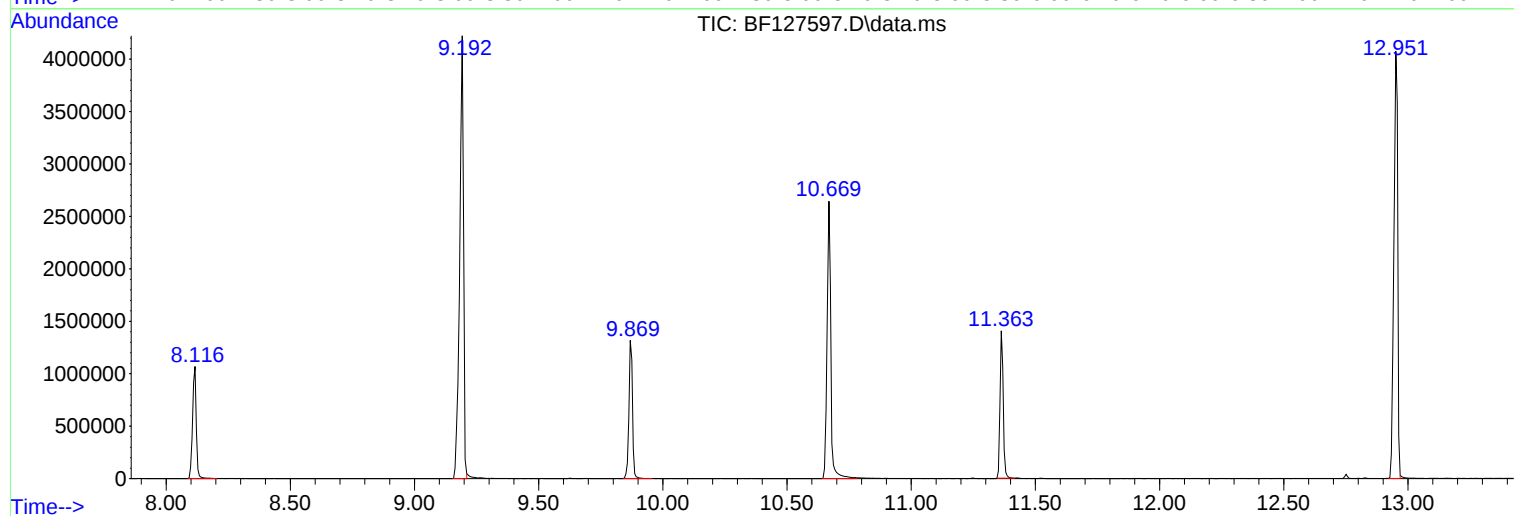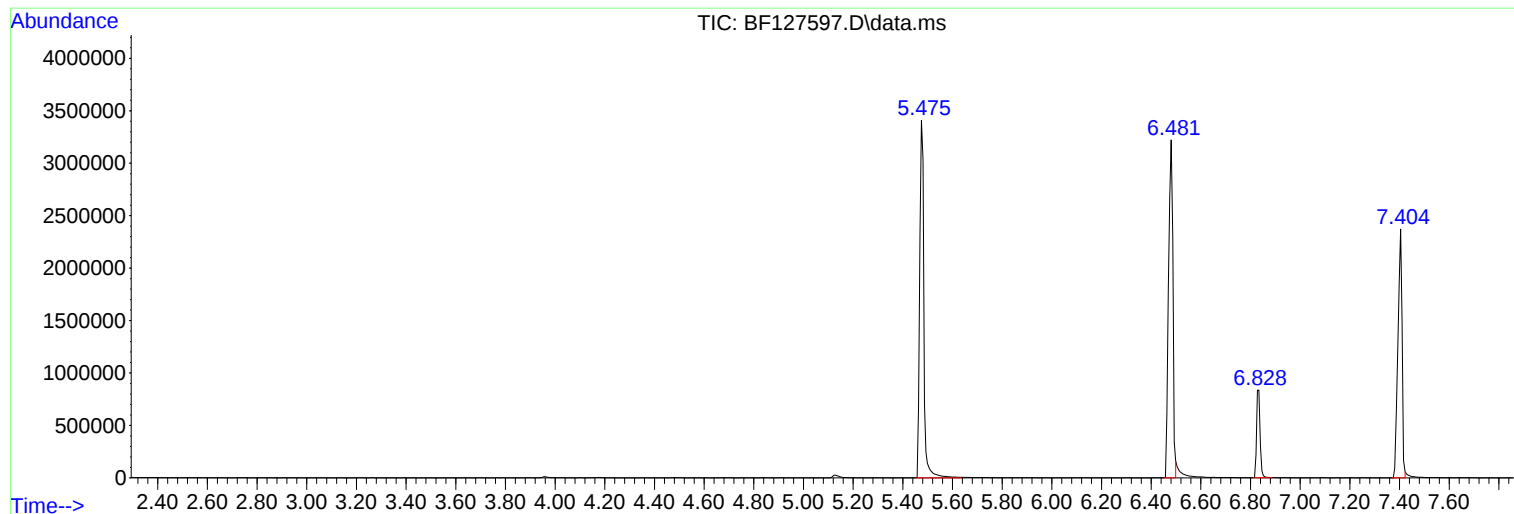

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF033122\
Data File : BF127597.D
Acq On : 31 Mar 2022 11:02
Operator : CG\JU
Sample : PB143744BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143744BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF033122\
Data File : BF127597.D
Acq On : 31 Mar 2022 11:02
Operator : CG\JU
Sample : PB143744BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143744BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------