


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF033122\
Data File : BF127595.D
Acq On : 31 Mar 2022 09:58
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Mar 29 07:13:31 2022

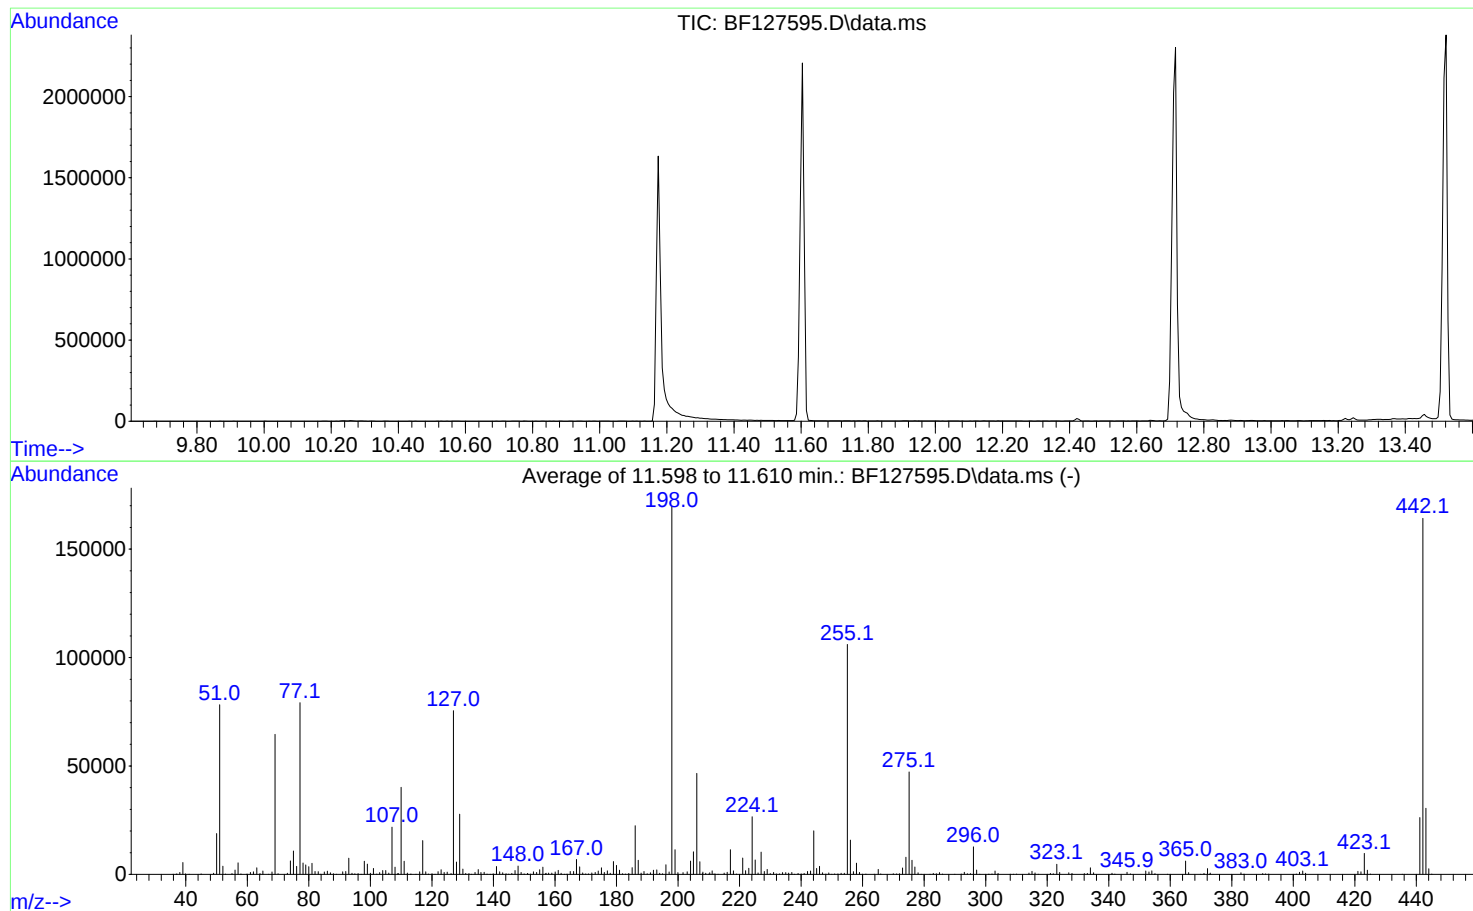




AutoFind: Scans 1583, 1584, 1585; Background Corrected with Scan 1577

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.1	78253	PASS
68	69	0.00	2	1.7	1106	PASS
69	198	0.00	100	38.1	64587	PASS
70	69	0.00	2	0.4	283	PASS
127	198	10	80	44.5	75539	PASS
197	198	0.00	2	0.7	1144	PASS
198	198	100	100	100.0	169672	PASS
199	198	5	9	6.7	11360	PASS
275	198	10	60	27.9	47256	PASS
365	198	1	100	3.6	6136	PASS
441	198	0.01	100	15.5	26231	PASS
442	442	50	100	100.0	164208	PASS
443	442	15	24	18.6	30491	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF033122\
 Data File : BF127595.D
 Acq On : 31 Mar 2022 09:58
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Apr 01 06:20:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 29 07:13:31 2022
 Response via : Initial Calibration

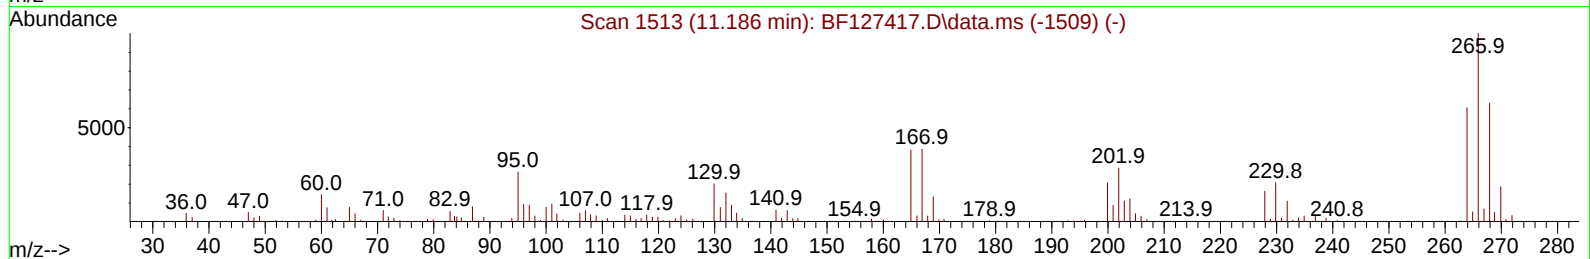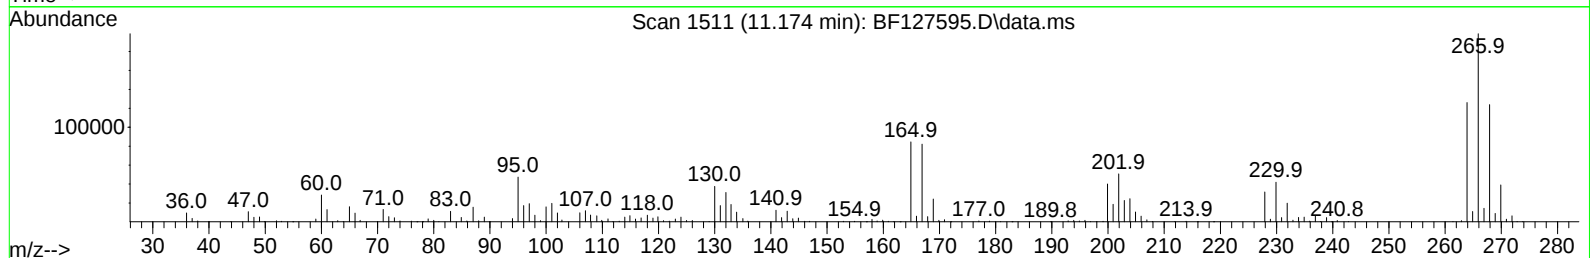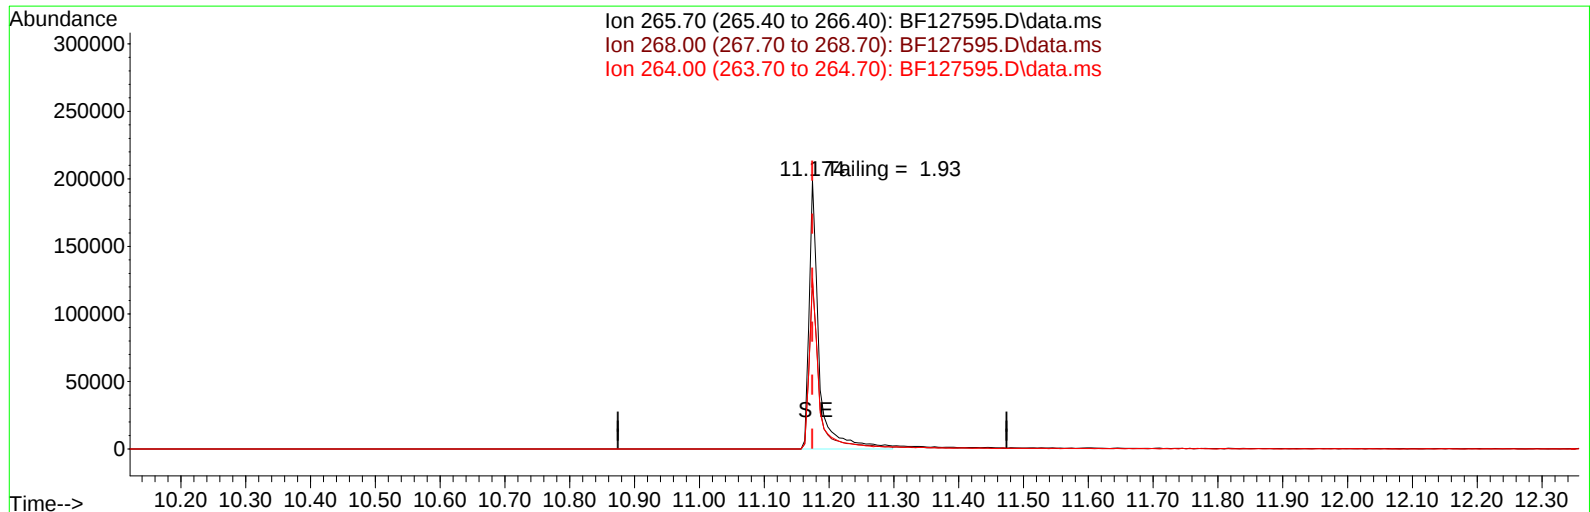

TIC: BF127595.D\data.ms

(70) Pentachlorophenol (C)

11.174min (+ 0.000) 63695.44 ng




response 217650

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	62.32
264.00	60.60	63.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF033122\
Data File : BF127595.D
Acq On : 31 Mar 2022 09:58
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 01 06:20:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 29 07:13:31 2022
Response via : Initial Calibration

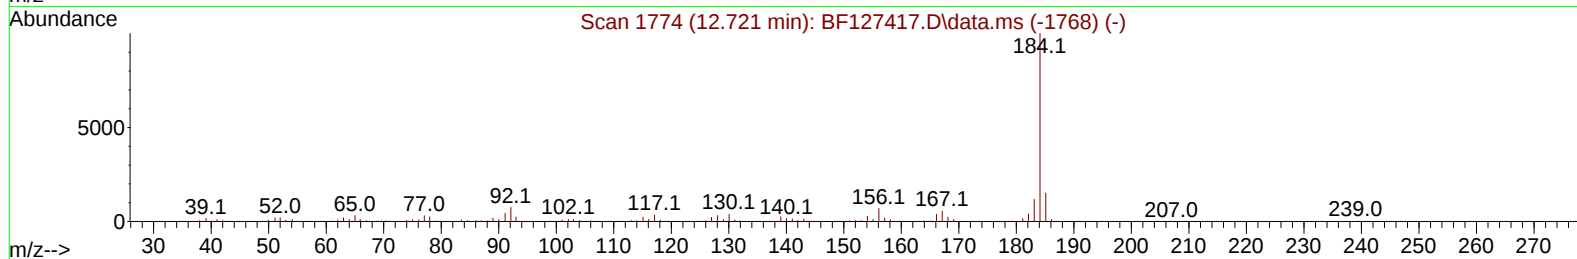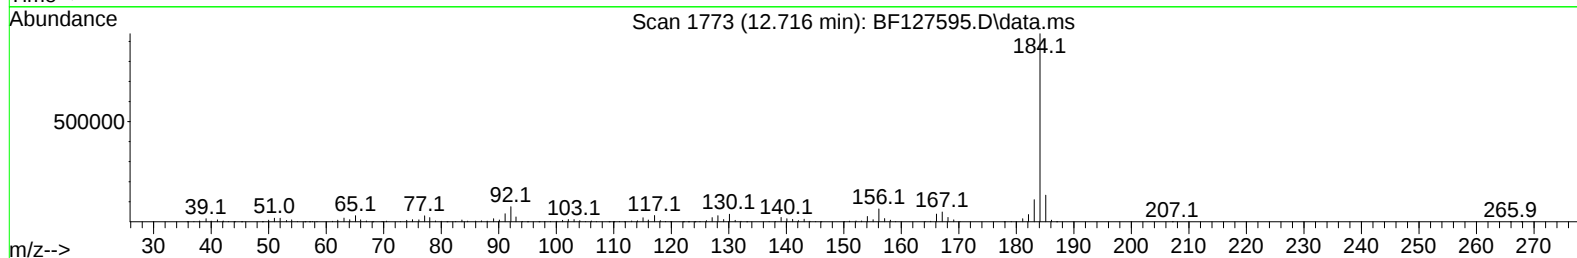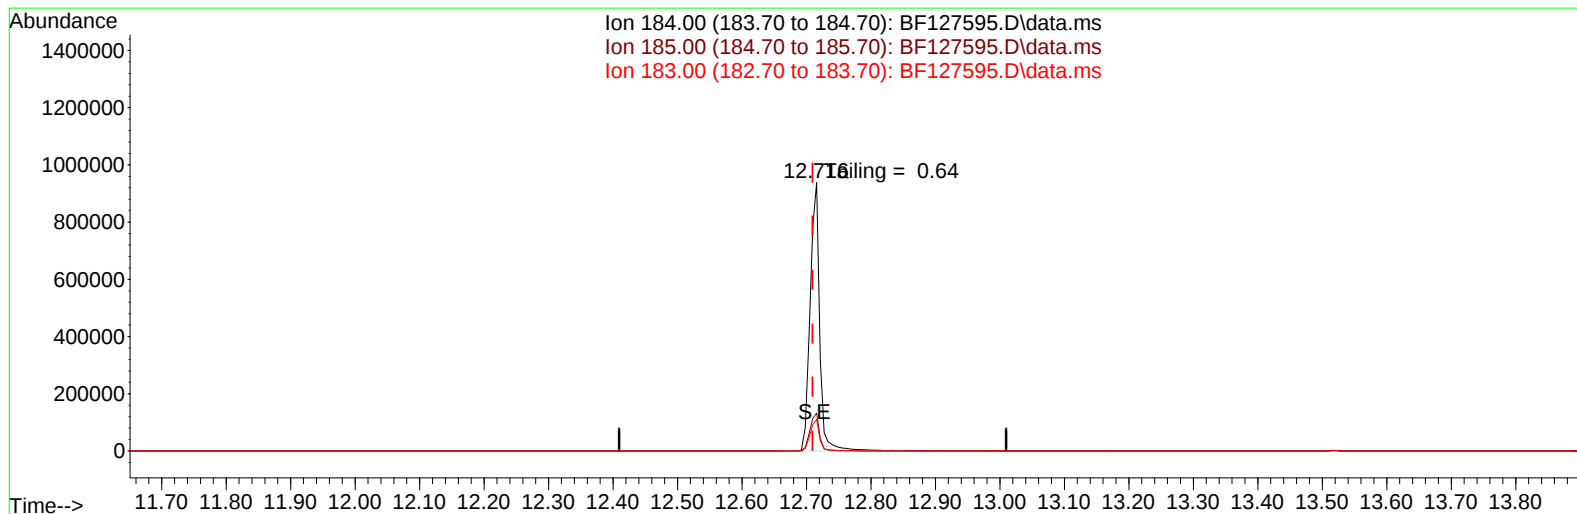

TIC: BF127595.D\data.ms

(77) Benzidine

12.716min (+ 0.006) 0.00 ng

response 971379

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.18
183.00	11.70	11.74
0.00	0.00	0.00

P

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/31/2022	BNA_F	<u>BF127595.D</u>
Compound Name	Response	Retention Time
DDT	446875	13.521
DDD	6128	13.245
DDE	674	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6802	453677	1.50

Instrument :
BNA_F
ClientSampleId :
DFTPP