
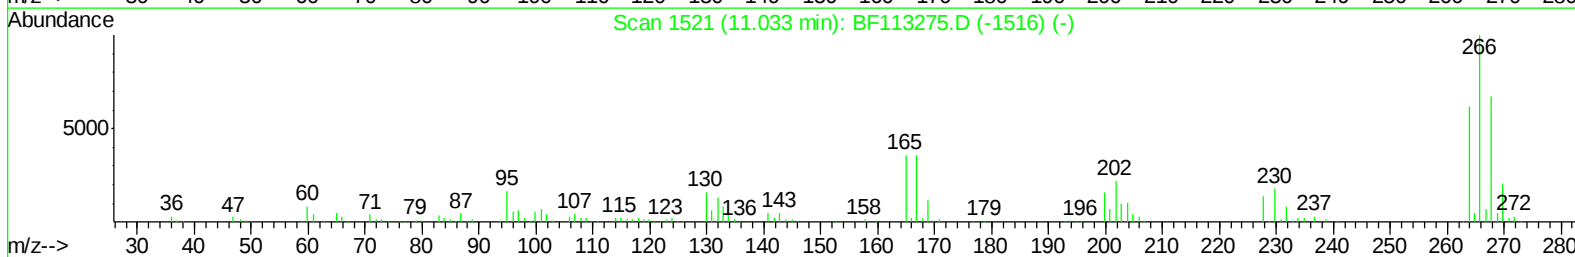
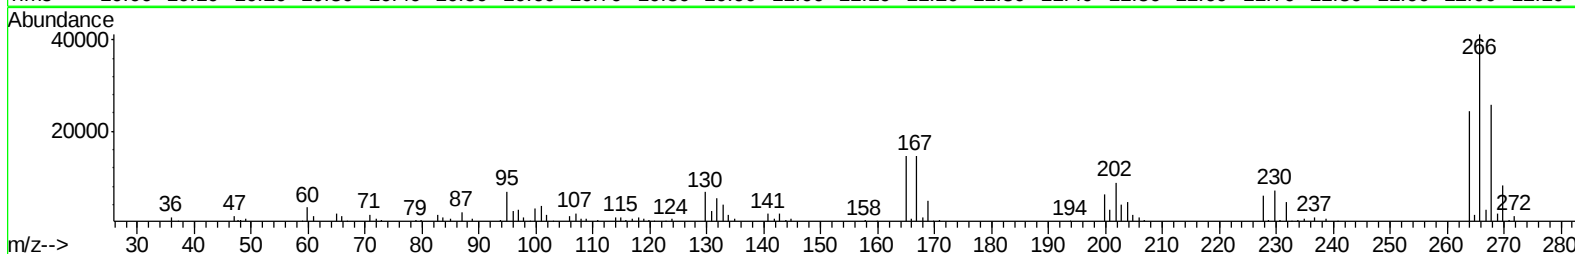


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040119\
Data File : BF113483.D
Acq On : 1 Apr 2019 23:03
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 08 02:21:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 26 03:32:08 2019
Response via : Initial Calibration

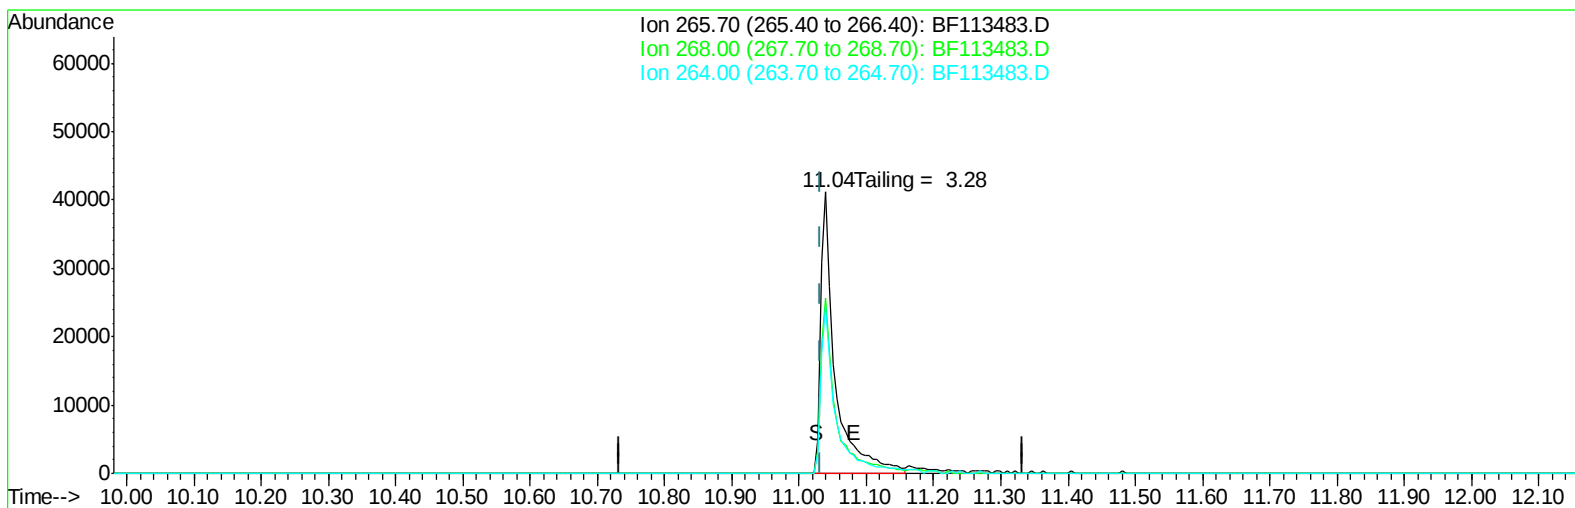

TIC: BF113483.D

(70) Pentachlorophenol (C)




11.039min (+0.006) 68382.21ng

response 62651

Ion	Exp%	Act%
265.70	100	100
268.00	67.20	62.48
264.00	61.50	58.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040119\
 Data File : BF113483.D
 Acq On : 1 Apr 2019 23:03
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 08 02:21:14 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 26 03:32:08 2019
 Response via : Initial Calibration

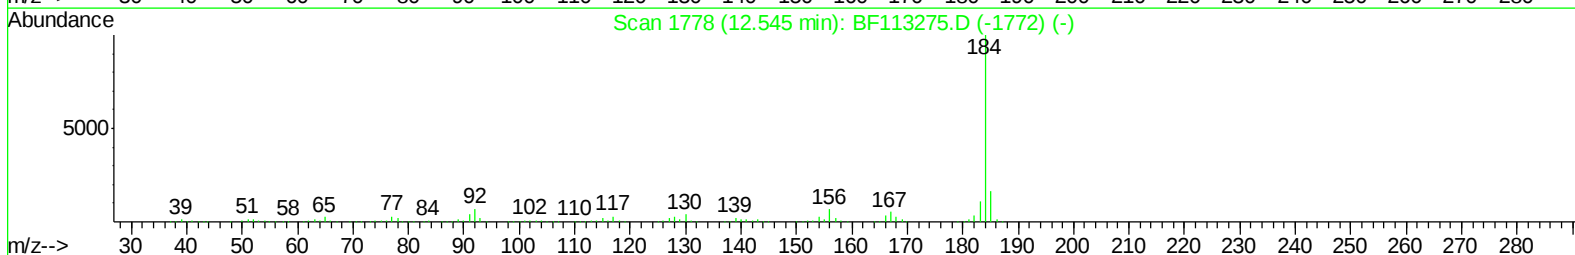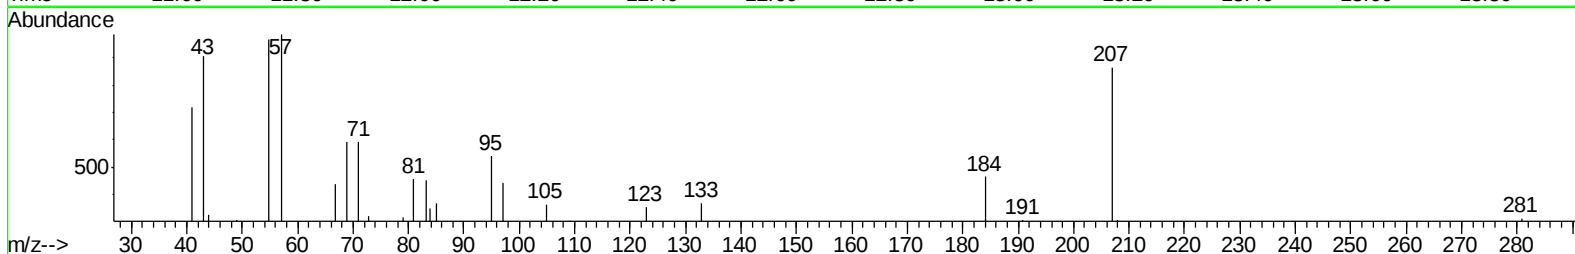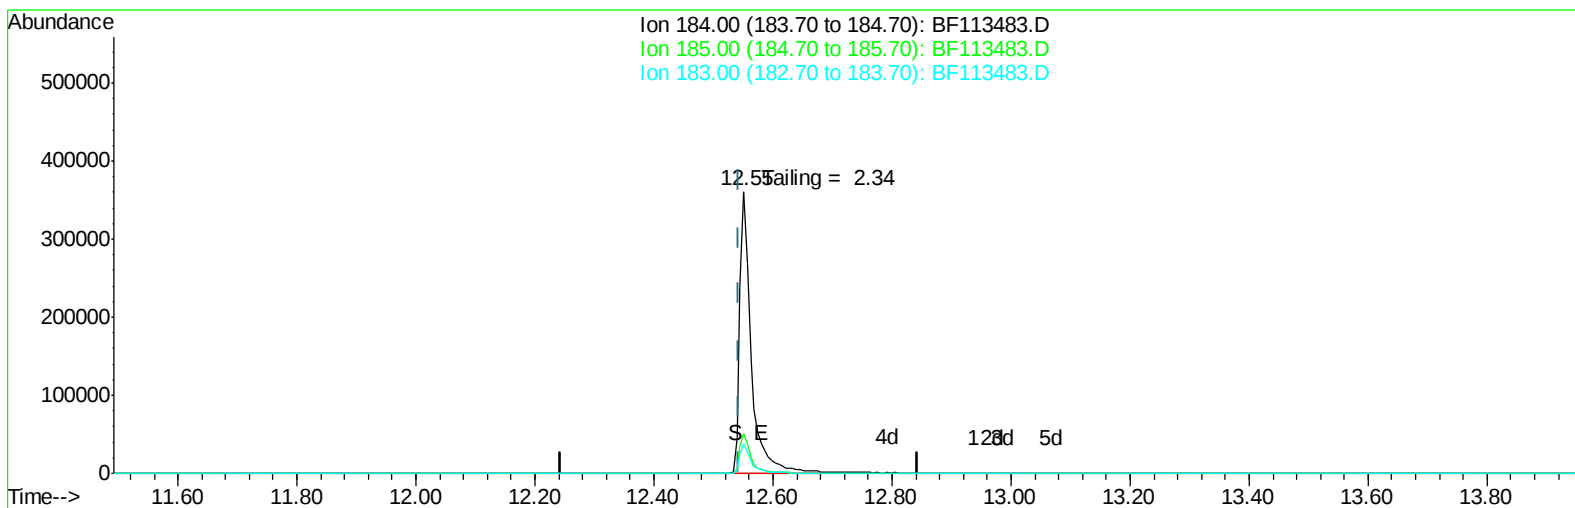

TIC: BF113483.D

(77) Benzidine

12.939min (+0.395) 126.55ng

response 567

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	0.00#
183.00	11.20	0.00#
0.00	0.00	0.00