


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040119\
 Data File : BF113458.D
 Acq On : 1 Apr 2019 11:13
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 26 03:32:08 2019

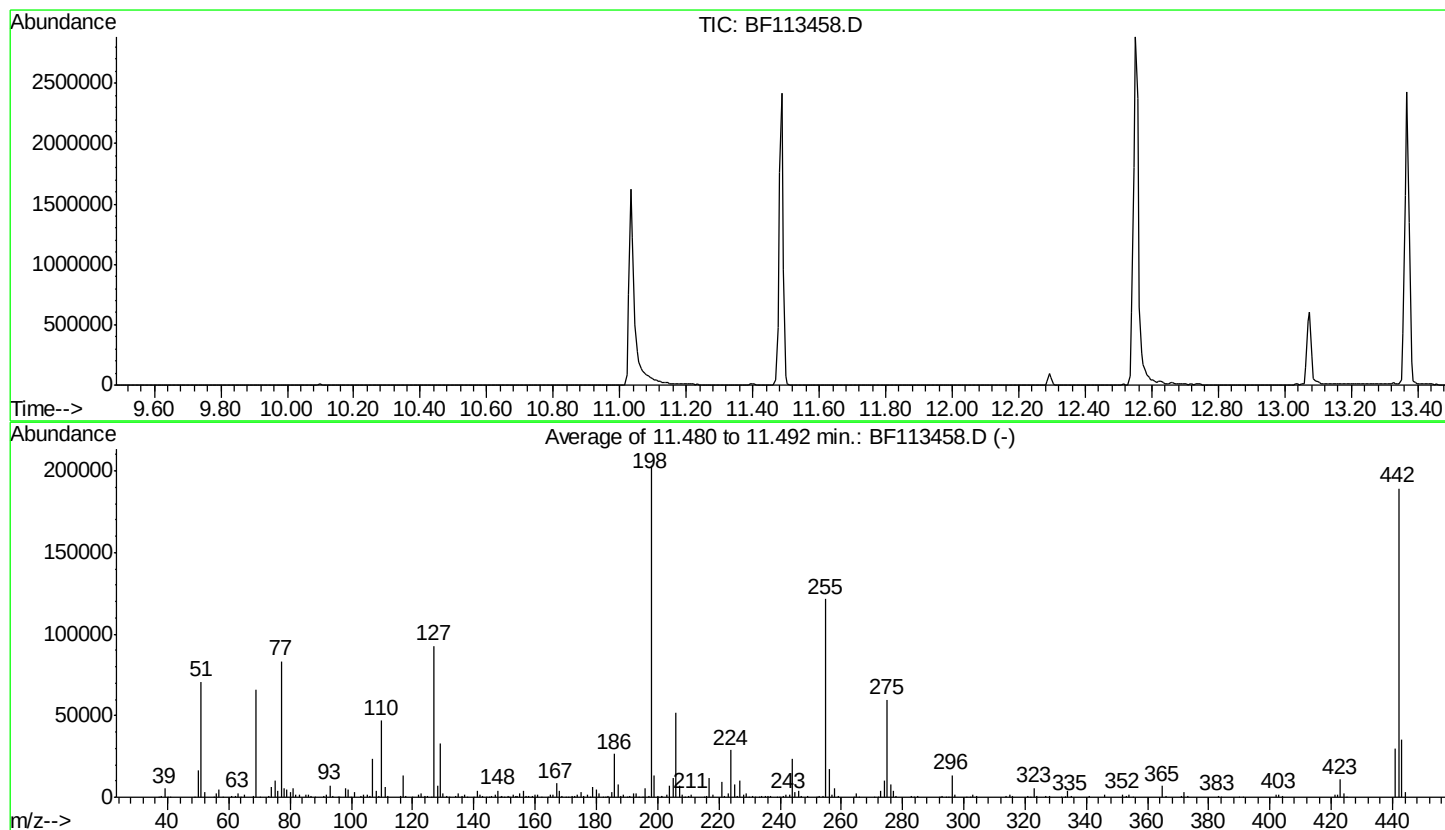

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	70968	PASS
68	69	0.00	2	1.8	1169	PASS
69	198	0.00	100	32.4	65794	PASS
70	69	0.00	2	0.5	351	PASS
127	198	10	80	45.6	92714	PASS
197	198	0.00	2	0.5	1053	PASS
198	198	100	100	100.0	203192	PASS
199	198	5	9	6.7	13525	PASS
275	198	10	60	29.4	59768	PASS
365	198	1	100	3.4	6973	PASS
441	198	0.01	100	14.6	29640	PASS
442	198	50	100	93.2	189344	PASS
443	442	15	24	18.8	35672	PASS