


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040119\
 Data File : BF113483.D
 Acq On : 1 Apr 2019 23:03
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 26 03:32:08 2019

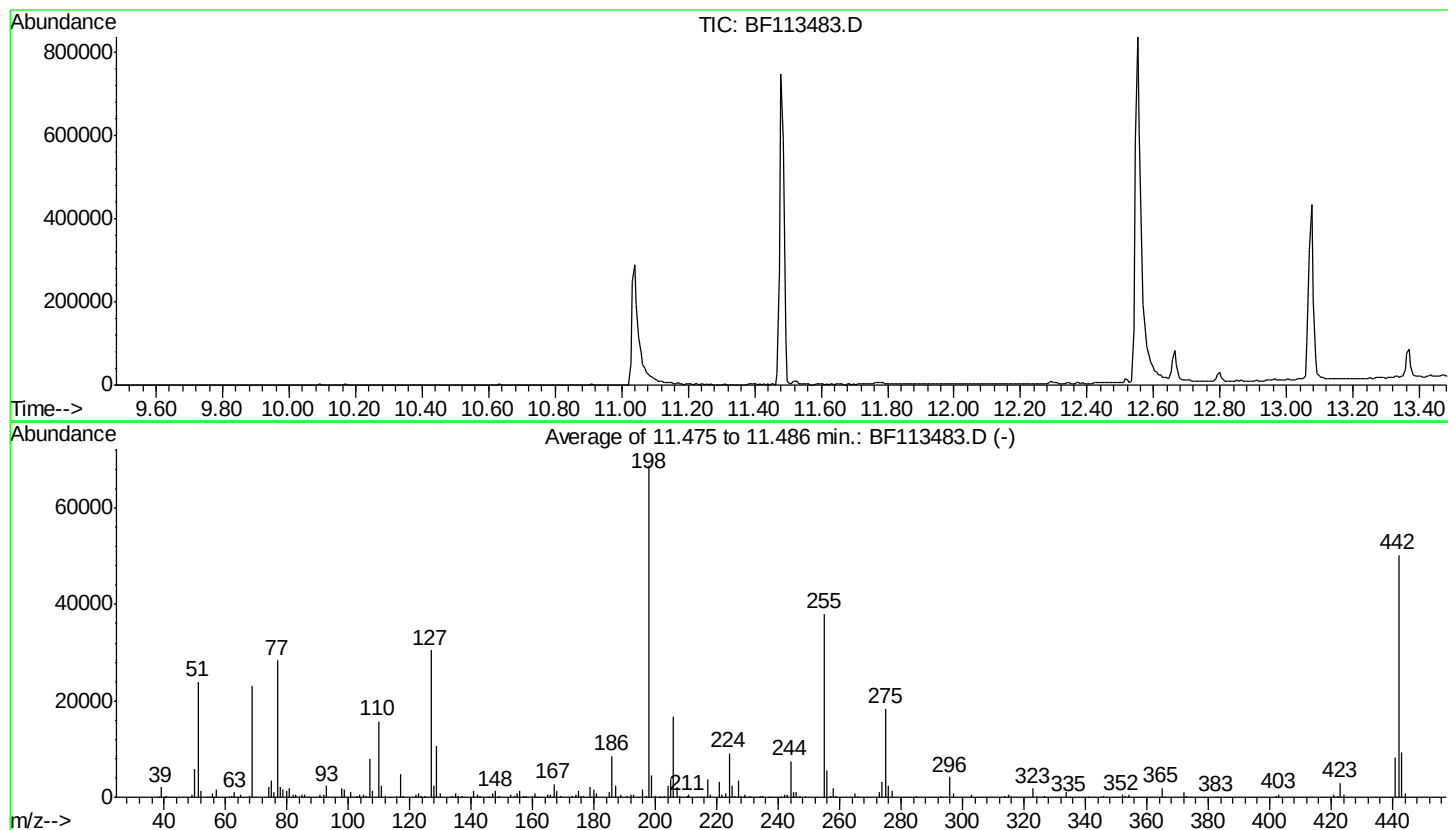

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	23984	PASS
68	69	0.00	2	1.2	275	PASS
69	198	0.00	100	33.5	23016	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.2	30440	PASS
197	198	0.00	2	0.4	302	PASS
198	198	100	100	100.0	68792	PASS
199	198	5	9	6.7	4628	PASS
275	198	10	60	26.8	18432	PASS
365	198	1	100	2.8	1899	PASS
441	198	0.01	100	11.8	8126	PASS
442	198	50	100	73.0	50214	PASS
443	442	15	24	18.6	9348	PASS