


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040120\
 Data File : BF119664.D
 Acq On : 1 Apr 2020 10:33
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 01 11:59:45 2020

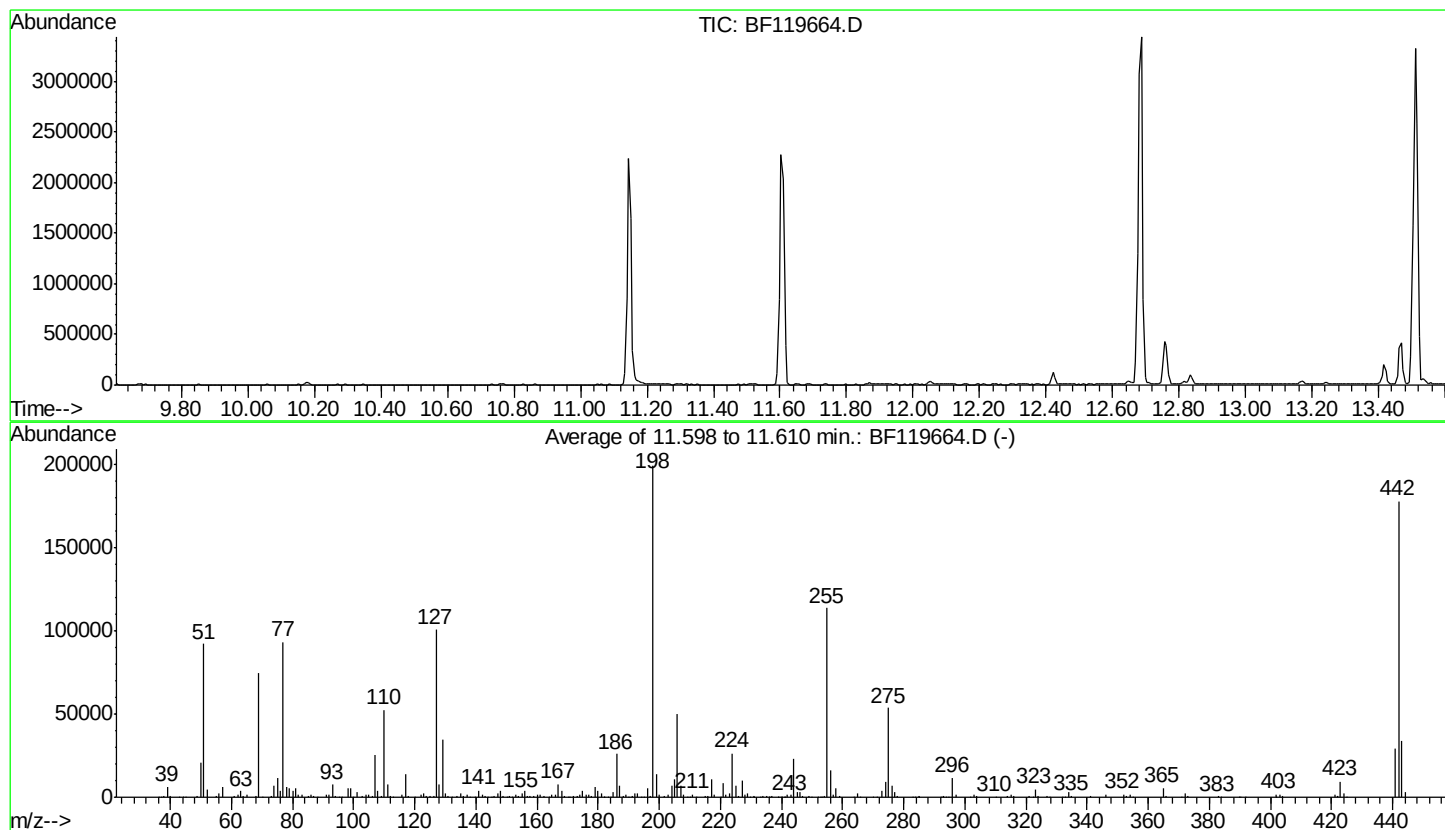

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.3	92191	PASS
68	69	0.00	2	1.6	1162	PASS
69	198	0.00	100	37.3	74213	PASS
70	69	0.00	2	0.4	316	PASS
127	198	10	80	50.6	100629	PASS
197	198	0.00	2	0.4	773	PASS
198	198	100	100	100.0	199002	PASS
199	198	5	9	6.8	13576	PASS
275	198	10	60	26.9	53520	PASS
365	198	1	100	2.7	5440	PASS
441	198	0.01	100	14.7	29280	PASS
442	198	50	100	89.2	177488	PASS
443	442	15	24	18.9	33610	PASS