


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040120\
 Data File : BF119684.D
 Acq On : 1 Apr 2020 22:35
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 01 11:59:45 2020

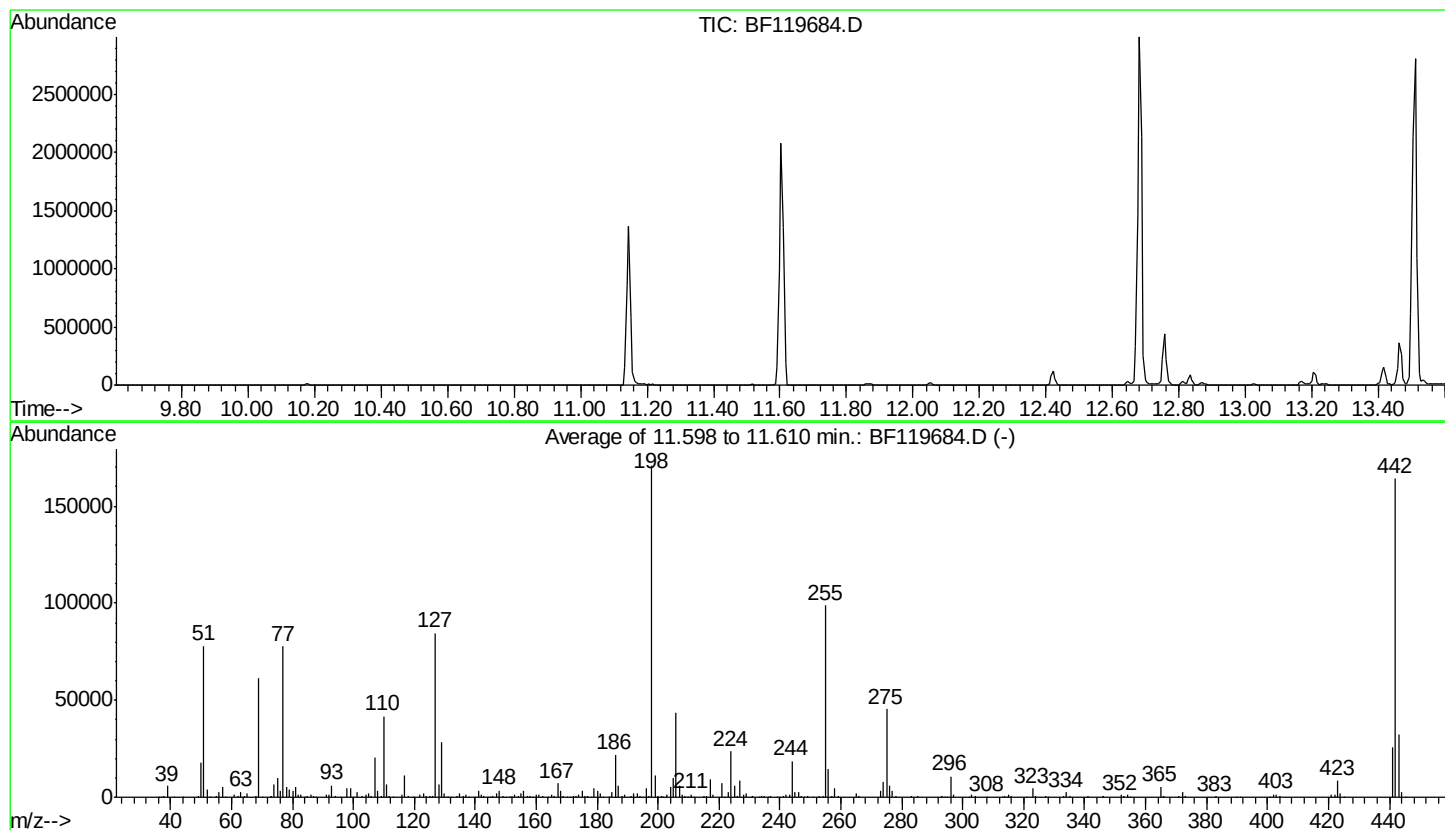

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.6	77920	PASS
68	69	0.00	2	1.5	946	PASS
69	198	0.00	100	35.8	61122	PASS
70	69	0.00	2	0.4	257	PASS
127	198	10	80	49.5	84629	PASS
197	198	0.00	2	0.5	806	PASS
198	198	100	100	100.0	170805	PASS
199	198	5	9	6.7	11524	PASS
275	198	10	60	26.6	45352	PASS
365	198	1	100	3.1	5323	PASS
441	198	0.01	100	15.1	25761	PASS
442	198	50	100	96.0	163984	PASS
443	442	15	24	19.5	32000	PASS