

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040219\
 Data File : BF113527.D
 Acq On : 3 Apr 2019 2:45
 Operator : JU/SJ
 Sample : K2170-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OIL-WATER-SEPERATOR-2

Quant Time: Apr 03 08:20:13 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 26 03:32:08 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.69	152	129909	20.00	ng	-0.01
21) Naphthalene-d8	7.97	136	446969	20.00	ng	-0.01
39) Acenaphthene-d10	9.72	164	185301	20.00	ng	-0.02
64) Phenanthrene-d10	11.20	188	352058	20.00	ng	-0.02
76) Chrysene-d12	13.83	240	330180	20.00	ng	-0.01
87) Perylene-d12	15.24	264	238705	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.32	112	789450	99.37	ng	0.00
7) Phenol-d6	6.35	99	907861	90.33	ng	-0.01
23) Nitrobenzene-d5	7.26	82	678502	90.10	ng	-0.01
42) 2,4,6-Tribromophenol	10.51	330	269462	117.73	ng	-0.02
45) 2-Fluorobiphenyl	9.05	172	1158557	101.40	ng	-0.02
79) Terphenyl-d14	12.79	244	1087528	72.60	ng	-0.01
Target Compounds						
10) Phenol	6.36	94	47989	4.182	ng	91
15) Benzyl Alcohol	6.86	79	1024084	154.447	ng	97
19) n-Nitroso-di-n-propylamine	7.11	70	34761	5.506	ng	# 77
20) 3+4-Methylphenols	7.12	107	151365	12.882	ng	# 81
32) Benzoic acid	7.92	122	1432975	297.939	ng	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040219\
Data File : BF113527.D
Acq On : 3 Apr 2019 2:45
Operator : JU/SJ
Sample : K2170-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OIL-WATER-SEPERATOR-2

Quant Time: Apr 03 08:20:13 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 26 03:32:08 2019
Response via : Initial Calibration

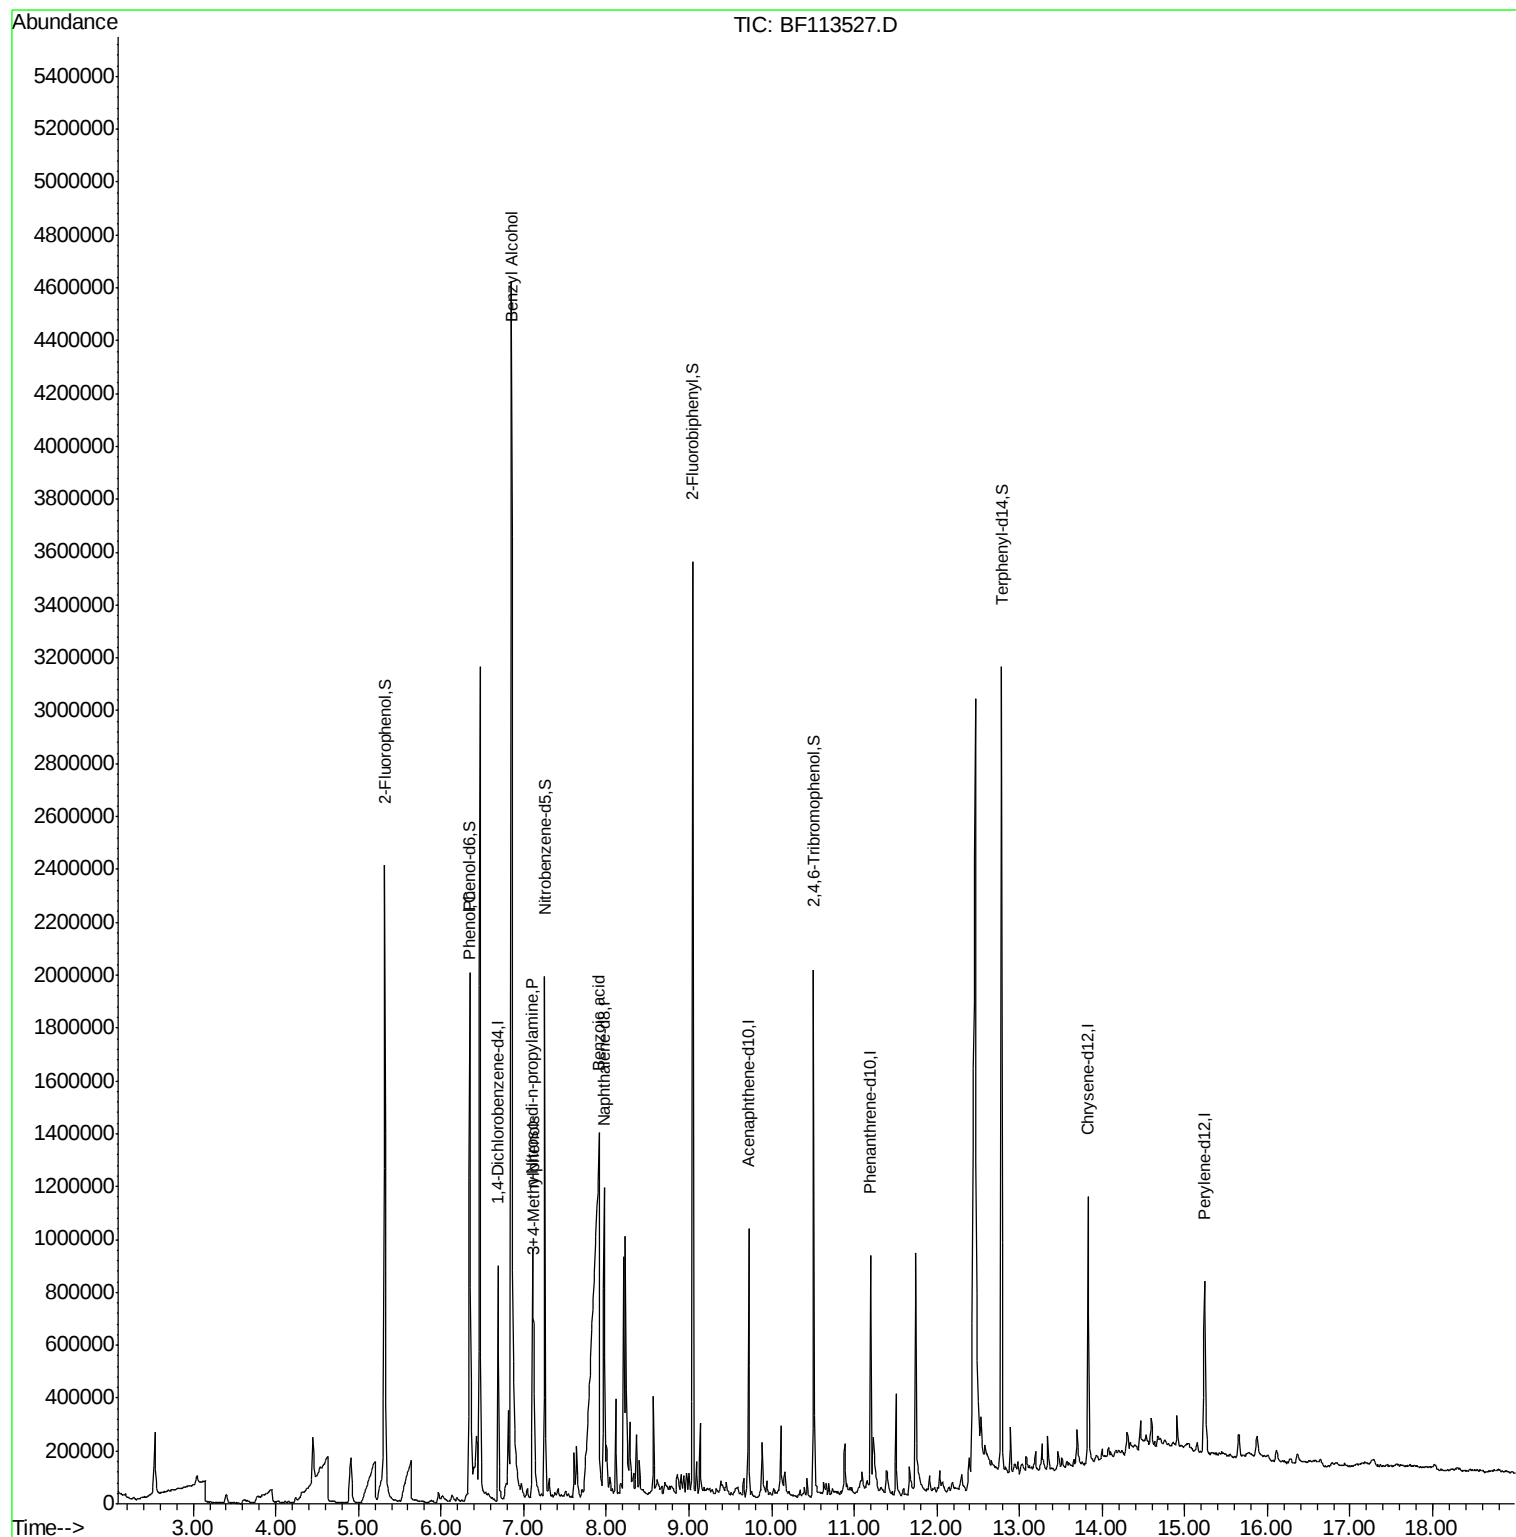




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.69 min Scan# 783
Delta R.T. -0.01 min
Lab File: BF113527.D
Acq: 3 Apr 2019 2:45

Instrument :
BNA_F
ClientSampleId :
OIL-WATER-SEPERATOR-2

Tgt Ion:152 Resp: 129909
Ion Ratio Lower Upper
152 100
150 157.7 124.7 187.1
115 58.9 46.0 69.0

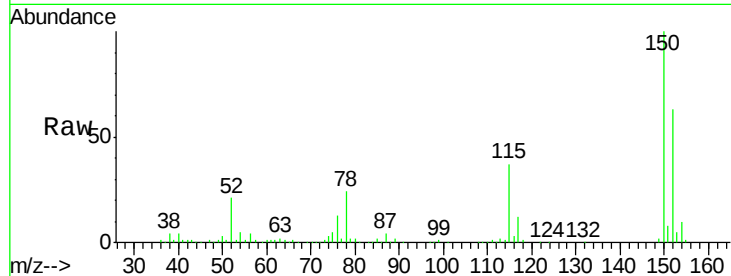


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

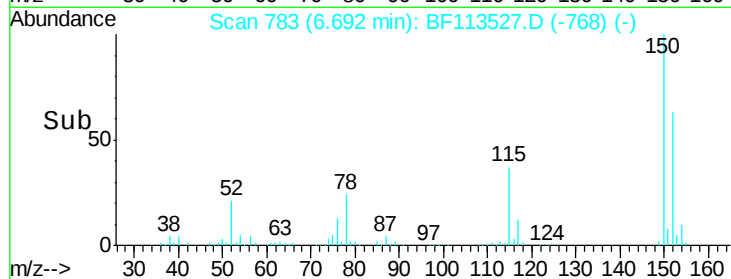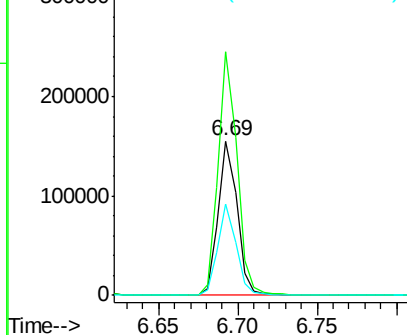



#5


2-Fluorophenol
Concen: 99.365 ng
RT: 5.32 min Scan# 550
Delta R.T. 0.01 min
Lab File: BF113527.D
Acq: 3 Apr 2019 2:45

Tgt Ion:112 Resp: 789450
Ion Ratio Lower Upper
112 100
64 58.9 49.2 73.8
63 29.8 24.9 37.3

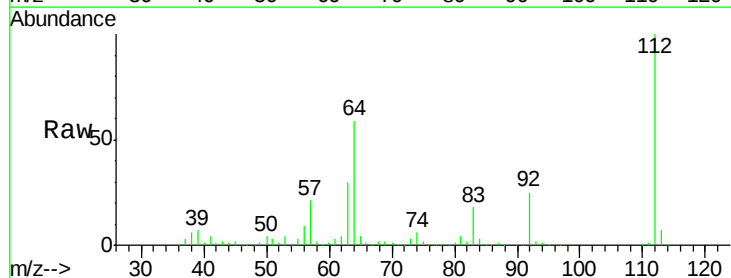

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

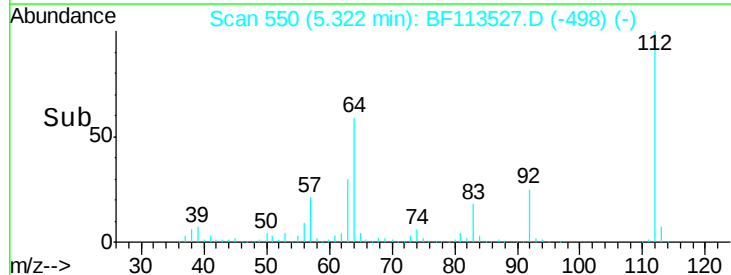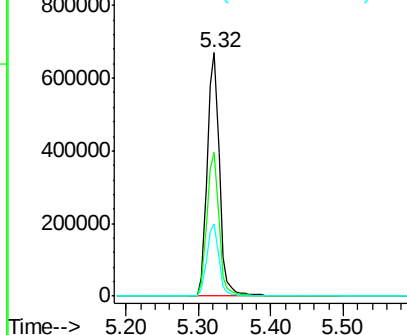

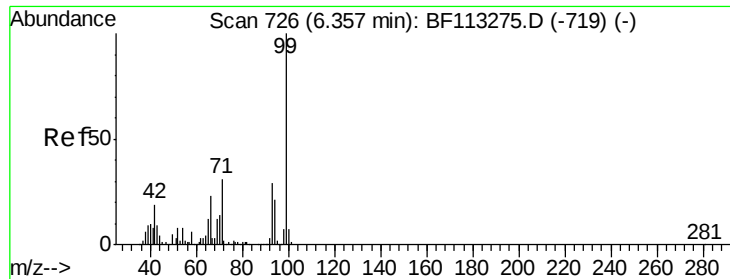

#7

Phenol-d6

Concen: 90.328 ng

RT: 6.35 min Scan# 724

Delta R.T. -0.01 min

Lab File: BF113527.D

Acq: 3 Apr 2019 2:45

Instrument :

BNA_F

ClientSampleId :

OIL-WATER-SEPARATOR-2


Tgt Ion: 99 Resp: 907861

Ion Ratio Lower Upper




99 100

42 18.3 14.8 22.2

71 31.8 24.9 37.3



Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

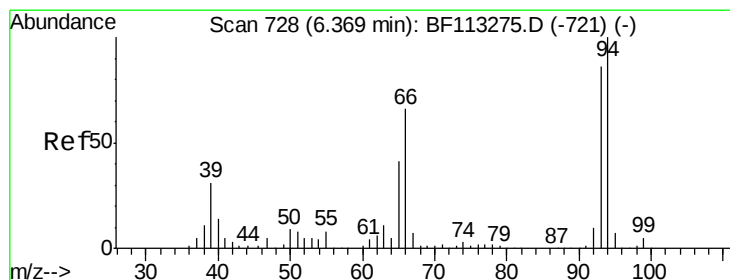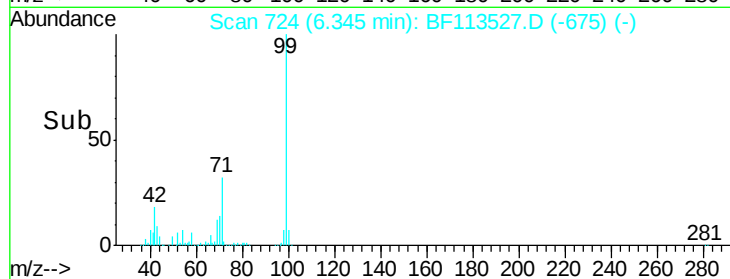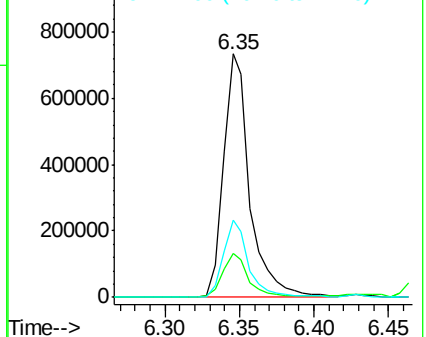

#10

Phenol

Concen: 4.182 ng

RT: 6.36 min Scan# 726

Delta R.T. -0.01 min

Lab File: BF113527.D

Acq: 3 Apr 2019 2:45


Tgt Ion: 94 Resp: 47989

Ion Ratio Lower Upper



94 100


65 33.4 21.4 61.4

66 71.9 46.4 86.4

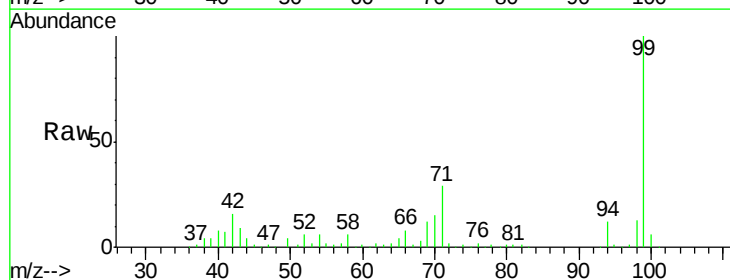

Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1

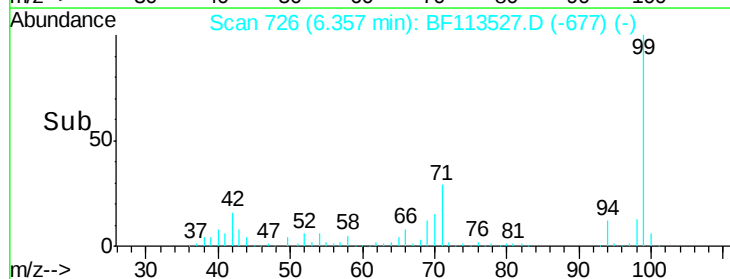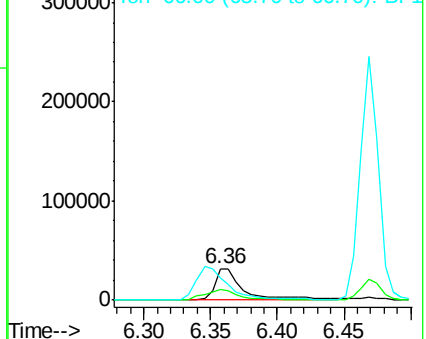

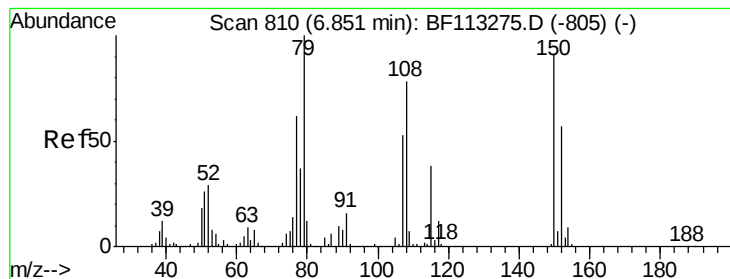

#15

Benzyl Alcohol

Concen: 154.447 ng

RT: 6.86 min Scan# 812

Delta R.T. 0.01 min

Lab File: BF113527.D

Acq: 3 Apr 2019 2:45

Instrument :

BNA_F

ClientSampleId :

OIL-WATER-SEPARATOR-2


Tgt Ion: 79 Resp: 1024084

Ion Ratio Lower Upper

79 100

108 82.1 62.0 93.0




77 62.5 49.9 74.9



Abundance Ion 79.00 (78.70 to 79.70): BF1

Ion 108.00 (107.70 to 108.70): BF1

Ion 77.00 (76.70 to 77.70): BF1

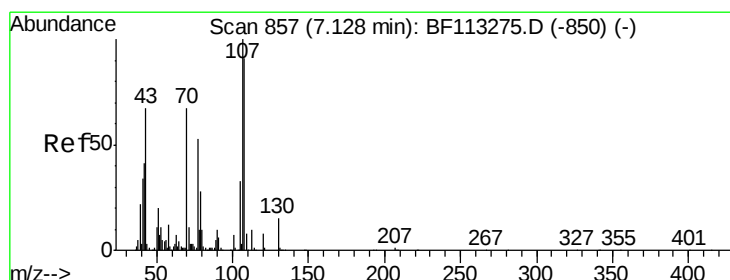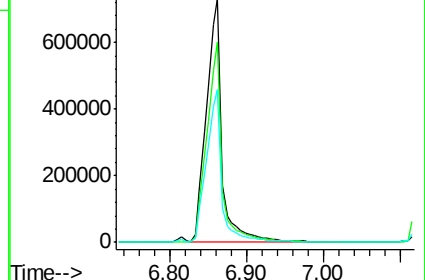

#19

n-Nitroso-di-n-propylamine

Concen: 5.506 ng

RT: 7.11 min Scan# 854

Delta R.T. -0.02 min

Lab File: BF113527.D

Acq: 3 Apr 2019 2:45

Tgt Ion: 70 Resp: 34761


Ion Ratio Lower Upper

70 100

42 47.2 48.4 72.6#

101 8.2 7.8 11.8

130 0.0 18.2 27.4#






Abundance Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): BF1

Ion 130.00 (129.70 to 130.70): BF1

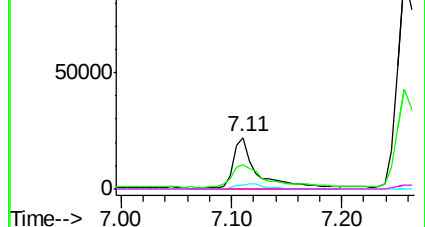



#20

3+4-Methylphenols

Concen: 12.882 ng

RT: 7.12 min Scan# 856

Delta R.T. -0.01 min

Lab File: BF113527.D

Acq: 3 Apr 2019 2:45

Instrument :

BNA_F

ClientSampleId :

OIL-WATER-SEPARATOR-2

Tgt Ion:107 Resp: 151365


Ion Ratio Lower Upper

107 100

108 82.4 71.4 111.4

77 27.8 33.5 73.5#

79 19.7 8.3 48.3



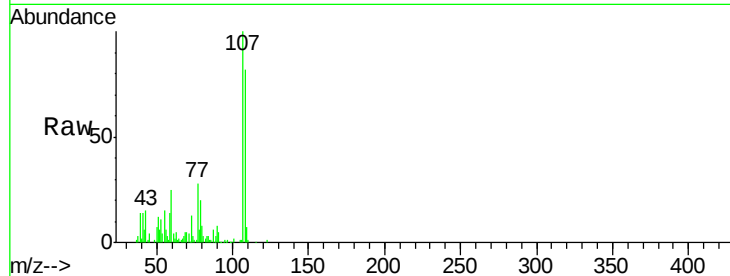


Abundance Ion 107.00 (106.70 to 107.70): E

Ion 108.00 (107.70 to 108.70): E

Ion 77.00 (76.70 to 77.70): BF1

Ion 79.00 (78.70 to 79.70): BF1

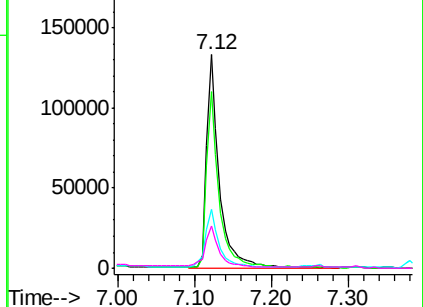

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.97 min Scan# 1001

Delta R.T. -0.01 min

Lab File: BF113527.D

Acq: 3 Apr 2019 2:45

Tgt Ion:136 Resp: 446969


Ion Ratio Lower Upper

136 100

137 10.9 8.9 13.3

54 7.6 7.0 10.6

68 5.7 4.8 7.2


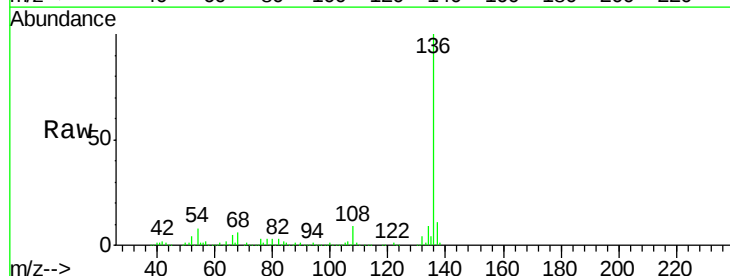



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

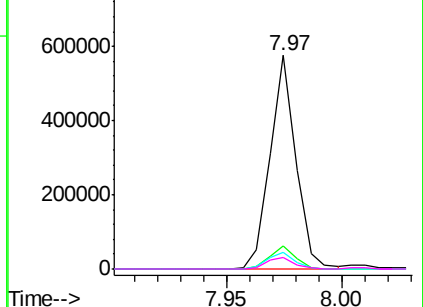







#23
Nitrobenzene-d5
Concen: 90.100 ng
RT: 7.26 min Scan# 879
Delta R.T. -0.01 min
Lab File: BF113527.D
Acq: 3 Apr 2019 2:45

Instrument :
BNA_F
ClientSampleId :
OIL-WATER-SEPERATOR-2

Tgt Ion: 82 Resp: 678502
Ion Ratio Lower Upper
82 100
128 46.1 36.5 54.7
54 52.5 42.2 63.2

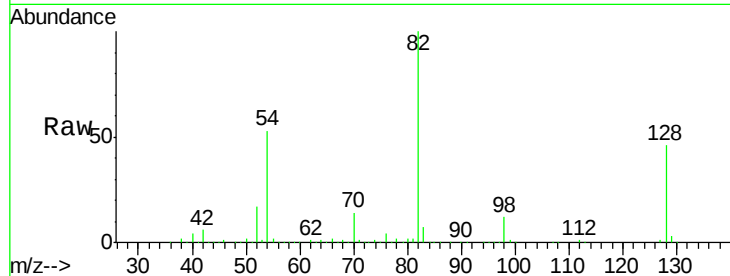


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): BF1
Ion 54.00 (53.70 to 54.70): BF1


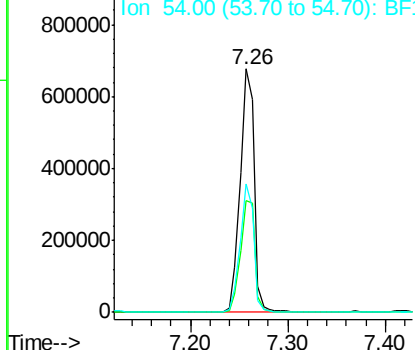



#32
Benzoic acid
Concen: 297.939 ng
RT: 7.92 min Scan# 991
Delta R.T. 0.12 min
Lab File: BF113527.D
Acq: 3 Apr 2019 2:45

Tgt Ion: 122 Resp: 1432975
Ion Ratio Lower Upper
122 100
105 120.1 100.4 140.4
77 88.7 69.0 109.0



Abundance Ion 122.00 (121.70 to 122.70): BF1
Ion 105.00 (104.70 to 105.70): BF1
Ion 77.00 (76.70 to 77.70): BF1

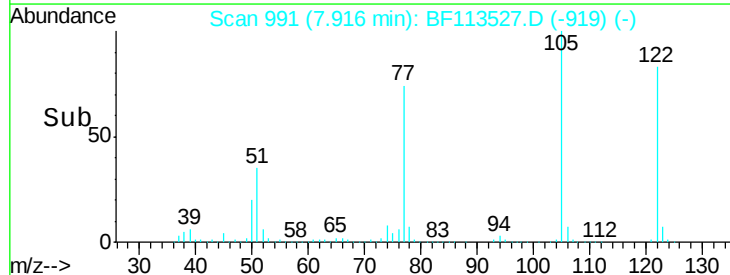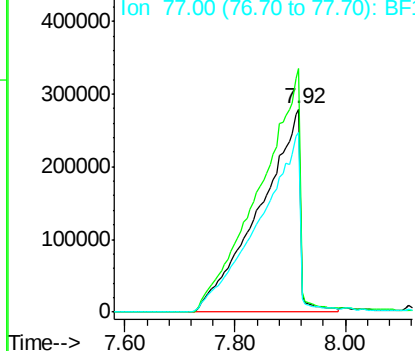

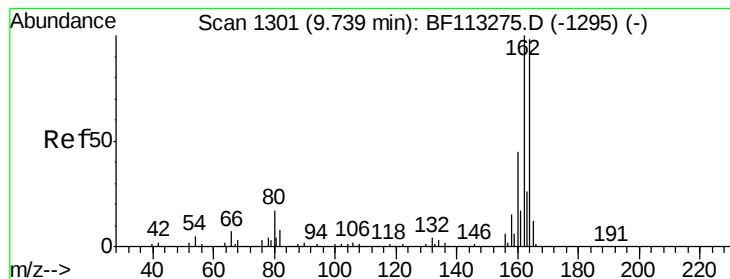

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.72 min Scan# 1298

Delta R.T. -0.02 min

Lab File: BF113527.D

Acq: 3 Apr 2019 2:45

Instrument :

BNA_F

ClientSampleId :

OIL-WATER-SEPARATOR-2


Tgt Ion:164 Resp: 185301

Ion Ratio Lower Upper

164 100

162 102.0 81.8 122.6




160 45.1 36.4 54.6



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

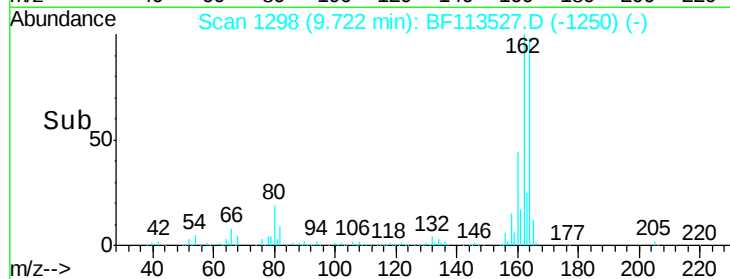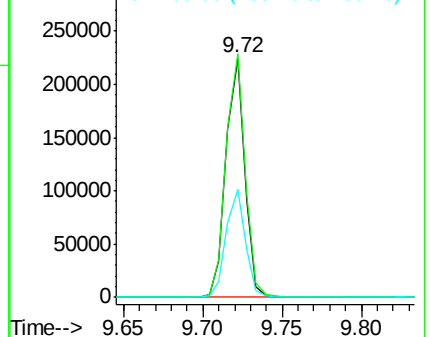

#42

2,4,6-Tribromophenol

Concen: 117.726 ng

RT: 10.51 min Scan# 1432

Delta R.T. -0.02 min

Lab File: BF113527.D

Acq: 3 Apr 2019 2:45


Tgt Ion:330 Resp: 269462

Ion Ratio Lower Upper

330 100

332 96.0 77.8 116.6



141 28.0 22.7 34.1




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



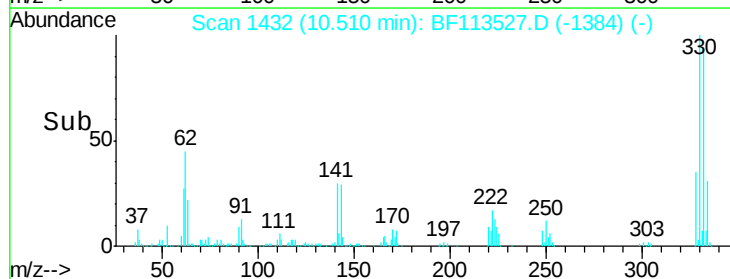
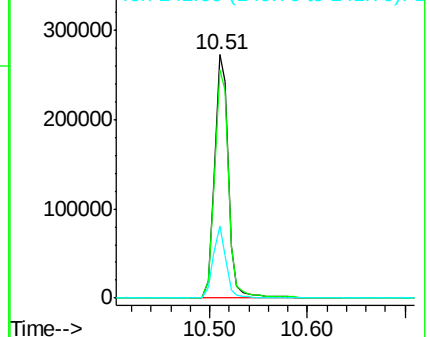


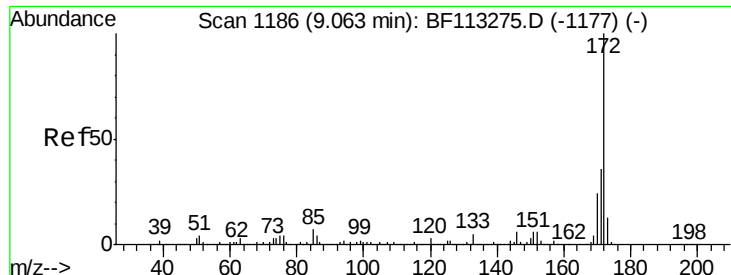

#45
 2-Fluorobiphenyl
 Concen: 101.399 ng
 RT: 9.05 min Scan# 1183
 Delta R.T. -0.02 min
 Lab File: BF113527.D
 Acq: 3 Apr 2019 2:45




Instrument :
 BNA_F
 ClientSampleId :
 OIL-WATER-SEPERATOR-2


Tgt Ion:172 Resp: 1158557
 Ion Ratio Lower Upper
 172 100
 171 35.9 29.0 43.6
 170 24.1 19.5 29.3

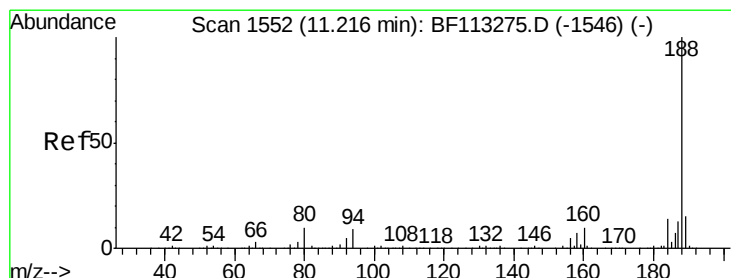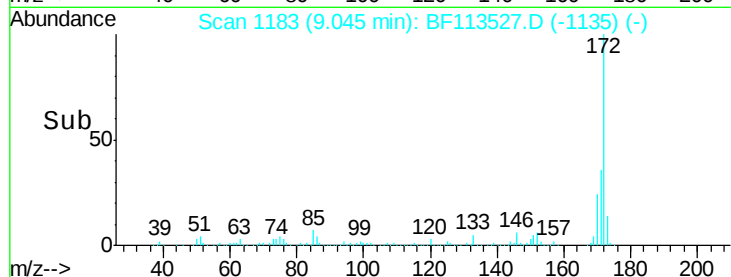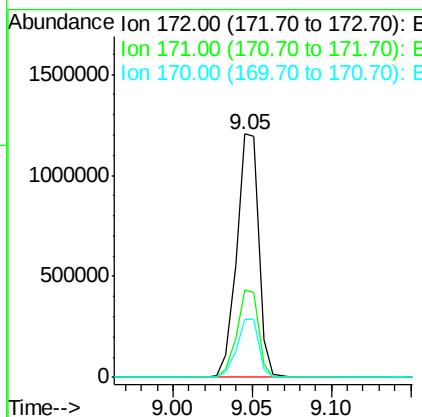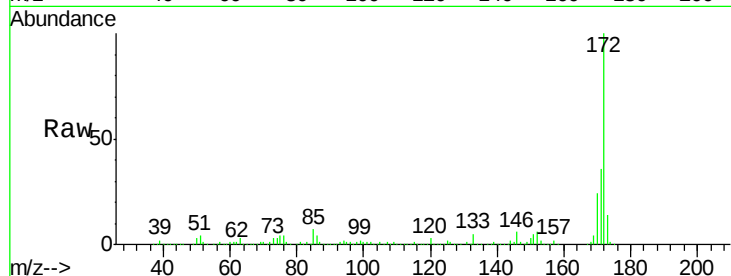

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.20 min Scan# 1549
 Delta R.T. -0.02 min
 Lab File: BF113527.D
 Acq: 3 Apr 2019 2:45

Tgt Ion:188 Resp: 352058
 Ion Ratio Lower Upper
 188 100
 94 9.9 7.0 10.6
 80 10.4 7.7 11.5

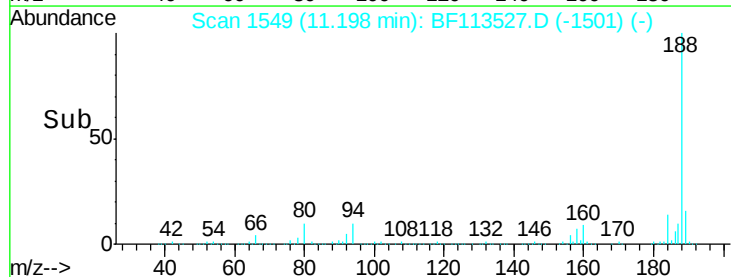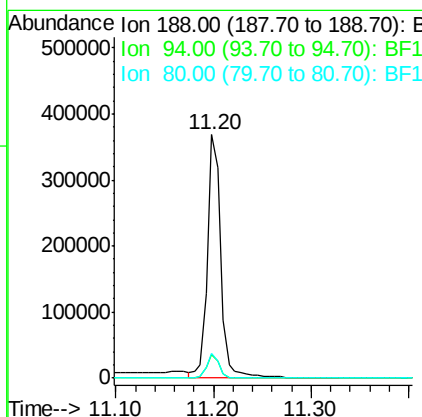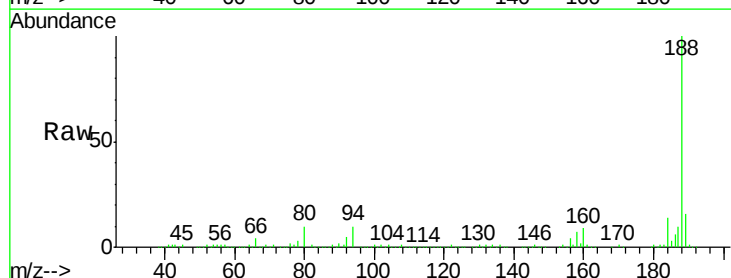



#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.83 min Scan# 1997

Delta R.T. -0.01 min

Lab File: BF113527.D

Acq: 3 Apr 2019 2:45

Instrument :

BNA_F

ClientSampleId :

OIL-WATER-SEPARATOR-2


Tgt Ion:240 Resp: 330180

Ion Ratio Lower Upper

240 100

120 10.9 8.8 13.2




236 25.4 20.9 31.3



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

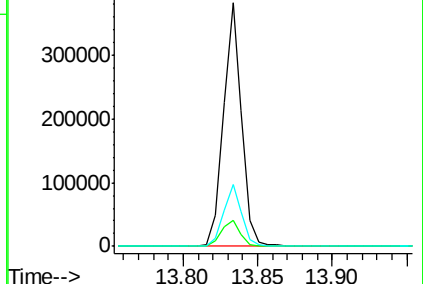

#79

Terphenyl-d14

Concen: 72.600 ng

RT: 12.79 min Scan# 1819

Delta R.T. -0.01 min

Lab File: BF113527.D

Acq: 3 Apr 2019 2:45


Tgt Ion:244 Resp: 1087528

Ion Ratio Lower Upper

244 100

212 6.6 5.5 8.3



122 10.1 8.6 13.0




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

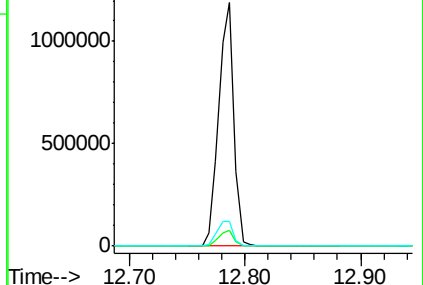

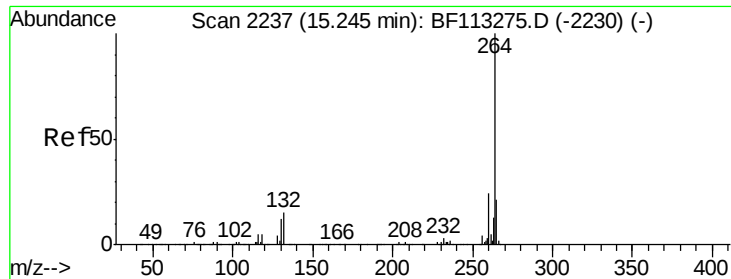

#87
Perylene-d12
Concen: 20.000 ng
RT: 15.24 min Scan# 2236
Delta R.T. -0.01 min
Lab File: BF113527.D
Acq: 3 Apr 2019 2:45

Instrument :
BNA_F
ClientSampleId :
OIL-WATER-SEPERATOR-2

Tgt Ion: 264 Resp: 238705
Ion Ratio Lower Upper
264 100
260 23.5 19.1 28.7
265 21.5 17.1 25.7

