


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040219\
 Data File : BF113500.D
 Acq On : 2 Apr 2019 12:32
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 26 03:32:08 2019

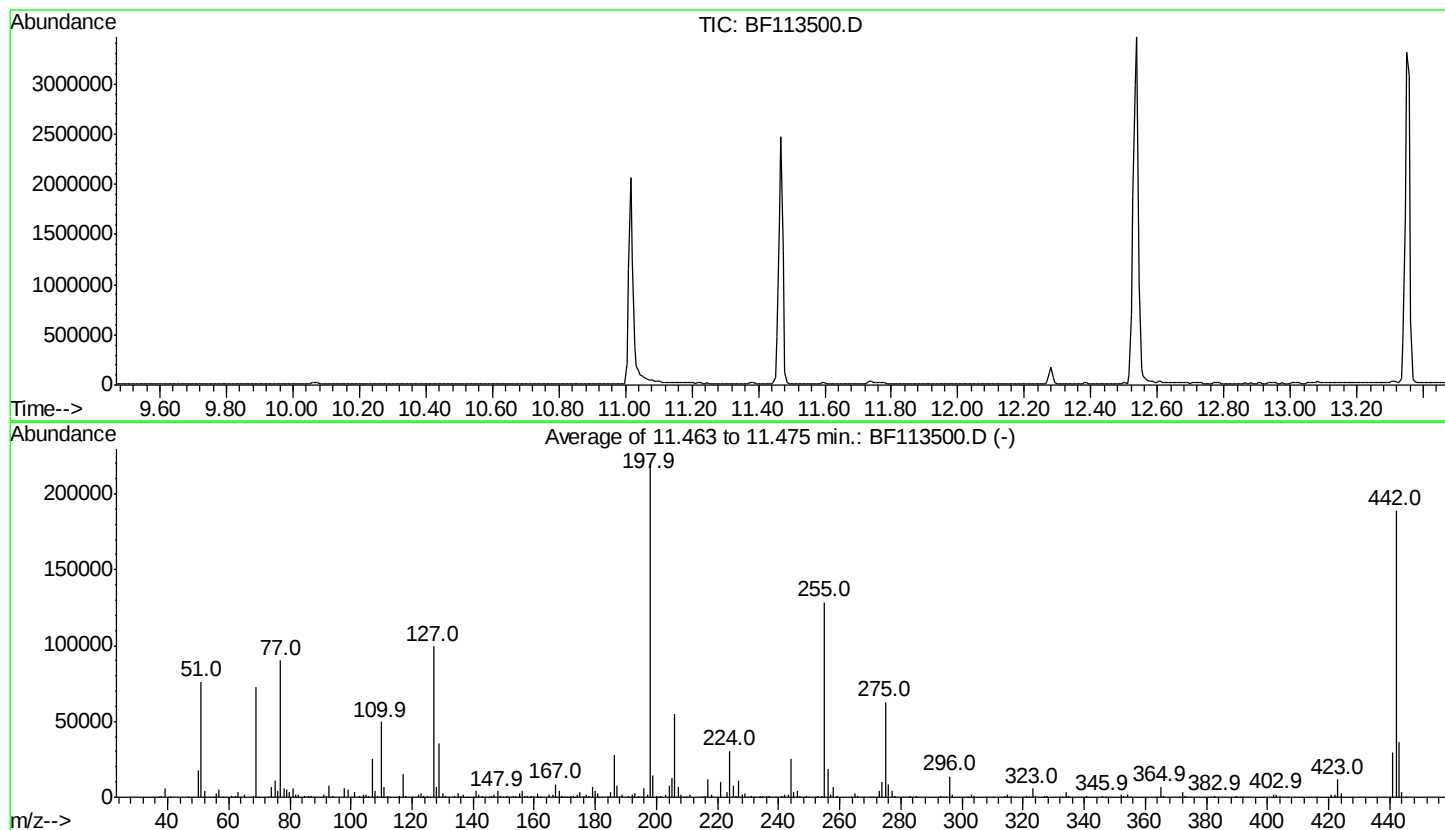

AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	76175	PASS
68	69	0.00	2	1.5	1115	PASS
69	198	0.00	100	33.1	72309	PASS
70	69	0.00	2	0.4	285	PASS
127	198	10	80	45.5	99477	PASS
197	198	0.00	2	0.6	1350	PASS
198	198	100	100	100.0	218602	PASS
199	198	5	9	6.6	14413	PASS
275	198	10	60	28.6	62568	PASS
365	198	1	100	3.2	6961	PASS
441	198	0.01	100	13.7	29917	PASS
442	198	50	100	86.3	188677	PASS
443	442	15	24	19.4	36552	PASS