


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040219\
 Data File : BF113525.D
 Acq On : 3 Apr 2019 1:41
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 26 03:32:08 2019

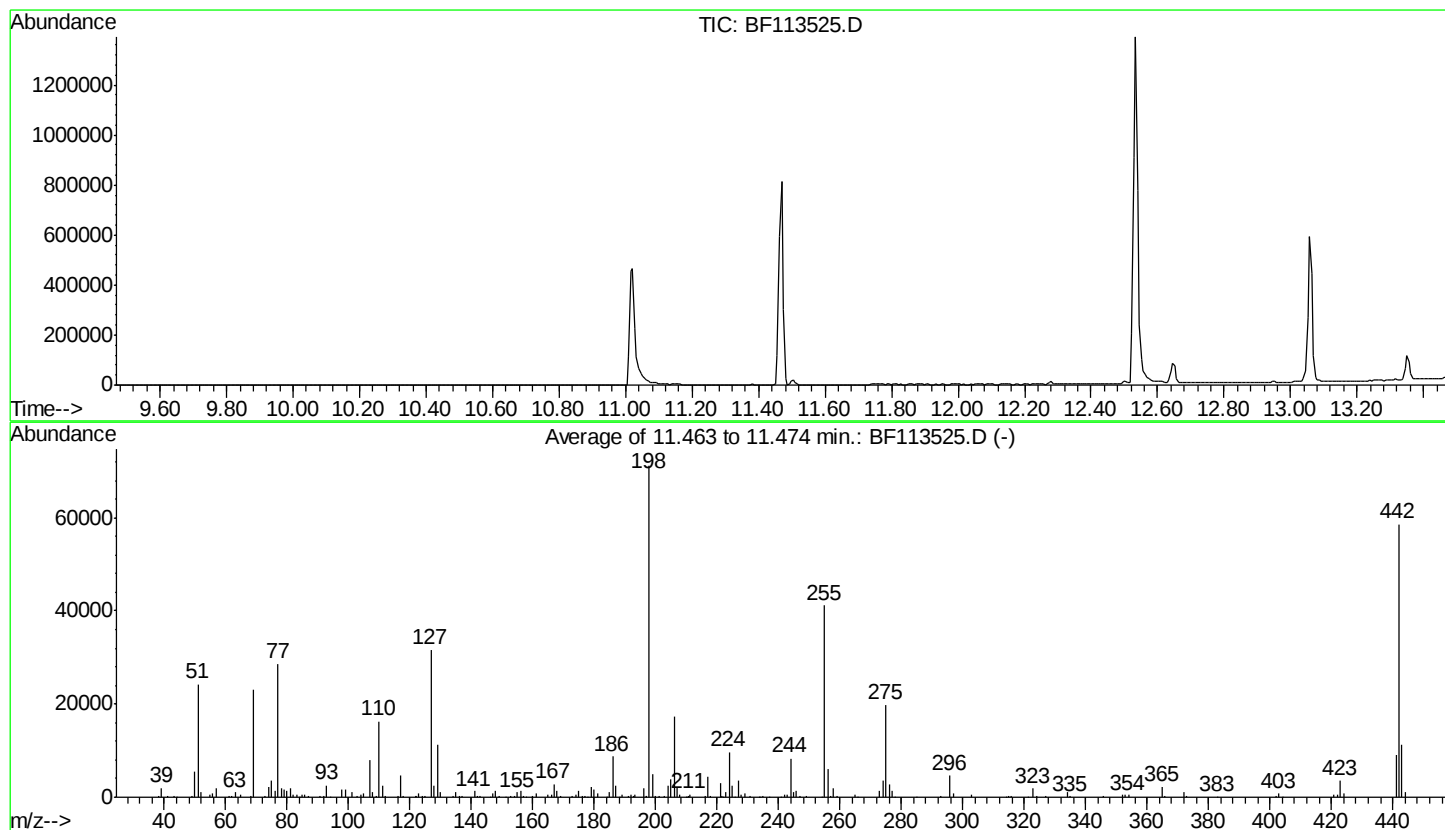

AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	24281	PASS
68	69	0.00	2	1.7	387	PASS
69	198	0.00	100	32.2	22952	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.5	31701	PASS
197	198	0.00	2	0.3	216	PASS
198	198	100	100	100.0	71176	PASS
199	198	5	9	6.9	4899	PASS
275	198	10	60	28.0	19908	PASS
365	198	1	100	3.1	2215	PASS
441	198	0.01	100	12.9	9181	PASS
442	198	50	100	82.3	58600	PASS
443	442	15	24	19.3	11304	PASS