
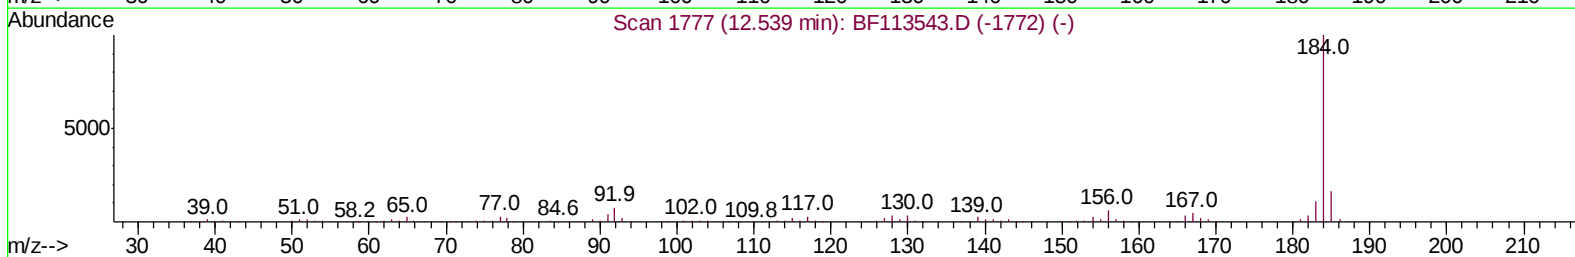
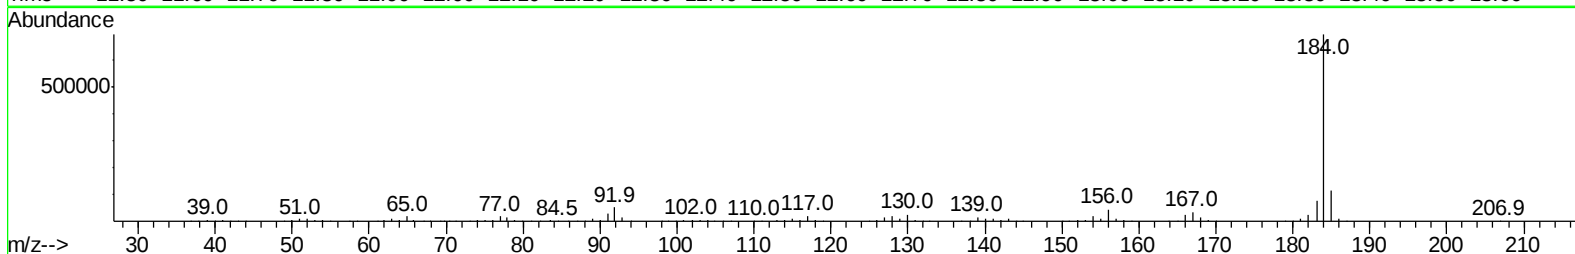


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF040319\
Data File : BF113549.D
Acq On : 3 Apr 2019 17:40
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 06:35:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 04 04:05:31 2019
Response via : Initial Calibration

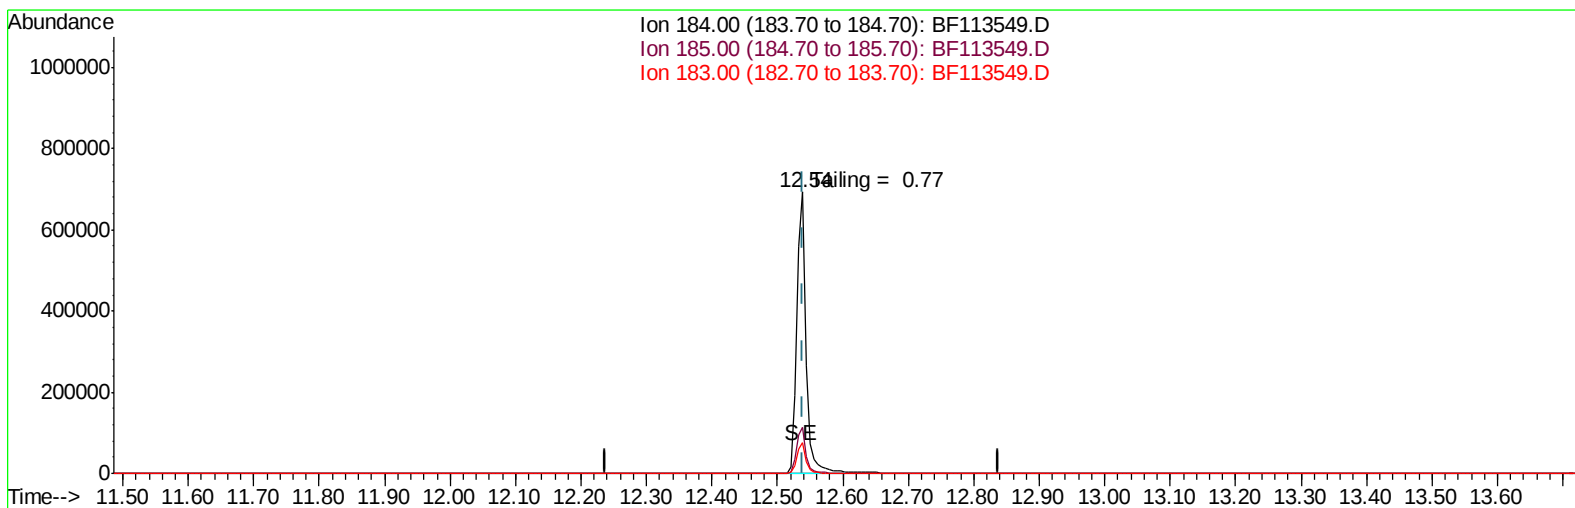

TIC: BF113549.D

(77) Benzidine




12.539min (0.000) 0.00ng

response 688857

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	16.19
183.00	11.20	10.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF040319\
Data File : BF113549.D
Acq On : 3 Apr 2019 17:40
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 06:35:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 04 04:05:31 2019
Response via : Initial Calibration

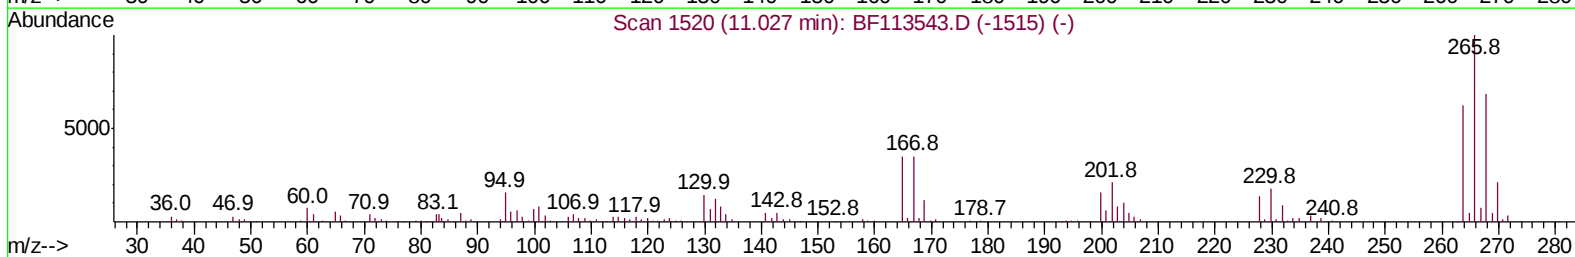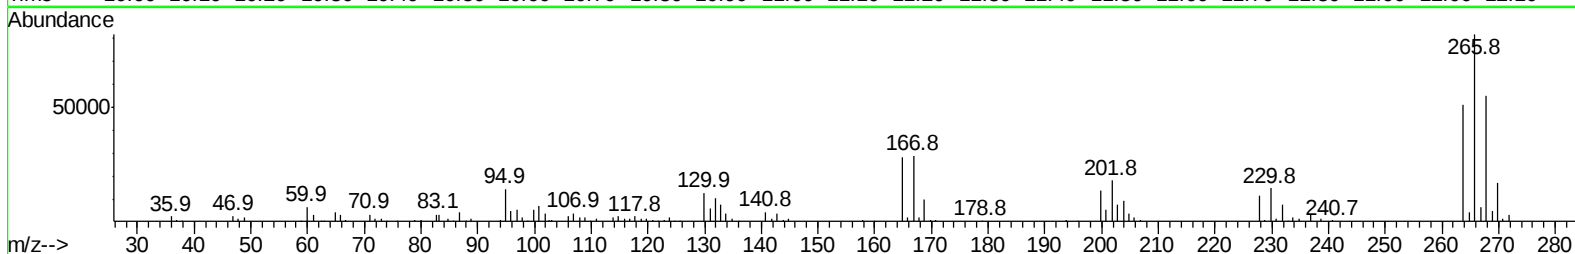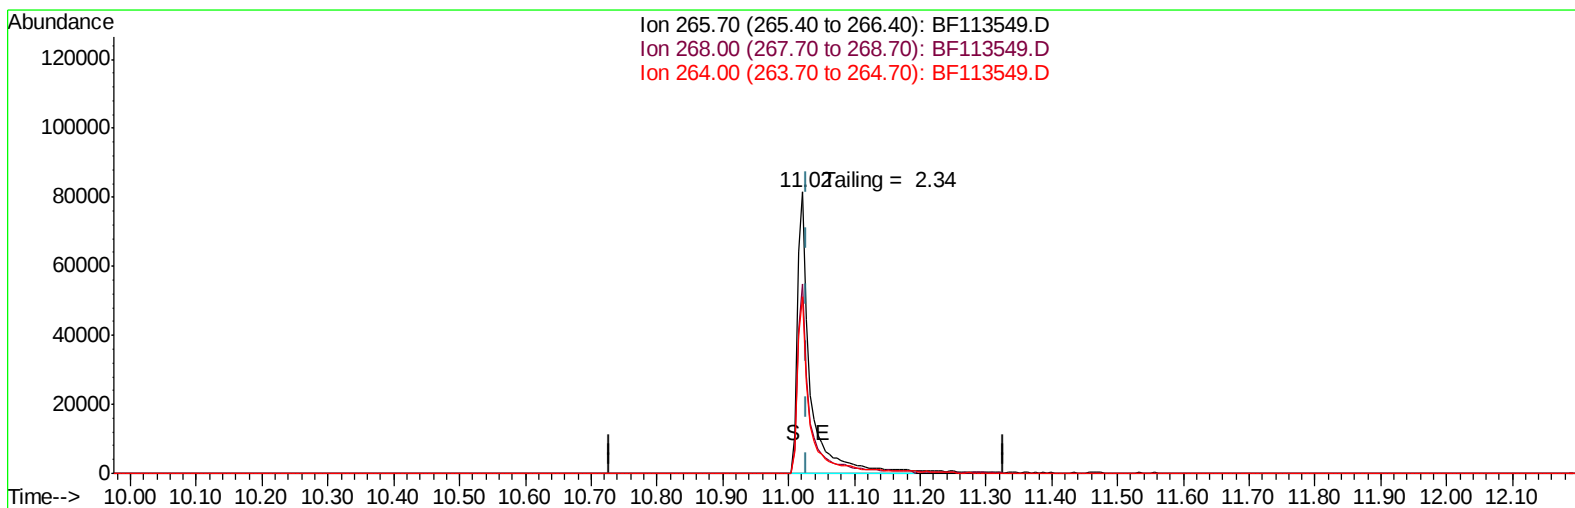

TIC: BF113549.D

(70) Pentachlorophenol (C)

11.022min (-0.006) 55388.07ng

response 111353

Ion	Exp%	Act%
265.70	100	100
268.00	67.20	67.36
264.00	61.50	62.60
0.00	0.00	0.00