
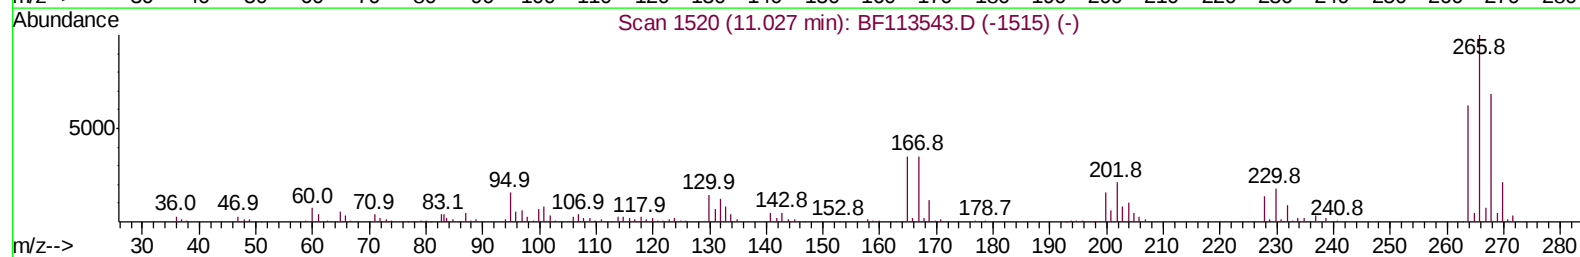
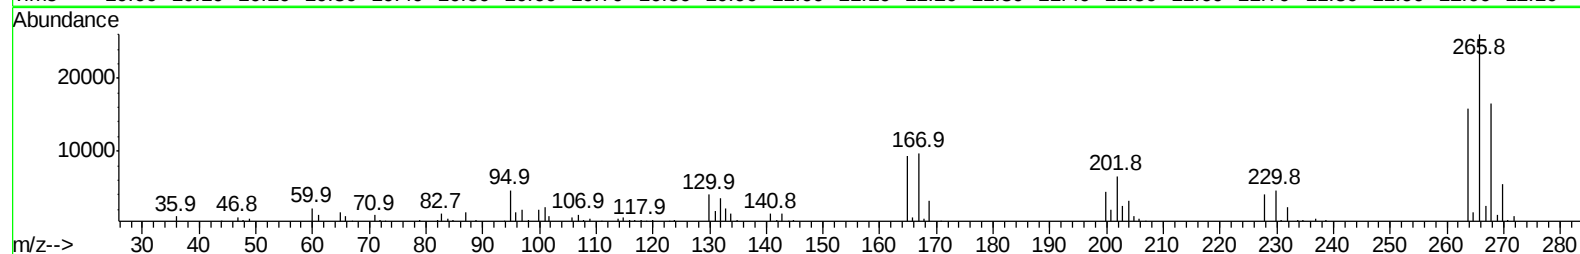


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF040319\
Data File : BF113573.D
Acq On : 4 Apr 2019 6:13
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 06:37:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 04 04:05:31 2019
Response via : Initial Calibration

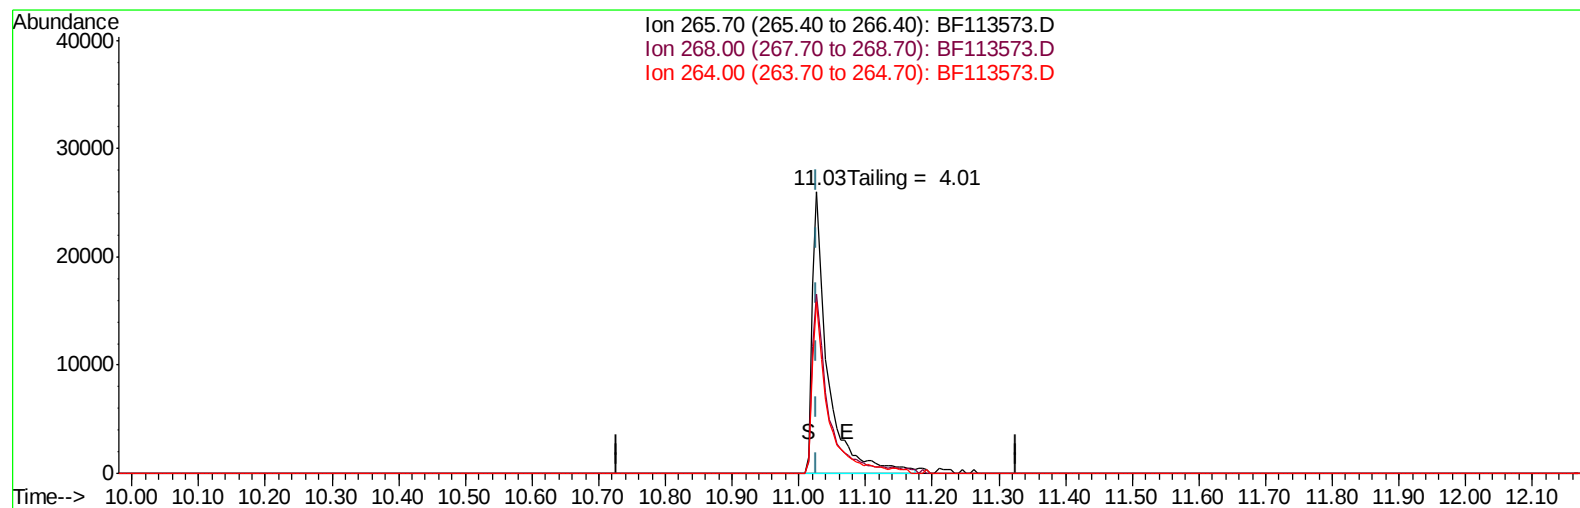

TIC: BF113573.D

(70) Pentachlorophenol (C)




11.027min (-0.000) 56185.09ng

response 40487

Ion	Exp%	Act%
265.70	100	100
268.00	67.20	63.65
264.00	61.50	66.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF040319\
Data File : BF113573.D
Acq On : 4 Apr 2019 6:13
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 06:37:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 04 04:05:31 2019
Response via : Initial Calibration

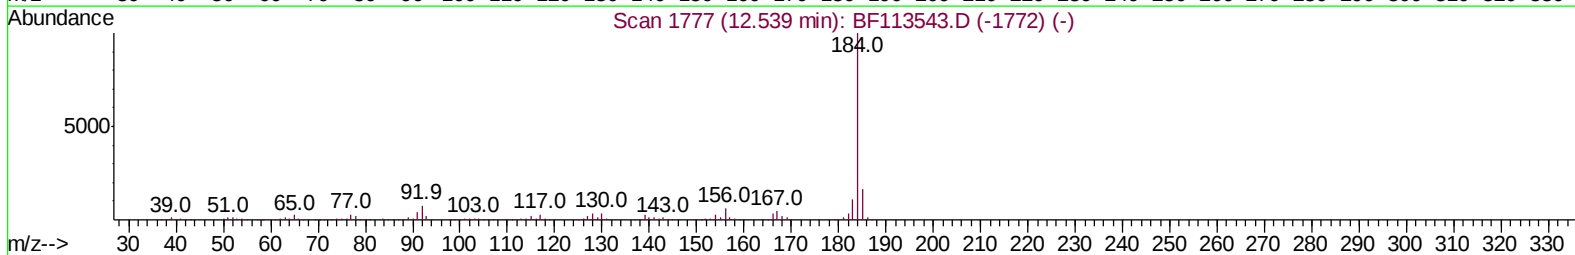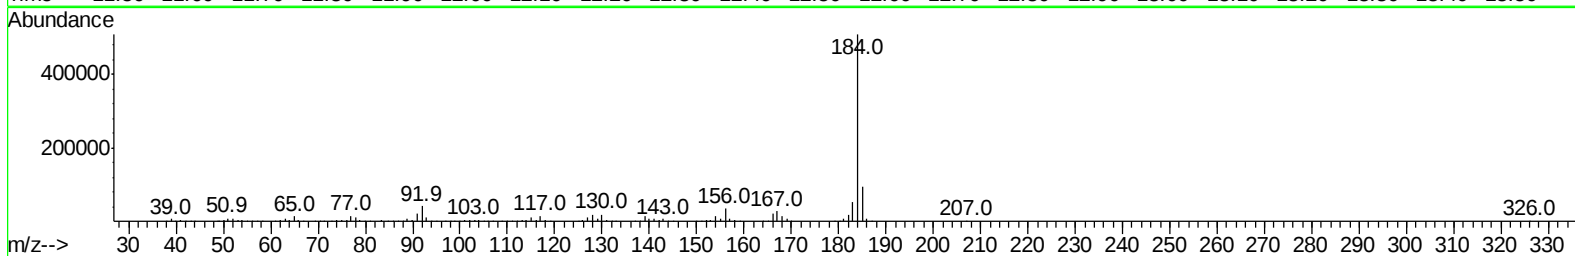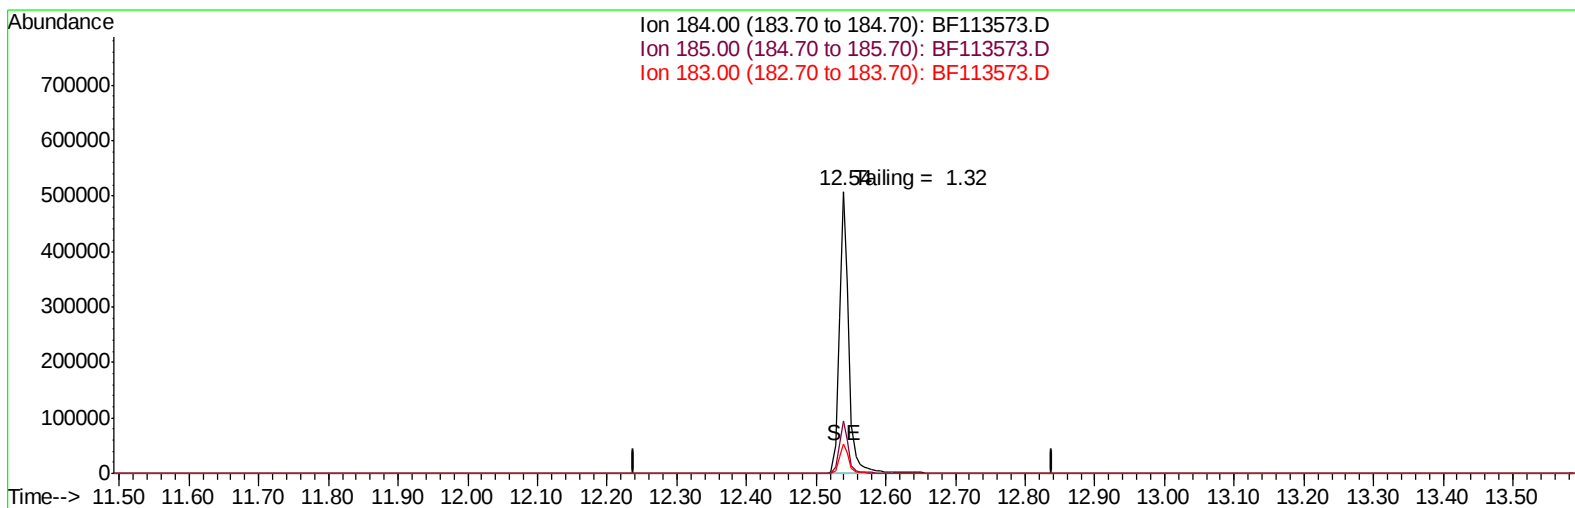

TIC: BF113573.D

(77) Benzidine

12.539min (-0.000) 116619.56ng m

response 481374

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	18.52
183.00	11.20	10.64
0.00	0.00	0.00