

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040319\
 Data File : BF113569.D
 Acq On : 4 Apr 2019 3:49
 Operator : JU/SJ
 Sample : K2178-02 5X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 COMP-17

Quant Time: Apr 04 07:36:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 04 04:05:31 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.69	152	127503	20.00	ng	0.00
21) Naphthalene-d8	7.97	136	466871	20.00	ng	0.00
39) Acenaphthene-d10	9.72	164	197000	20.00	ng	0.00
64) Phenanthrene-d10	11.20	188	367112	20.00	ng	0.00
76) Chrysene-d12	13.84	240	292920	20.00	ng	0.00
87) Perylene-d12	15.26	264	217199	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.30	112	101134	13.53	ng	0.00
7) Phenol-d6	6.33	99	144608	15.69	ng	0.00
23) Nitrobenzene-d5	7.25	82	73556	9.23	ng	-0.01
42) 2,4,6-Tribromophenol	10.52	330	24479	10.34	ng	0.00
45) 2-Fluorobiphenyl	9.05	172	162929	13.31	ng	0.00
79) Terphenyl-d14	12.79	244	164560	11.44	ng	0.00


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040319\
Data File : BF113569.D
Acq On : 4 Apr 2019 3:49
Operator : JU/SJ
Sample : K2178-02 5X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-17

Quant Time: Apr 04 07:36:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 04 04:05:31 2019
Response via : Initial Calibration

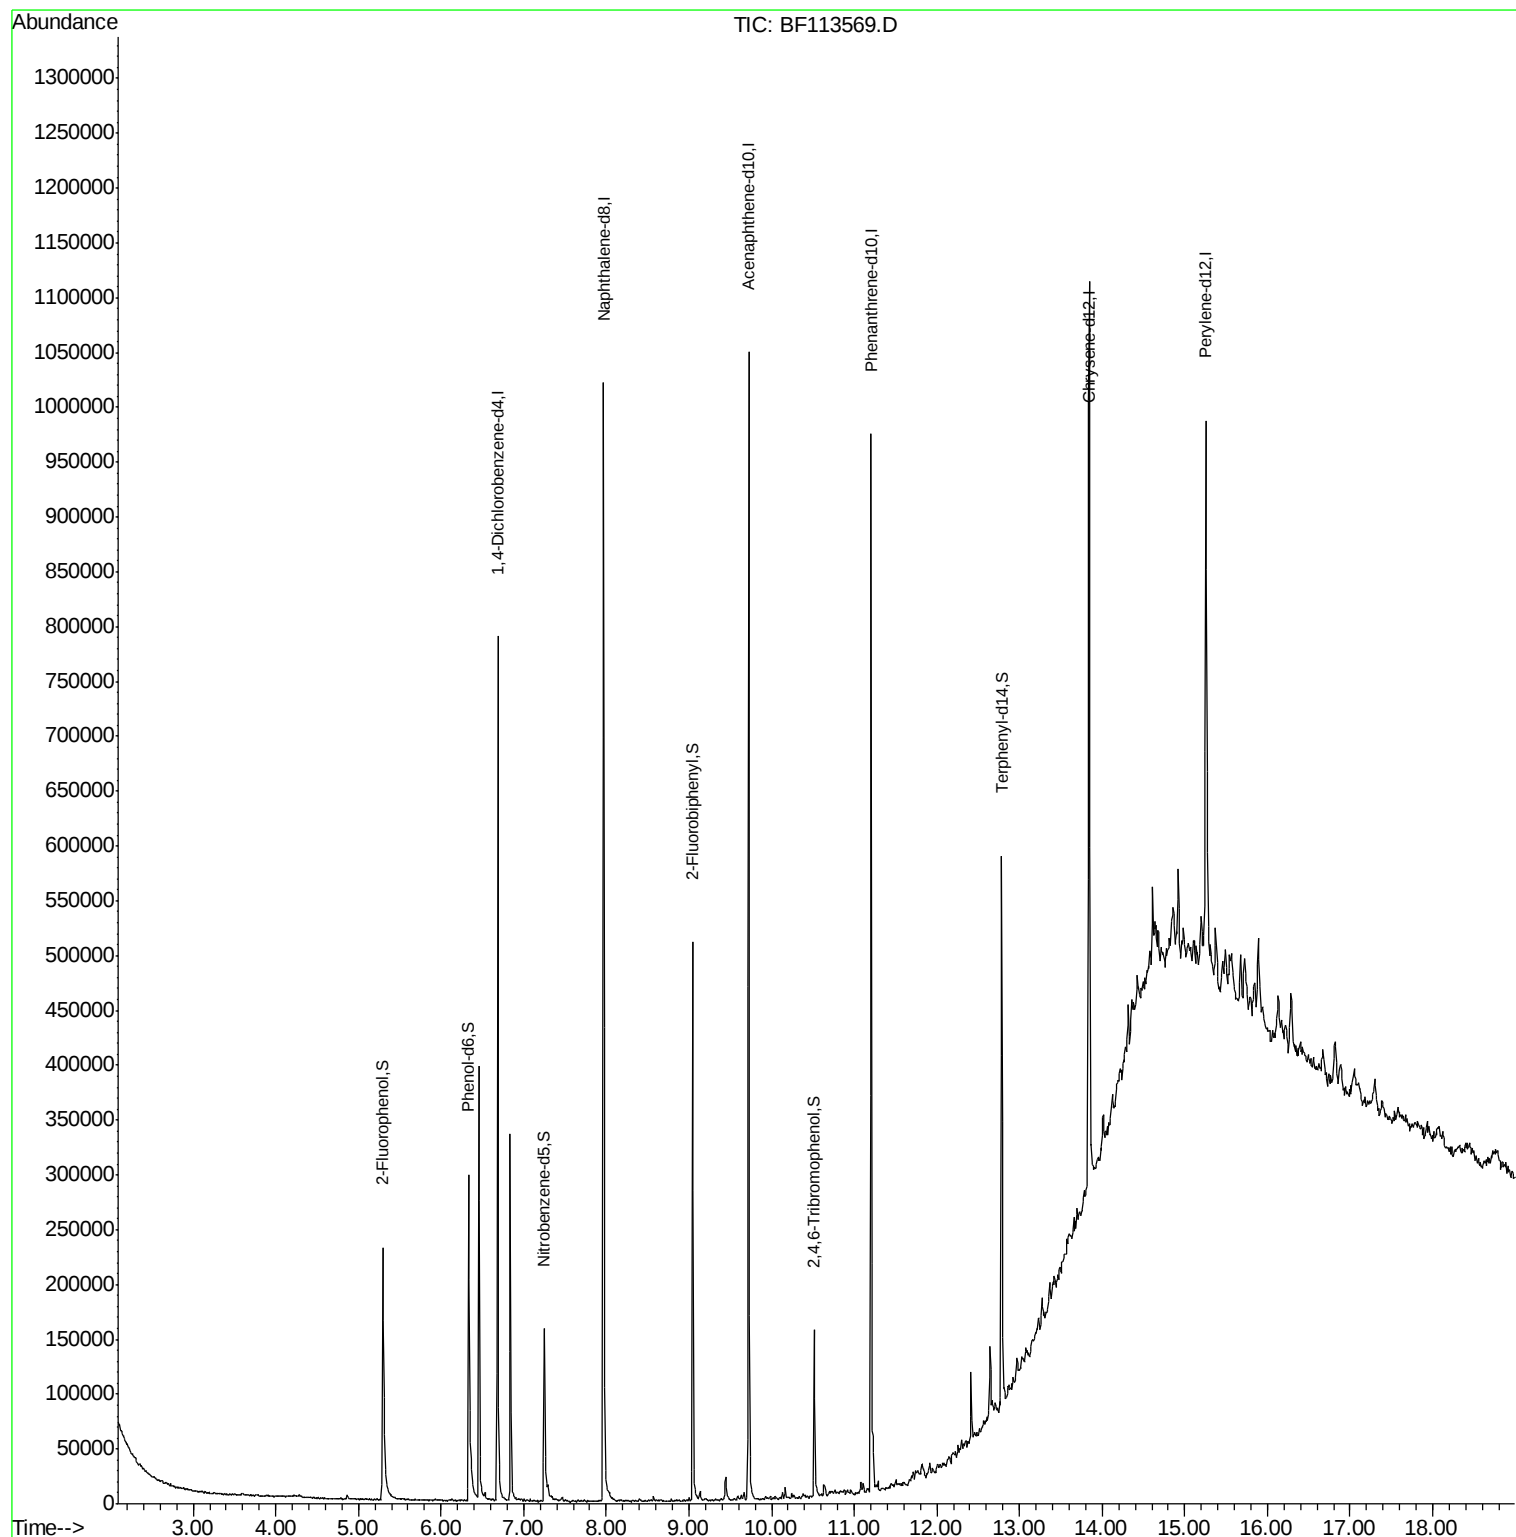




#1



1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.69 min Scan# 782
 Delta R.T. -0.00 min
 Lab File: BF113569.D
 Acq: 4 Apr 2019 3:49

Instrument :
 BNA_F
 ClientSampleId :
 COMP-17

Tgt Ion:152 Resp: 127503
 Ion Ratio Lower Upper
 152 100
 150 157.8 124.7 187.1
 115 53.8 46.0 69.0

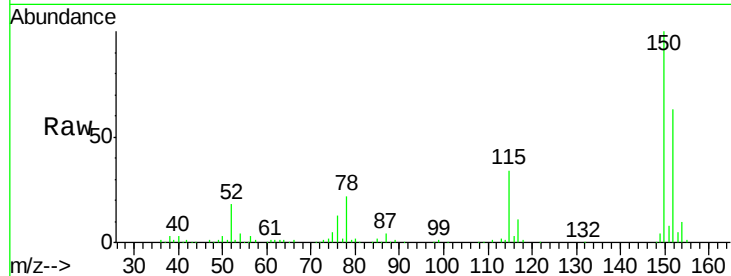


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

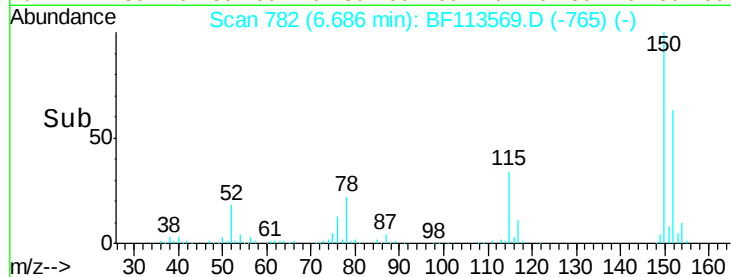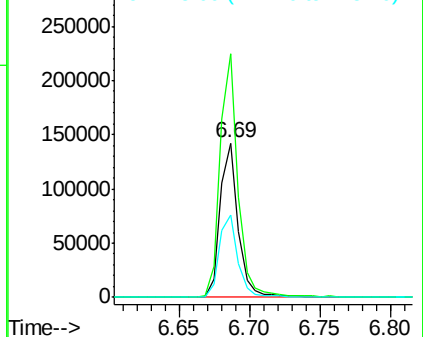



#5


2-Fluorophenol
 Concen: 13.526 ng
 RT: 5.30 min Scan# 546
 Delta R.T. -0.00 min
 Lab File: BF113569.D
 Acq: 4 Apr 2019 3:49

Tgt Ion:112 Resp: 101134
 Ion Ratio Lower Upper
 112 100
 64 59.3 49.2 73.8
 63 27.7 24.9 37.3

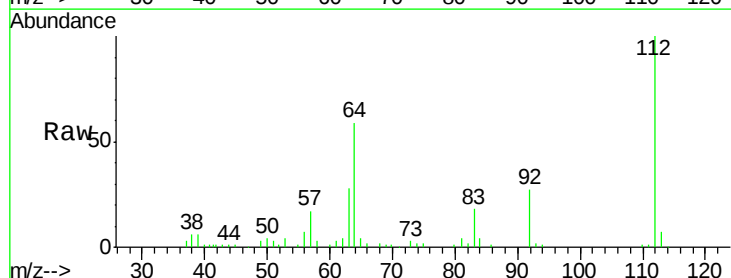

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

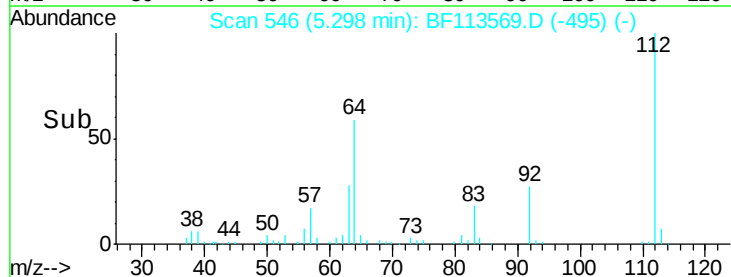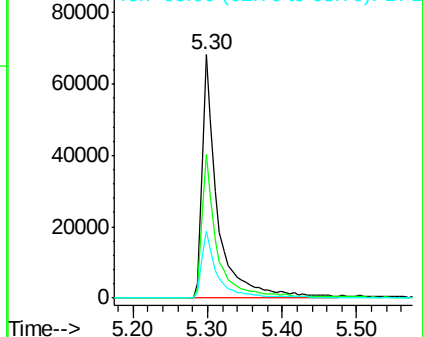

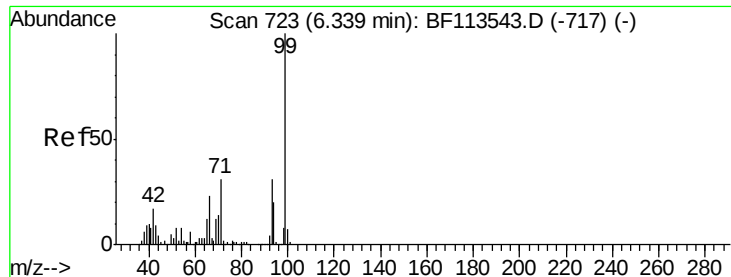

#7

Phenol-d6

Concen: 15.692 ng

RT: 6.33 min Scan# 722

Delta R.T. -0.01 min

Lab File: BF113569.D

Acq: 4 Apr 2019 3:49

Instrument :

BNA_F

ClientSampleId :

COMP-17





Tgt Ion: 99 Resp: 144608

Ion Ratio Lower Upper

99 100

42 17.9 14.8 22.2

71 30.6 24.9 37.3

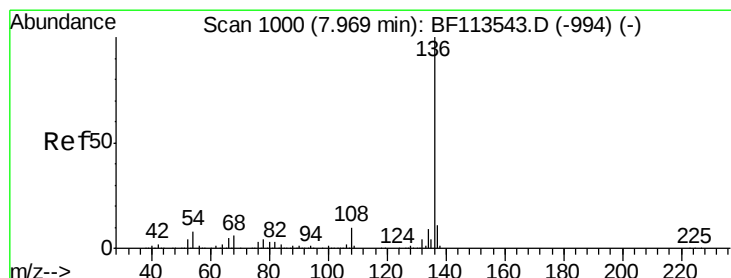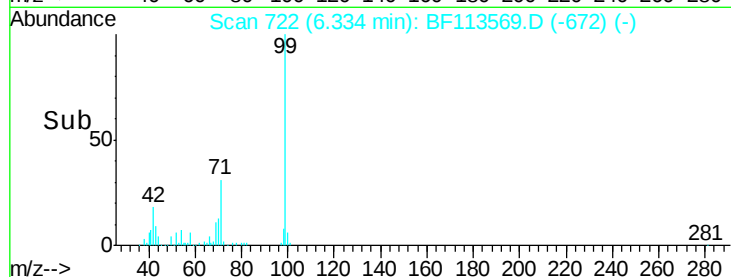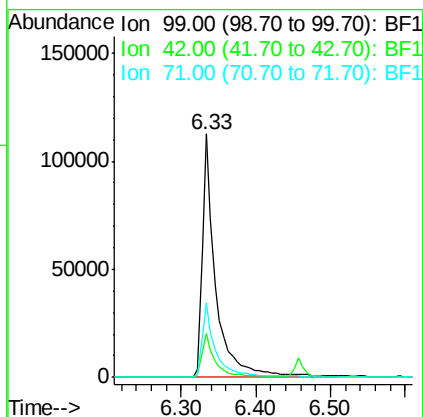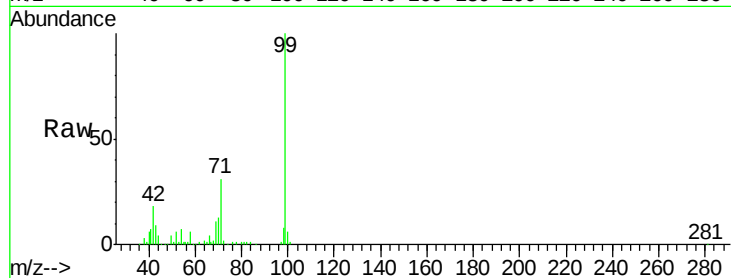

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.97 min Scan# 1000

Delta R.T. -0.00 min

Lab File: BF113569.D

Acq: 4 Apr 2019 3:49

Tgt Ion: 136 Resp: 466871




Ion Ratio Lower Upper

136 100

137 10.8 8.9 13.3

54 7.5 7.0 10.6

68 5.9 4.8 7.2

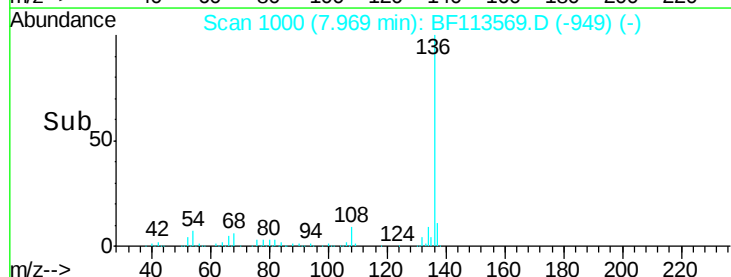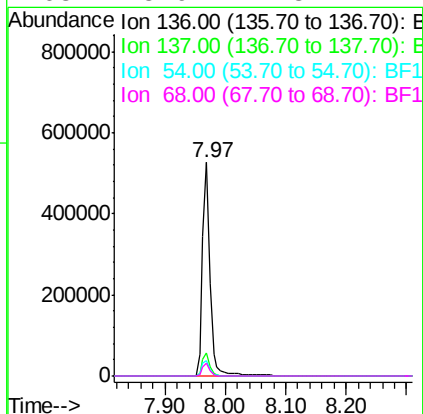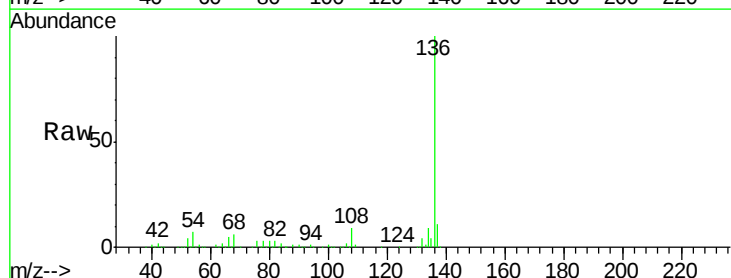







#23
 Nitrobenzene-d5
 Concen: 9.229 ng
 RT: 7.25 min Scan# 877
 Delta R.T. -0.01 min
 Lab File: BF113569.D
 Acq: 4 Apr 2019 3:49

Instrument :
 BNA_F
 ClientSampleId :
 COMP-17

Tgt Ion: 82 Resp: 73556
 Ion Ratio Lower Upper
 82 100
 128 42.0 36.5 54.7
 54 49.2 42.2 63.2

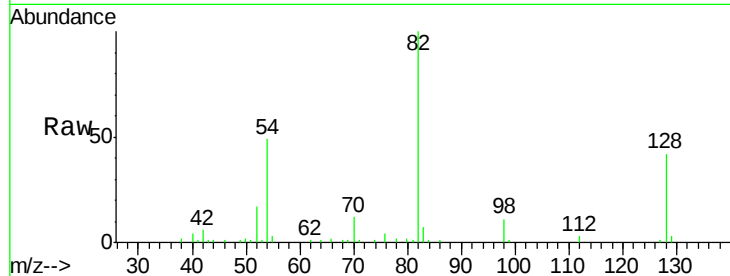


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1

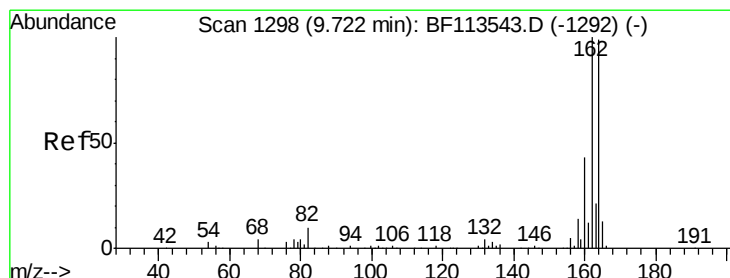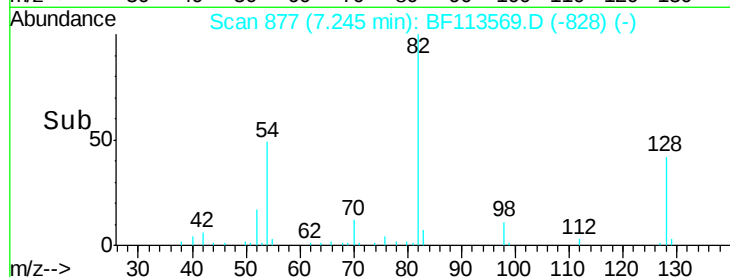
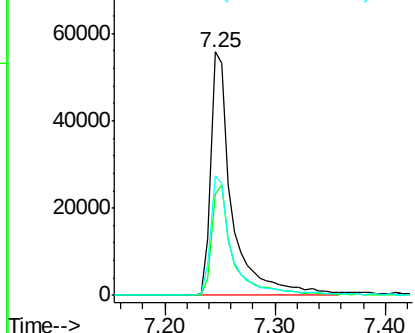



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.72 min Scan# 1298
 Delta R.T. -0.00 min
 Lab File: BF113569.D
 Acq: 4 Apr 2019 3:49

Tgt Ion: 164 Resp: 197000
 Ion Ratio Lower Upper
 164 100
 162 99.8 81.8 122.6
 160 44.5 36.4 54.6

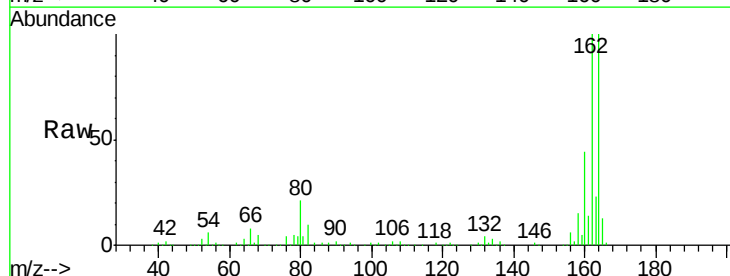

Abundance Ion 164.00 (163.70 to 164.70): BF1
 Ion 162.00 (161.70 to 162.70): BF1
 Ion 160.00 (159.70 to 160.70): BF1



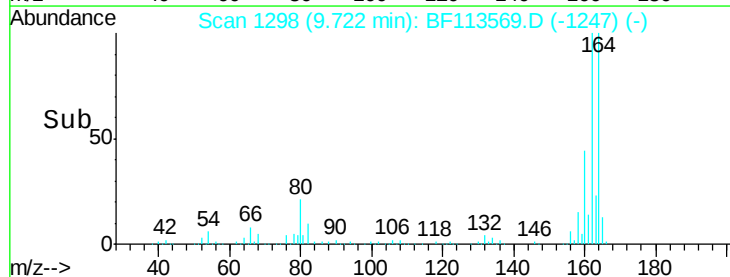
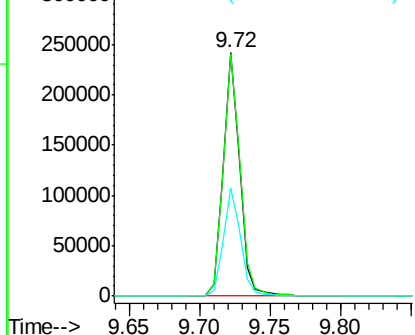


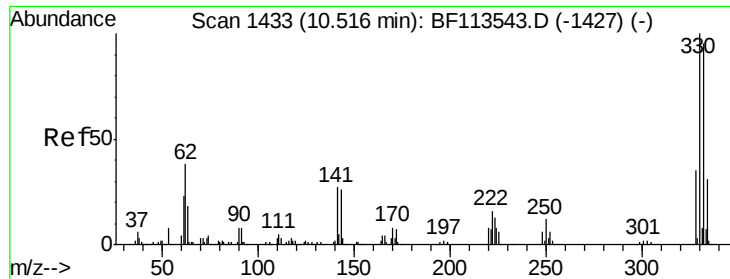

#42
 2,4,6-Tribromophenol
 Concen: 10.344 ng
 RT: 10.52 min Scan# 1433
 Delta R.T. -0.00 min
 Lab File: BF113569.D
 Acq: 4 Apr 2019 3:49




Instrument :
 BNA_F
 ClientSampleId :
 COMP-17


Tgt Ion:330 Resp: 24479
 Ion Ratio Lower Upper
 330 100
 332 96.3 77.8 116.6
 141 28.6 22.7 34.1

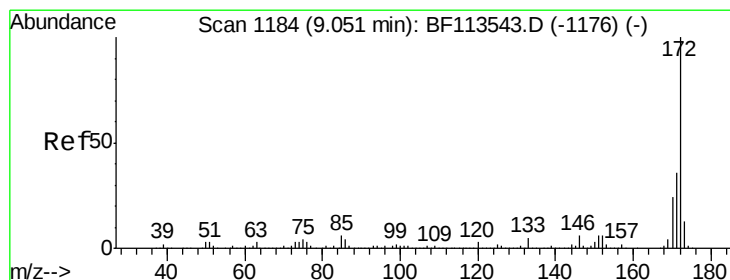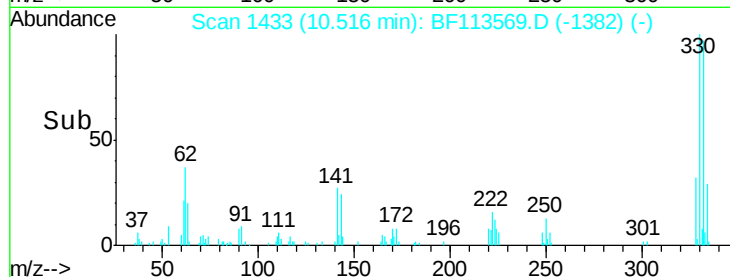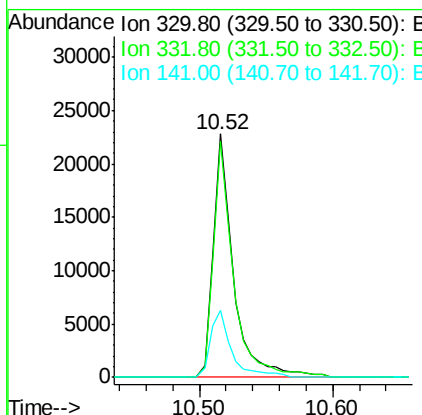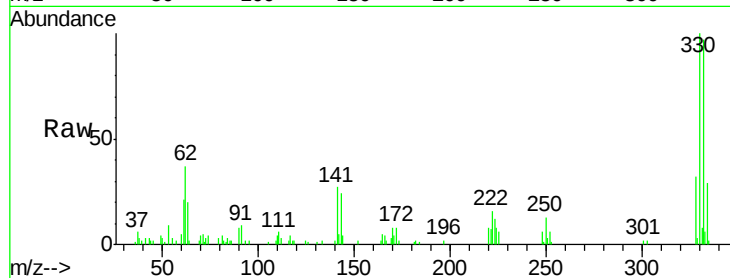

#45
 2-Fluorobiphenyl
 Concen: 13.315 ng
 RT: 9.05 min Scan# 1183
 Delta R.T. -0.01 min
 Lab File: BF113569.D
 Acq: 4 Apr 2019 3:49

Tgt Ion:172 Resp: 162929
 Ion Ratio Lower Upper
 172 100
 171 35.2 29.0 43.6
 170 23.3 19.5 29.3

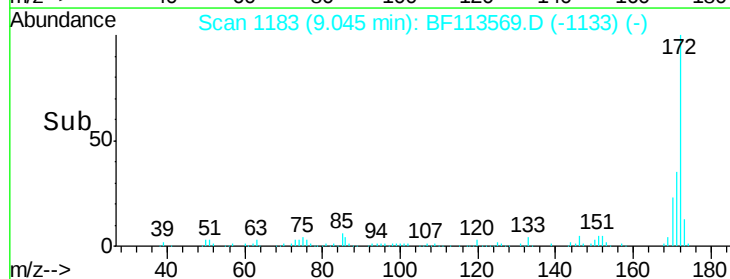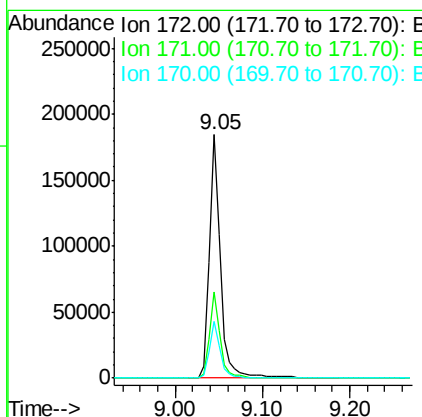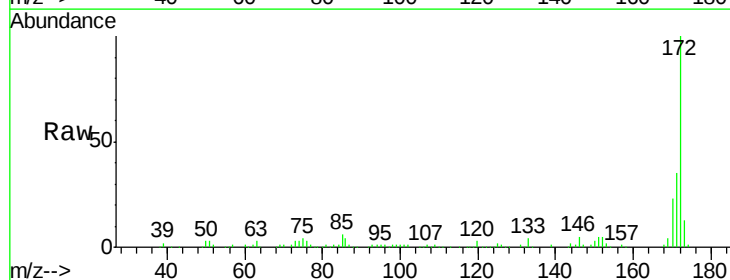

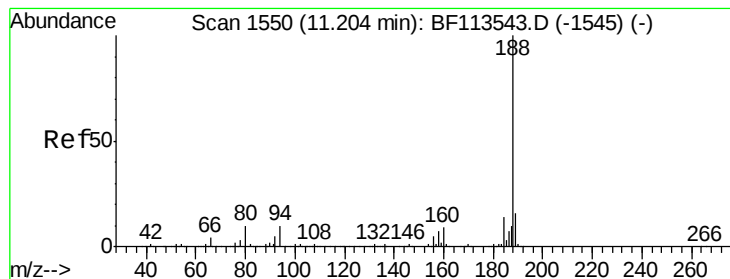

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.20 min Scan# 1550

Delta R.T. -0.00 min

Lab File: BF113569.D

Acq: 4 Apr 2019 3:49

Instrument :

BNA_F

ClientSampled :

COMP-17


Tgt Ion:188 Resp: 367112

Ion Ratio Lower Upper

188 100

94 9.6 7.0 10.6




80 9.8 7.7 11.5

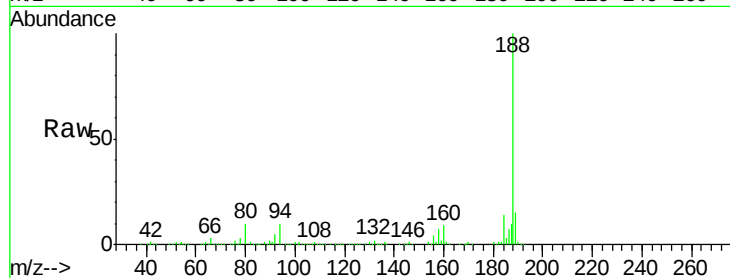

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

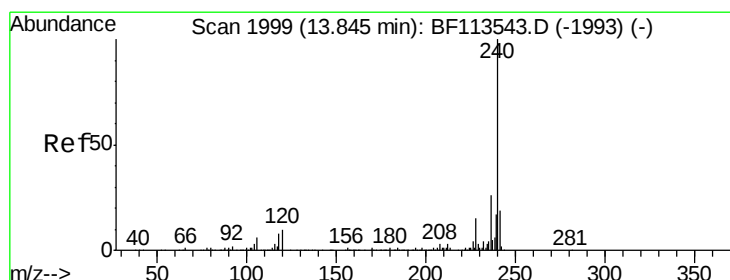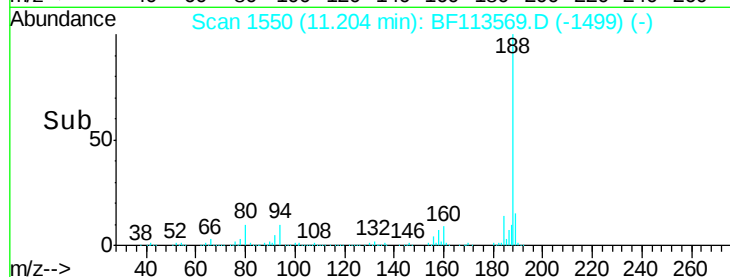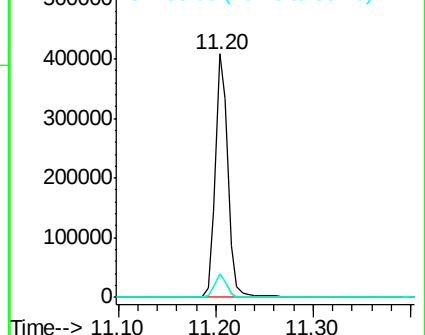

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.84 min Scan# 1999

Delta R.T. -0.00 min

Lab File: BF113569.D

Acq: 4 Apr 2019 3:49


Tgt Ion:240 Resp: 292920

Ion Ratio Lower Upper

240 100

120 9.5 8.8 13.2



236 25.7 20.9 31.3

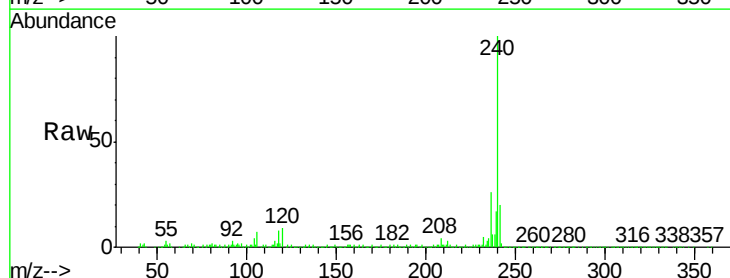


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

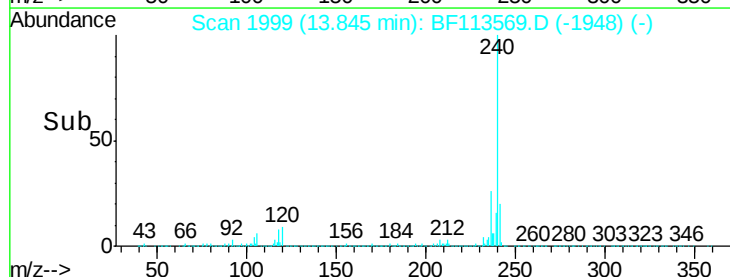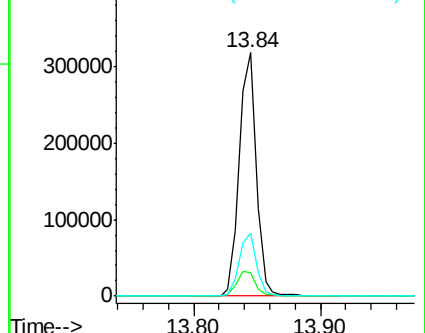

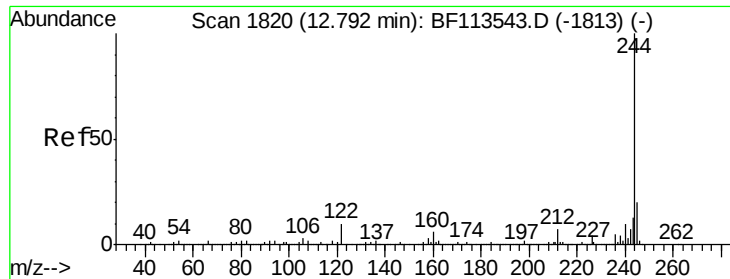

#79

Terphenyl-d14

Concen: 11.438 ng

RT: 12.79 min Scan# 1819

Delta R.T. -0.01 min

Lab File: BF113569.D

Acq: 4 Apr 2019 3:49

Instrument :

BNA_F

ClientSampleId :

COMP-17


Tgt Ion:244 Resp: 164560

Ion Ratio Lower Upper

244 100

212 5.9 5.5 8.3




122 10.8 8.6 13.0

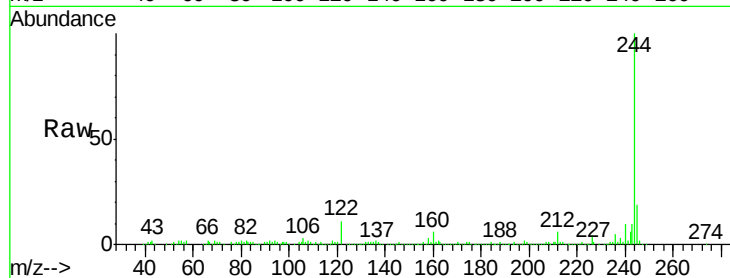

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

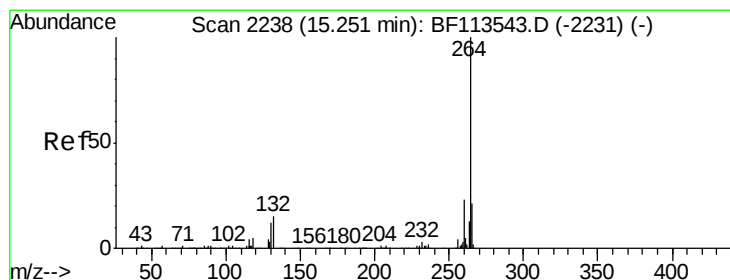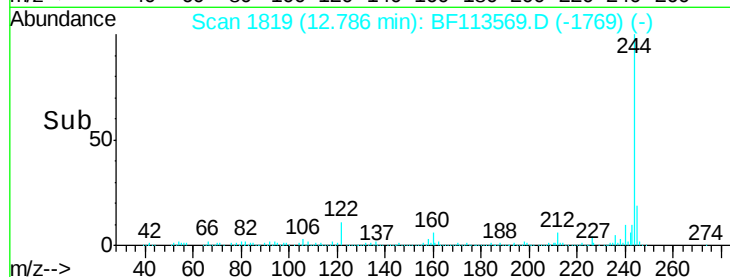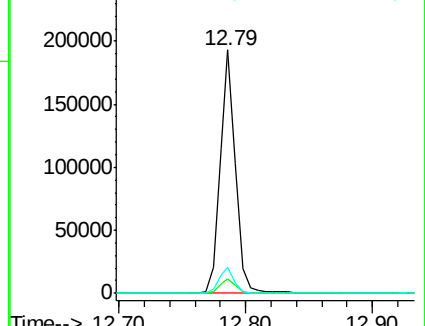

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.26 min Scan# 2239

Delta R.T. 0.01 min

Lab File: BF113569.D

Acq: 4 Apr 2019 3:49


Tgt Ion:264 Resp: 217199

Ion Ratio Lower Upper

264 100

260 23.6 19.1 28.7

265 21.7 17.1 25.7

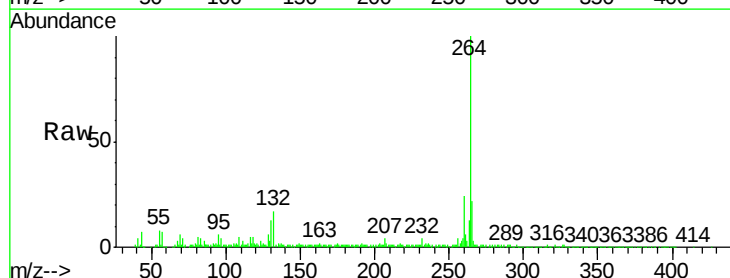

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

