

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040319\
 Data File : BF113568.D
 Acq On : 4 Apr 2019 3:19
 Operator : JU/SJ
 Sample : K2178-01 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 COMP-16

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.298	543	546	564	rBV	252356	341277	39.12%	4.270%
2	6.334	719	722	740	rBV	300606	388976	44.59%	4.866%
3	6.457	740	743	754	rVB	389206	383310	43.94%	4.796%
4	6.686	778	782	798	rBV	652551	577341	66.18%	7.223%
5	6.839	805	808	823	rBV	330562	319802	36.66%	4.001%
6	7.251	874	878	890	rBV	158288	206108	23.63%	2.579%
7	7.969	996	1000	1008	rBV	760646	673373	77.19%	8.424%
8	9.045	1180	1183	1194	rBV	499208	422383	48.42%	5.284%
9	9.445	1247	1251	1259	rVB	18393	19596	2.25%	0.245%
10	9.722	1295	1298	1302	rBV2	834869	699433	80.18%	8.750%
11	9.751	1302	1303	1307	rVB	21639	17760	2.04%	0.222%
12	10.269	1389	1391	1395	rBV	14470	14824	1.70%	0.185%
13	10.516	1429	1433	1443	rVB	206938	224061	25.68%	2.803%
14	11.110	1531	1534	1537	rVB2	11676	13365	1.53%	0.167%
15	11.204	1547	1550	1553	rBV	909955	813698	93.28%	10.180%
16	11.227	1553	1554	1558	rVV	172638	112847	12.94%	1.412%
17	11.280	1558	1563	1567	rVB2	47623	54277	6.22%	0.679%
18	11.445	1588	1591	1595	rBV	14713	18369	2.11%	0.230%
19	11.604	1615	1618	1625	rBV7	10652	15352	1.76%	0.192%
20	11.710	1633	1636	1638	rBV	21927	18506	2.12%	0.232%
21	11.739	1638	1641	1646	rVV	28263	32891	3.77%	0.411%
22	11.816	1651	1654	1657	rBV	30368	33315	3.82%	0.417%
23	12.004	1684	1686	1690	rBV	18113	20143	2.31%	0.252%
24	12.151	1706	1711	1714	rBV5	13429	23156	2.65%	0.290%
25	12.257	1726	1729	1732	rBV	19129	25781	2.96%	0.323%
26	12.415	1752	1756	1761	rBV	247336	223662	25.64%	2.798%
27	12.645	1790	1795	1798	rBV	195479	209147	23.98%	2.617%
28	12.786	1815	1819	1823	rBV	613261	536244	61.47%	6.709%
29	13.839	1994	1998	2001	rBV	842069	872344	100.00%	10.914%
30	15.256	2235	2239	2247	rVB	492665	681777	78.15%	8.530%


Sum of corrected areas: 7993118

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040319\
Data File : BF113568.D
Acq On : 4 Apr 2019 3:19
Operator : JU/SJ
Sample : K2178-01 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-16

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

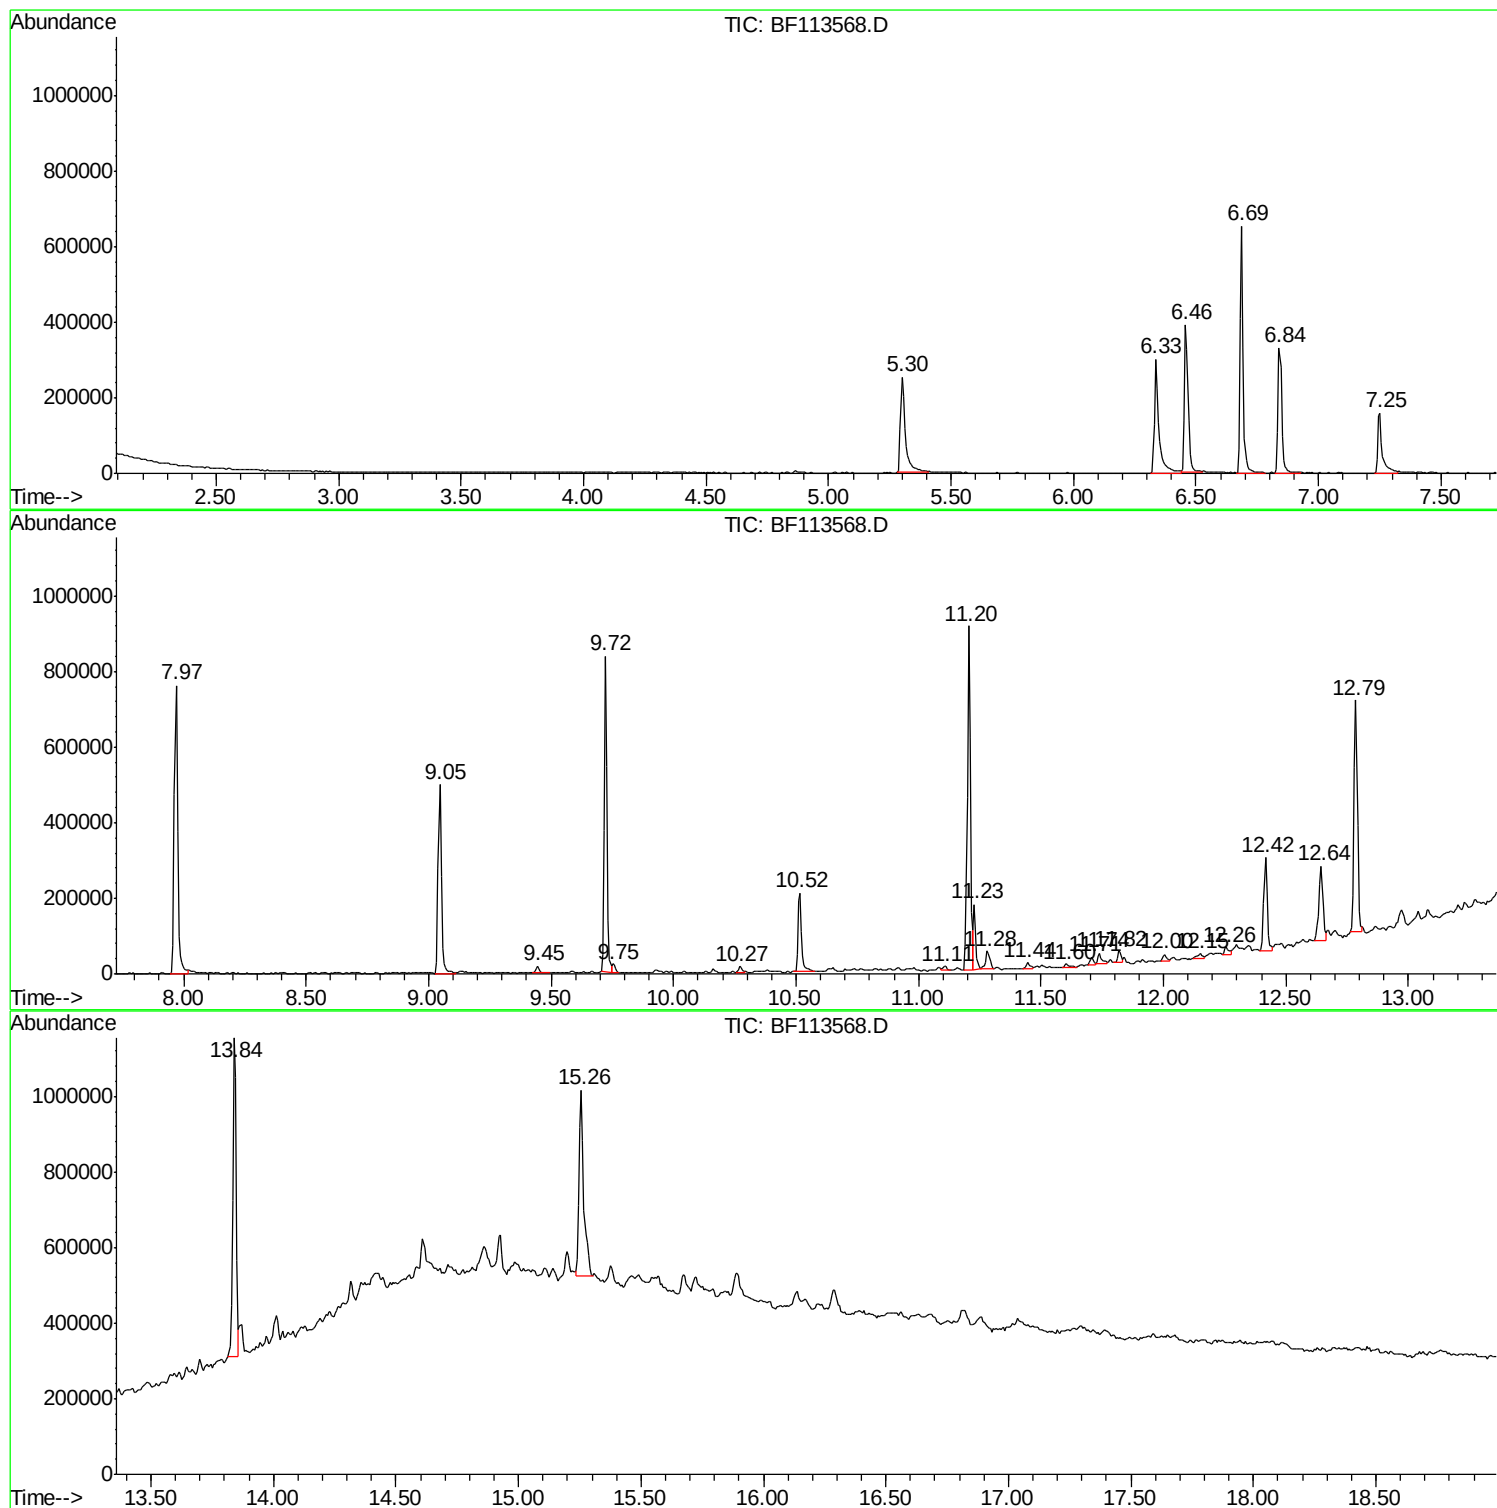

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040319\
Data File : BF113568.D
Acq On : 4 Apr 2019 3:19
Operator : JU/SJ
Sample : K2178-01 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-16










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.46 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.46	13.28 ng	383310	1,4-Dichlorobenzene-d4	6.69

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
5		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9

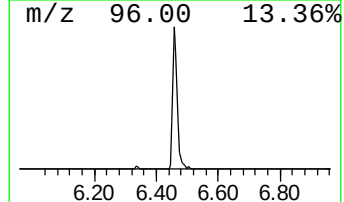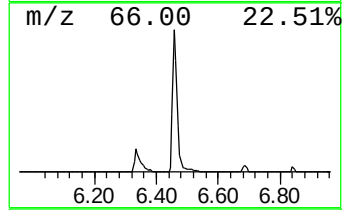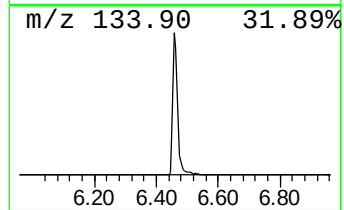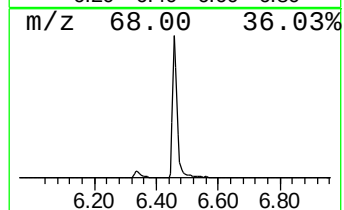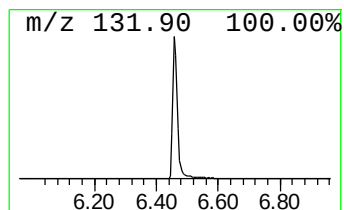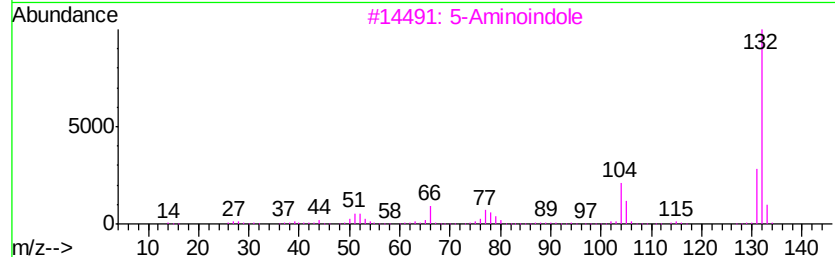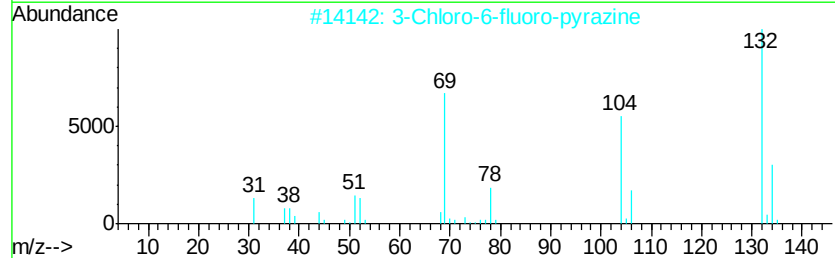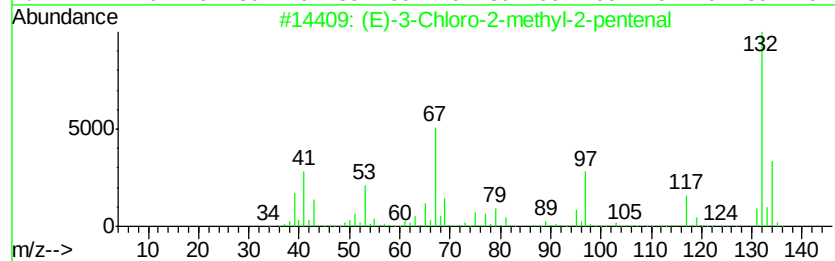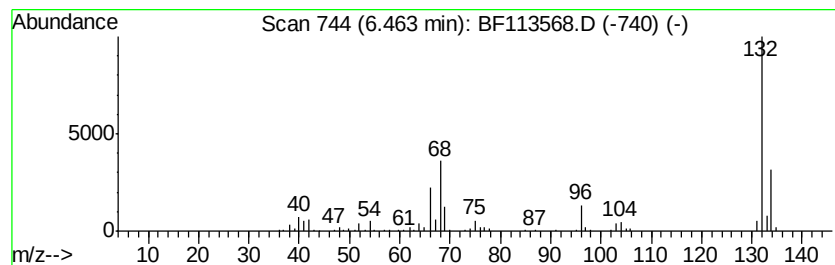

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040319\
Data File : BF113568.D
Acq On : 4 Apr 2019 3:19
Operator : JU/SJ
Sample : K2178-01 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-16

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.46	6.46	13.3	ng	383310	1	6.69	577341	20.0