


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040319\
 Data File : BF113540.D
 Acq On : 3 Apr 2019 11:02
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 04 04:05:31 2019

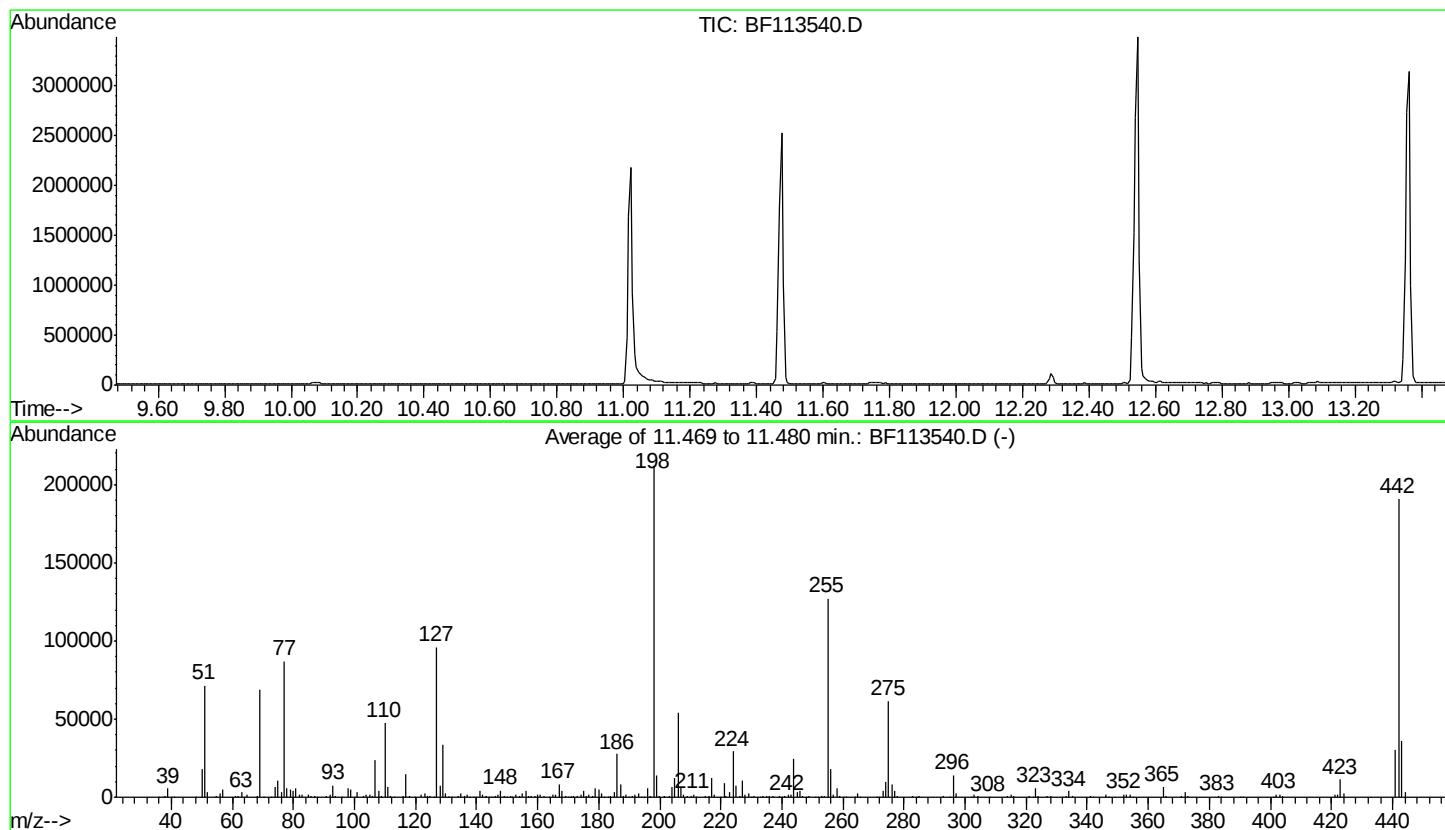

AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	71556	PASS
68	69	0.00	2	1.5	1029	PASS
69	198	0.00	100	32.5	68962	PASS
70	69	0.00	2	0.5	349	PASS
127	198	10	80	45.4	96274	PASS
197	198	0.00	2	0.3	636	PASS
198	198	100	100	100.0	212205	PASS
199	198	5	9	6.8	14355	PASS
275	198	10	60	29.0	61592	PASS
365	198	1	100	3.1	6654	PASS
441	198	0.01	100	14.3	30240	PASS
442	198	50	100	90.1	191104	PASS
443	442	15	24	19.0	36312	PASS