


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040319\
 Data File : BF113549.D
 Acq On : 3 Apr 2019 17:40
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 04 04:05:31 2019

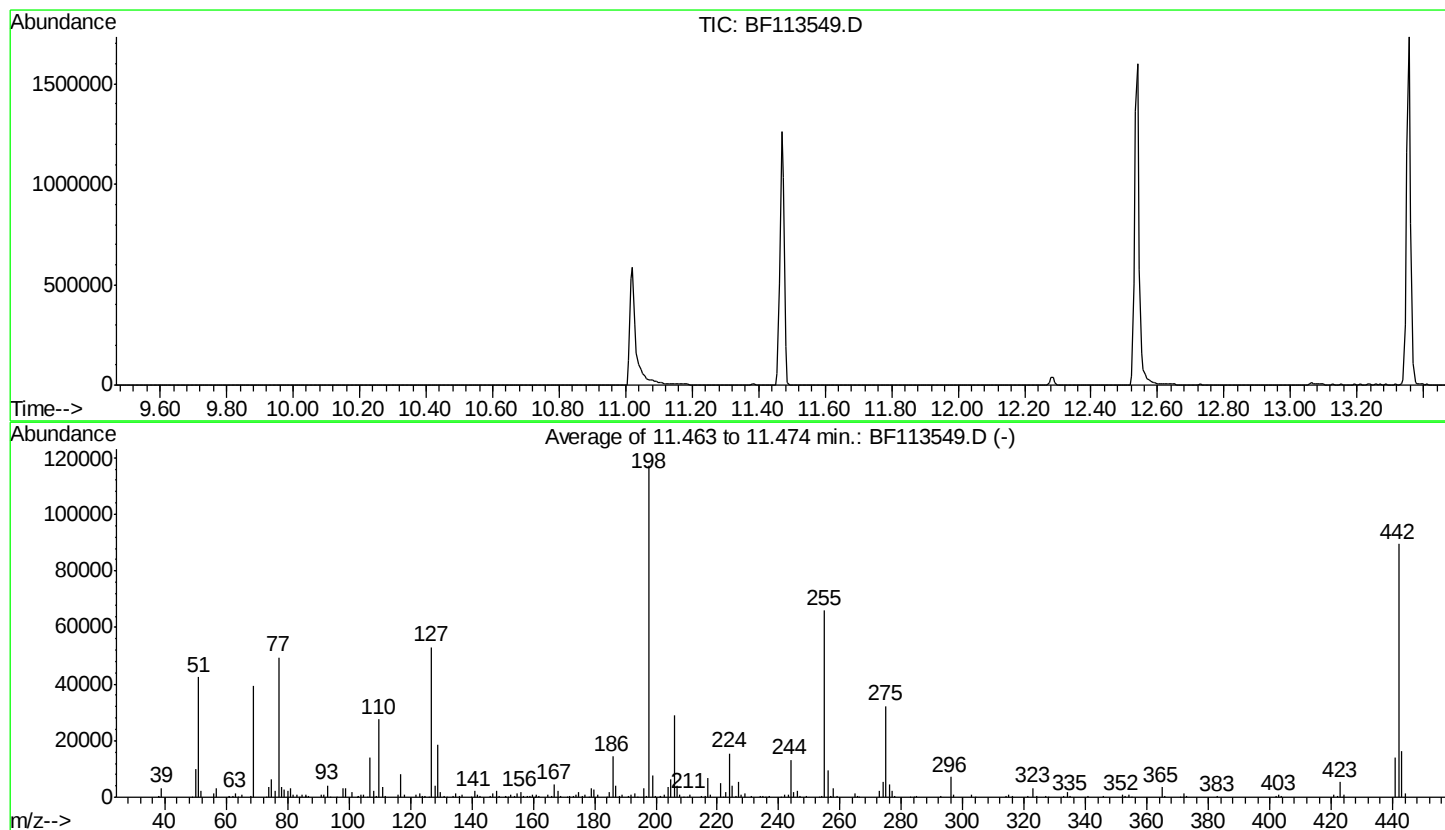

AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	42341	PASS
68	69	0.00	2	1.5	585	PASS
69	198	0.00	100	33.6	39362	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.3	53058	PASS
197	198	0.00	2	0.6	674	PASS
198	198	100	100	100.0	117192	PASS
199	198	5	9	6.5	7635	PASS
275	198	10	60	27.4	32135	PASS
365	198	1	100	2.9	3439	PASS
441	198	0.01	100	11.9	13937	PASS
442	198	50	100	76.4	89482	PASS
443	442	15	24	18.4	16433	PASS