


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040319\
 Data File : BF113573.D
 Acq On : 4 Apr 2019 6:13
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 04 04:05:31 2019

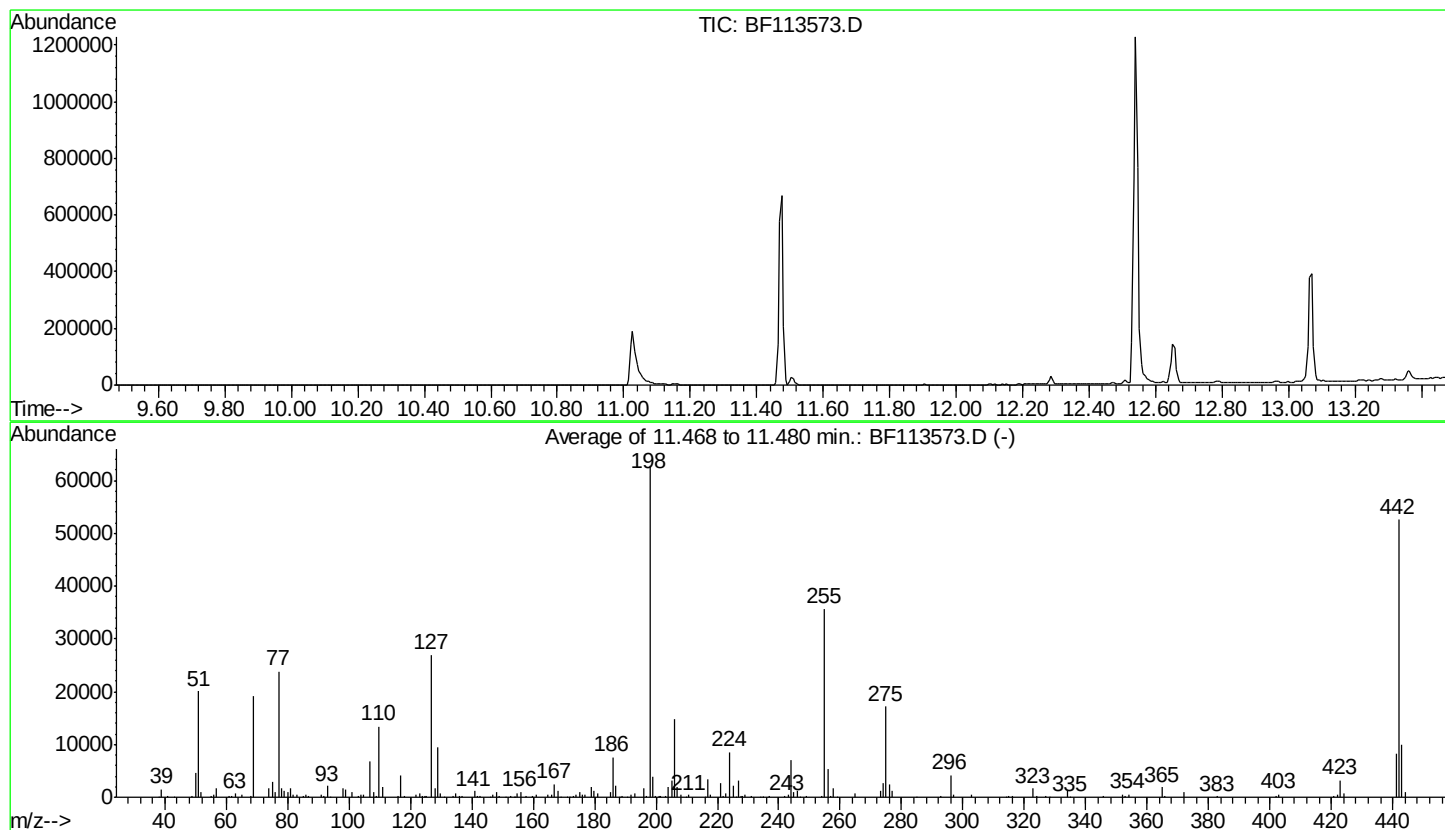

AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	20076	PASS
68	69	0.00	2	1.7	322	PASS
69	198	0.00	100	30.4	19123	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.9	26974	PASS
197	198	0.00	2	0.6	353	PASS
198	198	100	100	100.0	62813	PASS
199	198	5	9	6.0	3799	PASS
275	198	10	60	27.4	17208	PASS
365	198	1	100	3.1	1938	PASS
441	198	0.01	100	13.2	8313	PASS
442	198	50	100	83.7	52584	PASS
443	442	15	24	19.1	10041	PASS