
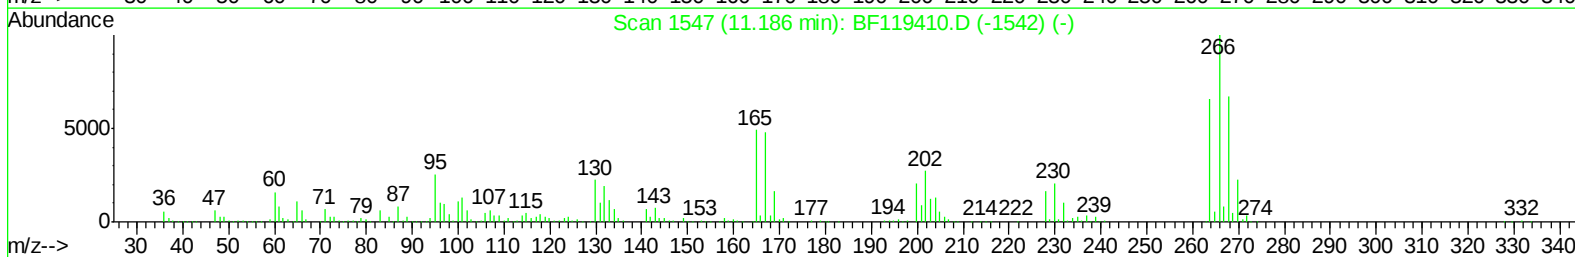
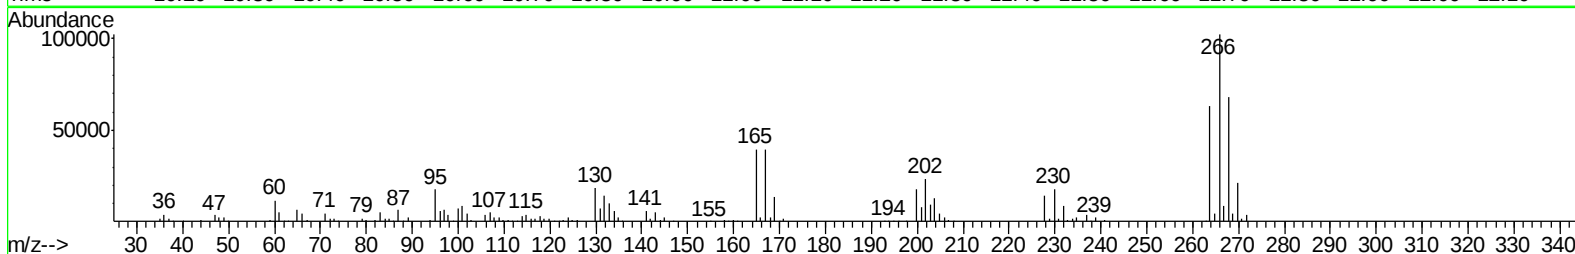


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040320\
Data File : BF119728.D
Acq On : 3 Apr 2020 19:47
Operator : MA/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 00:04:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 01 11:59:45 2020
Response via : Initial Calibration

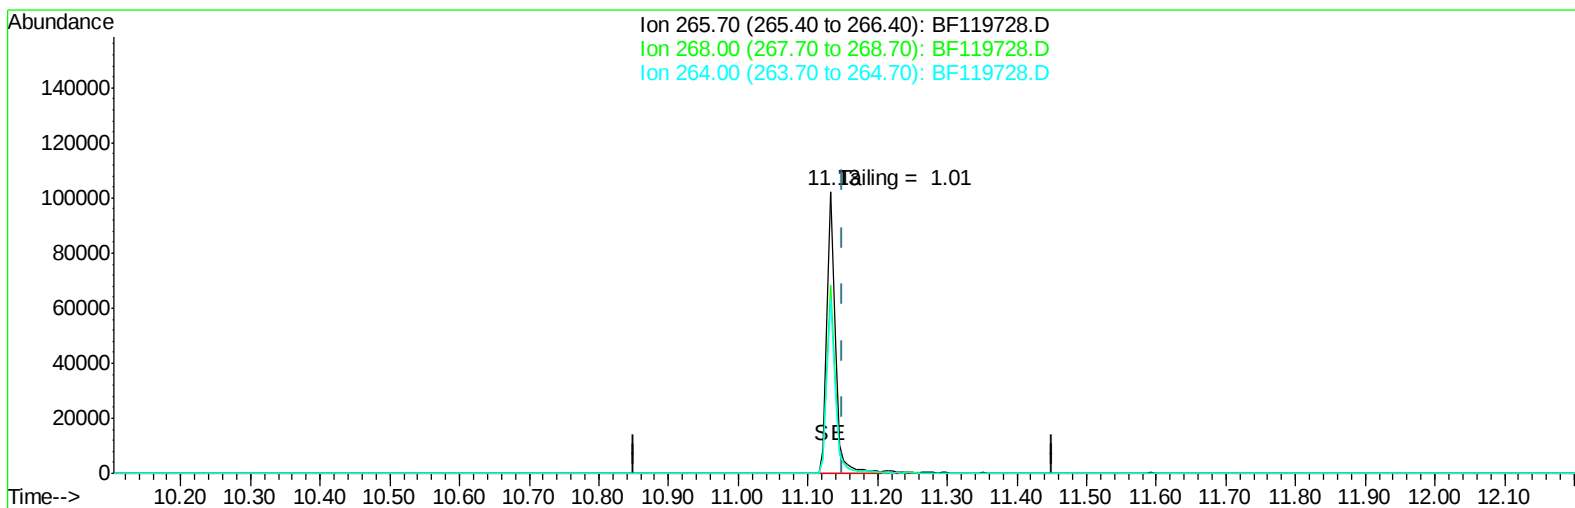

TIC: BF119728.D

(70) Pentachlorophenol (C)




11.133min (-0.018) 31272.10ng

response 85493

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	66.67
264.00	61.20	61.70
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040320\
 Data File : BF119728.D
 Acq On : 3 Apr 2020 19:47
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 00:04:46 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 01 11:59:45 2020
 Response via : Initial Calibration

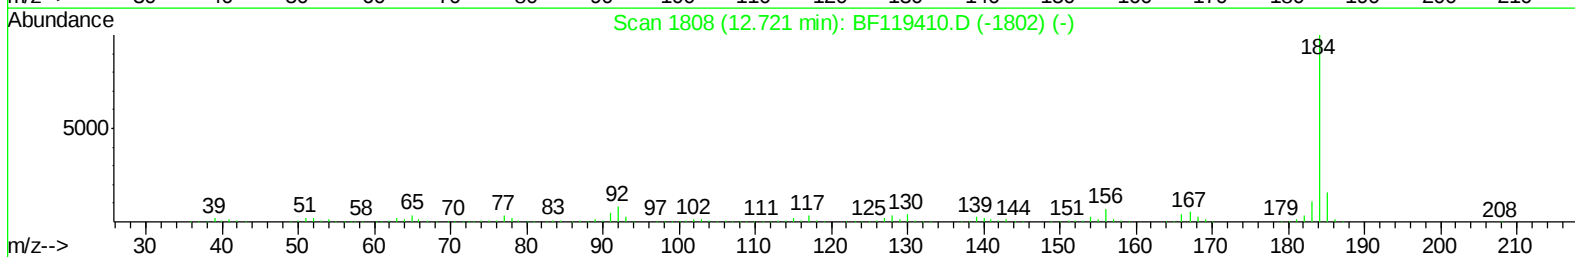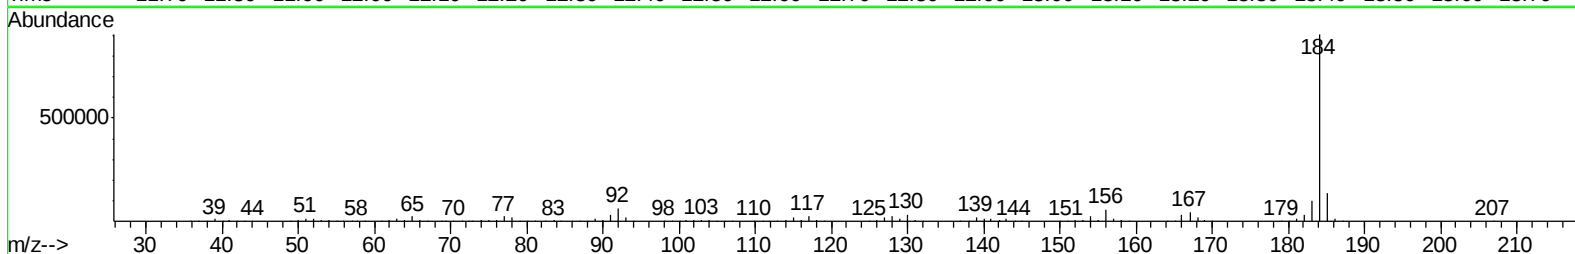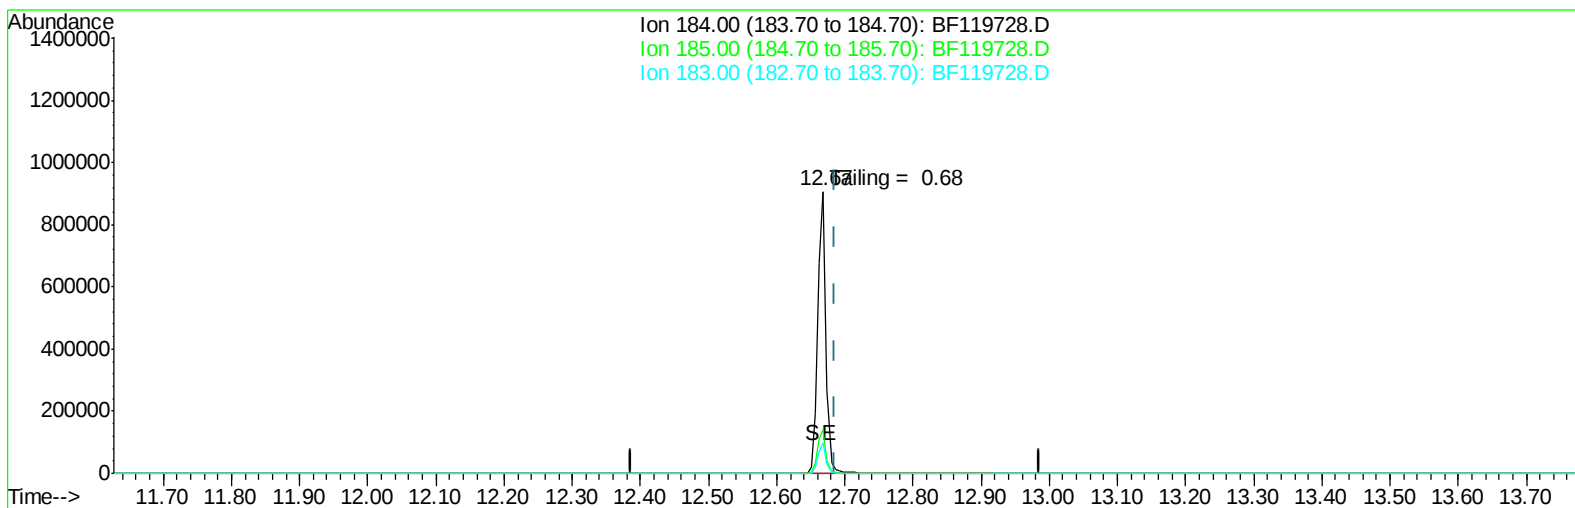

TIC: BF119728.D

(77) Benzidine

12.668min (-0.018) 0.00ng

response 760280

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	15.30
183.00	11.30	11.00
0.00	0.00	0.00