
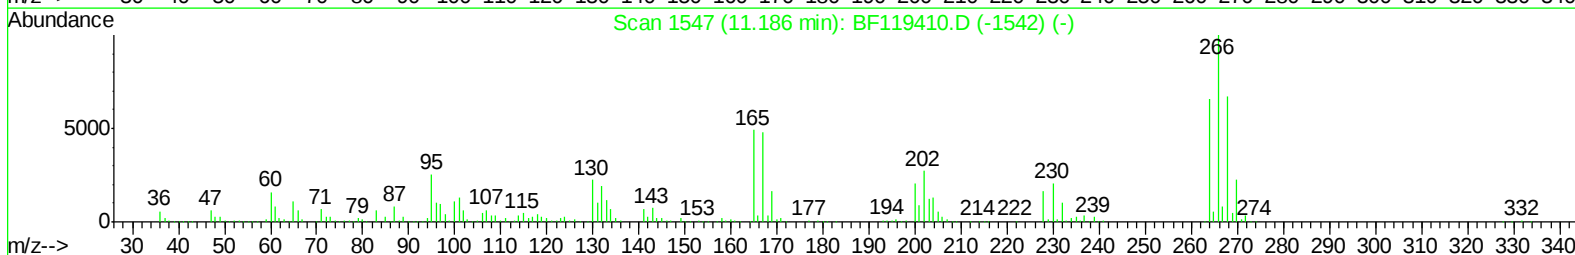
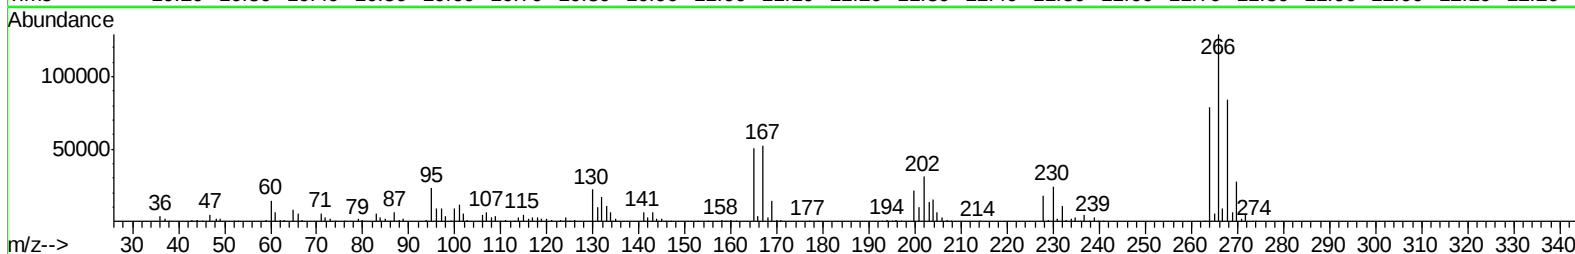


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040320\
Data File : BF119739.D
Acq On : 4 Apr 2020 2:10
Operator : MA/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 02:45:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 01 11:59:45 2020
Response via : Initial Calibration

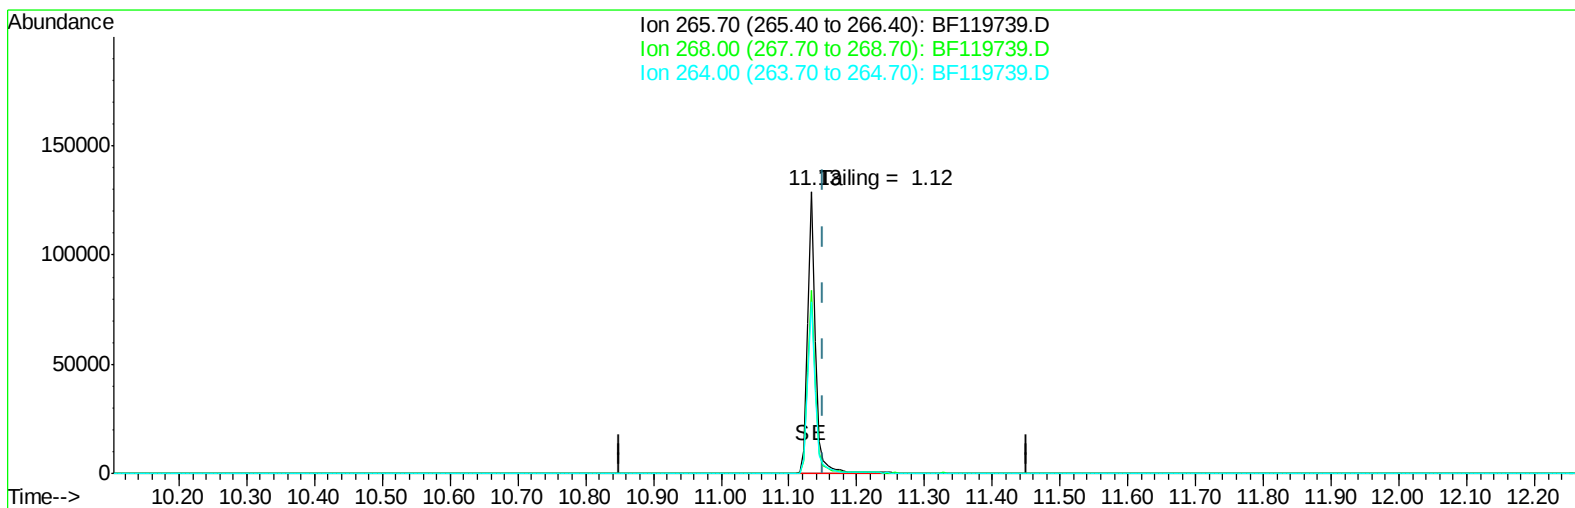

TIC: BF119739.D

(70) Pentachlorophenol (C)




11.133min (-0.018) 29810.69ng

response 108392

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	64.91
264.00	61.20	61.04
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040320\
Data File : BF119739.D
Acq On : 4 Apr 2020 2:10
Operator : MA/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 02:45:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 01 11:59:45 2020
Response via : Initial Calibration

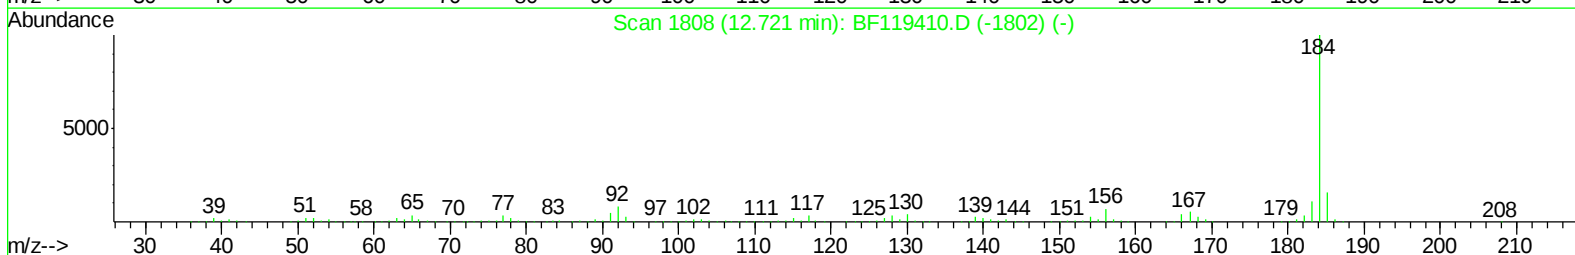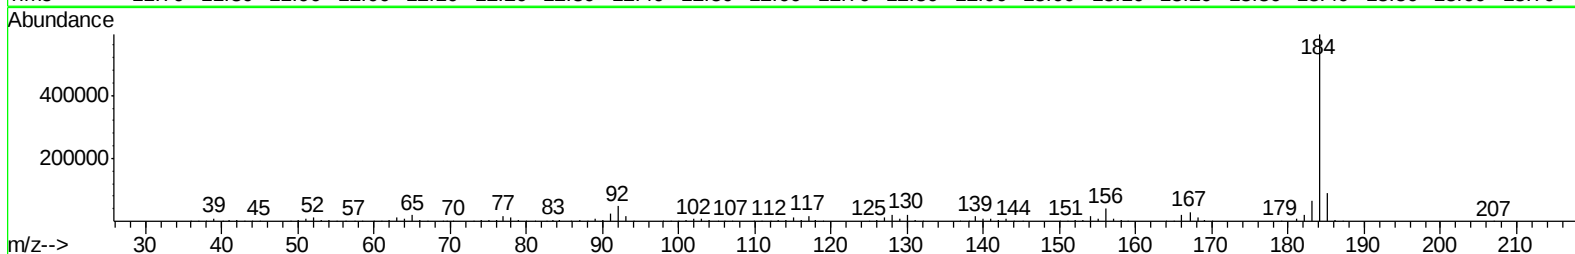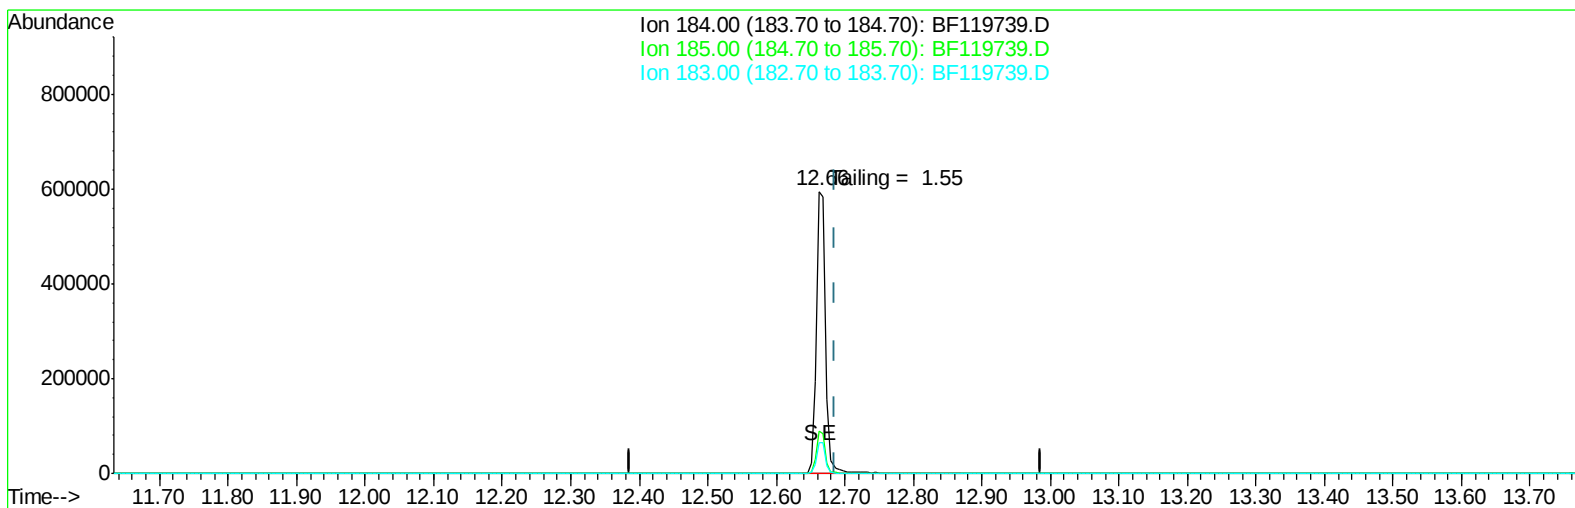

TIC: BF119739.D

(77) Benzidine

12.663min (-0.024) 0.00ng

response 573125

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	14.97
183.00	11.30	11.07
0.00	0.00	0.00