

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF040320\
 Data File : BF119720.D
 Acq On : 3 Apr 2020 15:41
 Operator : MA/SJ
 Sample : L2107-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 S32-MULTI-IDW01

Quant Time: Apr 03 16:13:49 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF031820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 01 11:59:45 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.80	152	222172	20.00	ng	-0.01
21) Naphthalene-d8	8.09	136	840029	20.00	ng	-0.02
39) Acenaphthene-d10	9.85	164	426117	20.00	ng	-0.02
64) Phenanthrene-d10	11.33	188	832523	20.00	ng	-0.02
76) Chrysene-d12	13.97	240	660030	20.00	ng	-0.02
87) Perylene-d12	15.43	264	610532	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.44	112	1814362	130.00	ng	0.02
7) Phenol-d6	6.44	99	2105547	118.10	ng	0.00
23) Nitrobenzene-d5	7.37	82	1547038	100.09	ng	-0.01
42) 2,4,6-Tribromophenol	10.64	330	707688	160.98	ng	-0.01
45) 2-Fluorobiphenyl	9.17	172	2760911	95.99	ng	-0.01
79) Terphenyl-d14	12.93	244	3162262	93.87	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF040320\
Data File : BF119720.D
Acq On : 3 Apr 2020 15:41
Operator : MA/SJ
Sample : L2107-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S32-MULTI-IDW01

Quant Time: Apr 03 16:13:49 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF031820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 01 11:59:45 2020
Response via : Initial Calibration

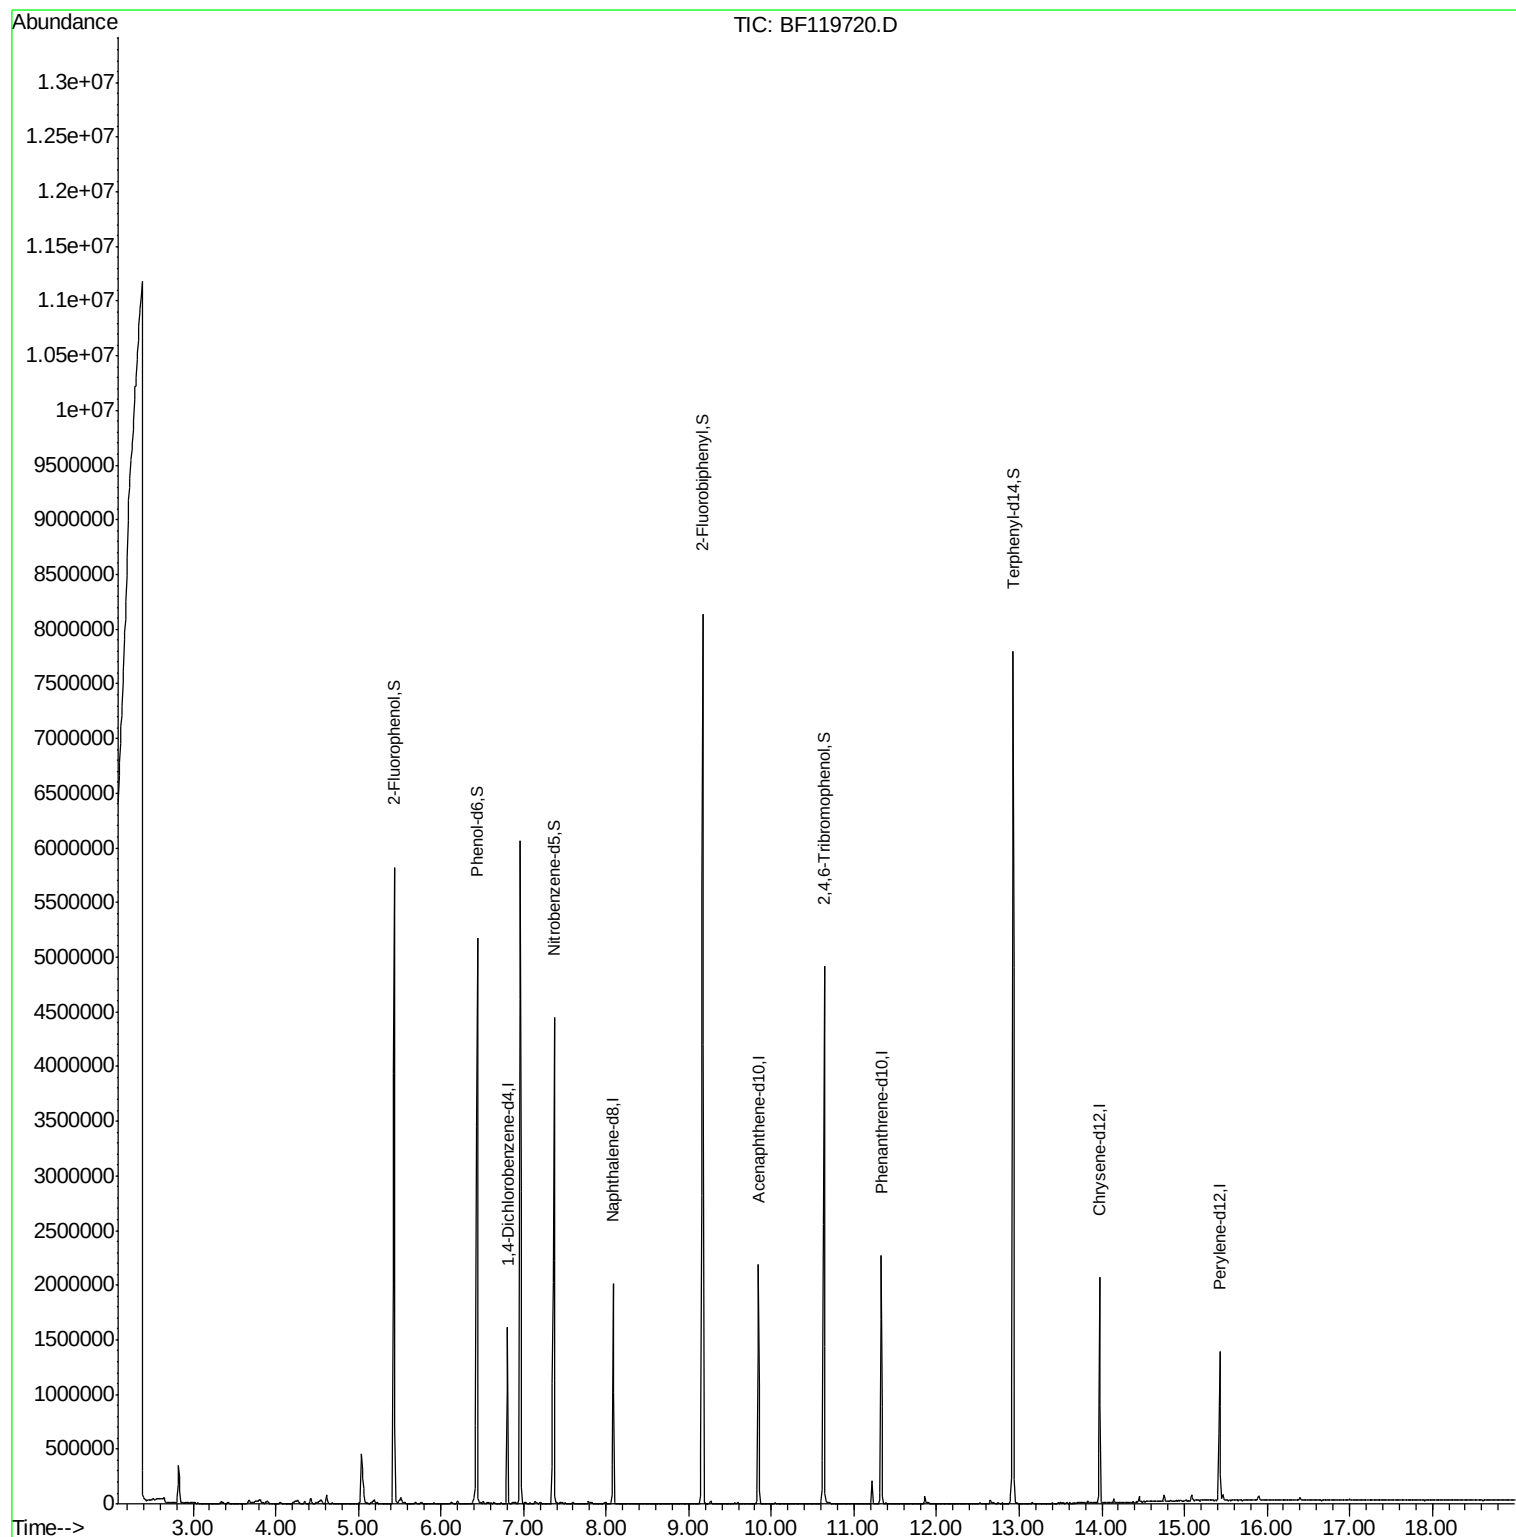

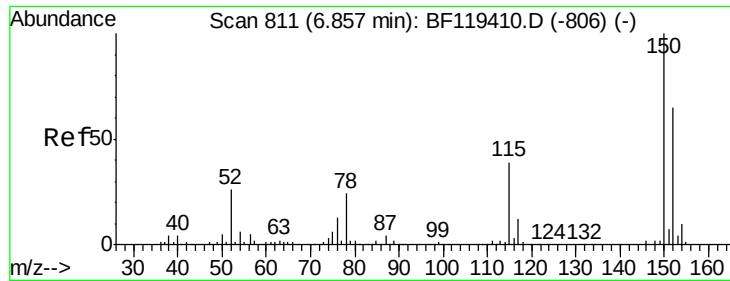


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.80 min Scan# 802
Delta R.T. -0.01 min
Lab File: BF119720.D
Acq: 3 Apr 2020 15:41

Instrument :
BNA_F
ClientSampleId :
S32-MULTI-IDW01

Tot Ion:152 Resp: 222172
Ion Ratio Lower Upper
152 100
150 157.6 124.5 186.7
115 58.6 49.6 74.4

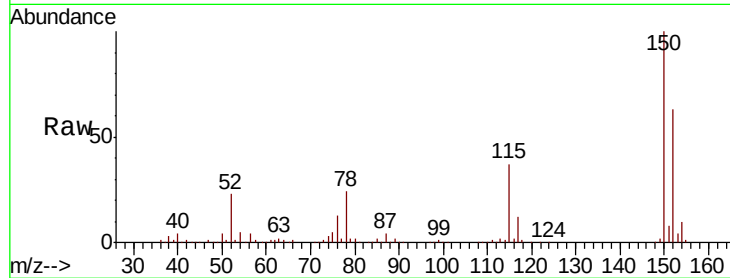


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

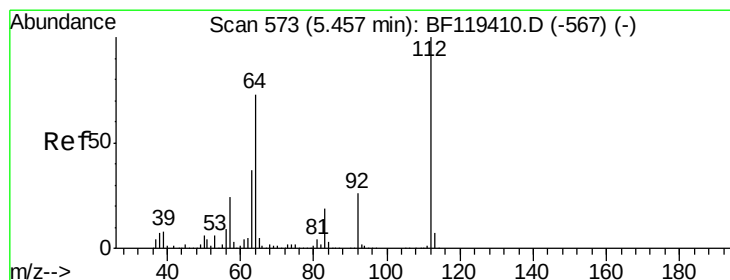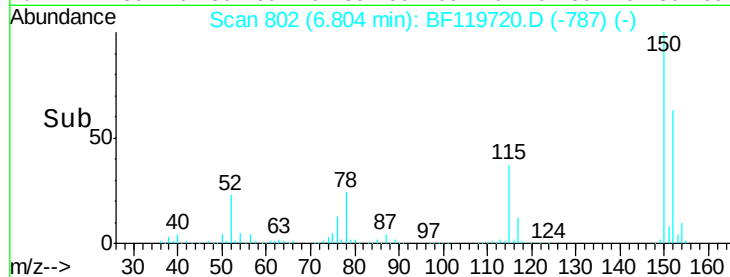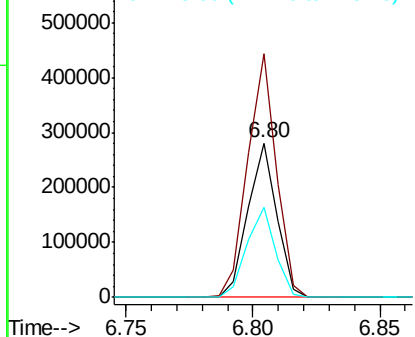



#5


2-Fluorophenol
Concen: 130.003 ng
RT: 5.44 min Scan# 570
Delta R.T. 0.02 min
Lab File: BF119720.D
Acq: 3 Apr 2020 15:41

Tgt Ion:112 Resp: 1814362
Ion Ratio Lower Upper
112 100
64 65.3 56.7 85.1
63 33.4 29.5 44.3

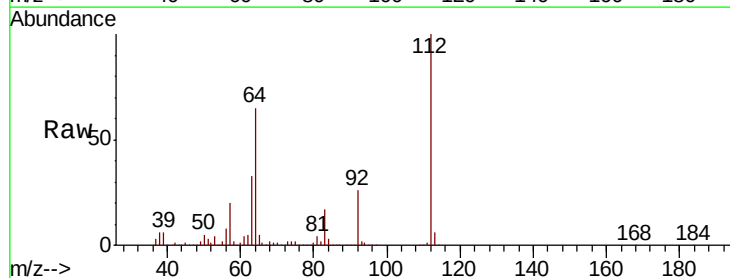

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

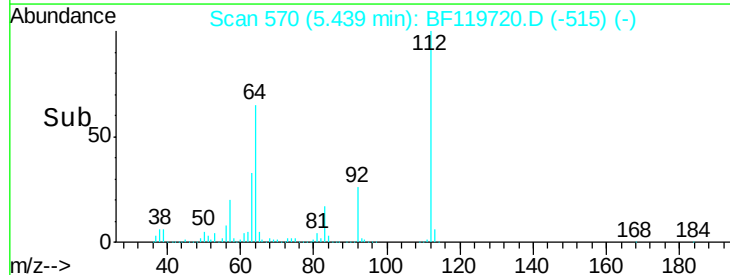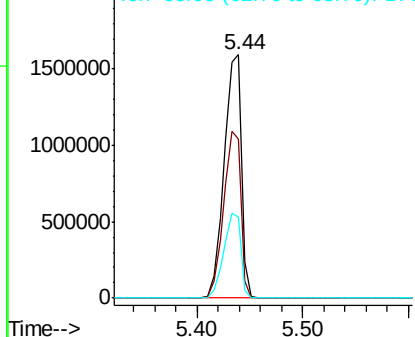

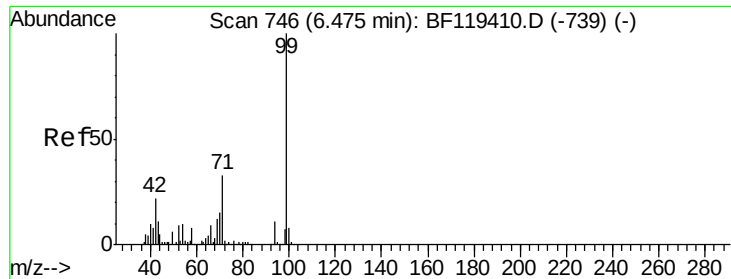

#7

Phenol-d6

Concen: 118.102 ng

RT: 6.44 min Scan# 740

Delta R.T. -0.01 min

Lab File: BF119720.D

Acq: 3 Apr 2020 15:41

Instrument :

BNA_F

ClientSampleId :

S32-MULTI-IDW01


Tot Ion: 99 Resp: 2105547

Ion Ratio Lower Upper




99 100

42 17.9 16.6 24.8

71 31.5 26.4 39.6

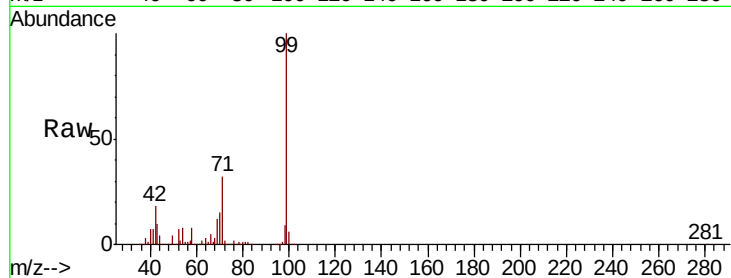

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

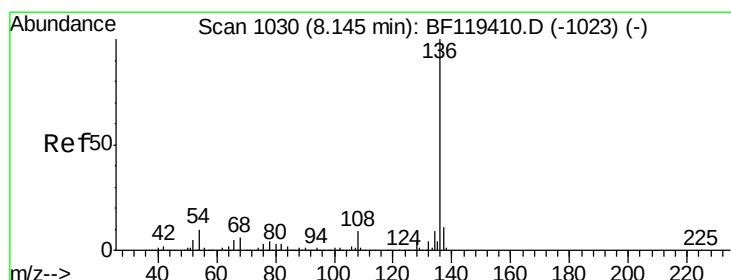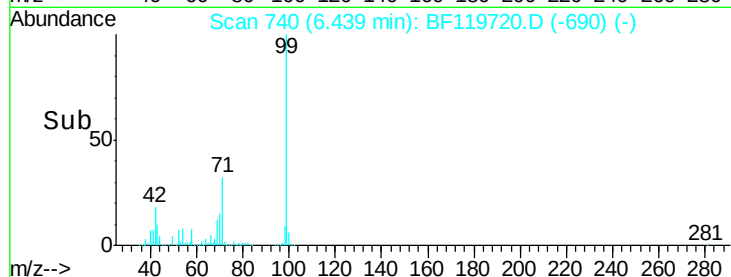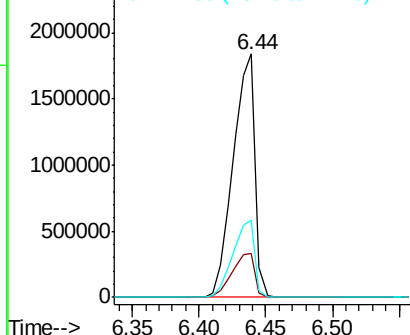

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.09 min Scan# 1020

Delta R.T. -0.02 min

Lab File: BF119720.D

Acq: 3 Apr 2020 15:41

Tgt Ion: 136 Resp: 840029


Ion Ratio Lower Upper

136 100



137 11.0 8.7 13.1


54 10.3 9.1 13.7

68 5.8 4.6 6.8

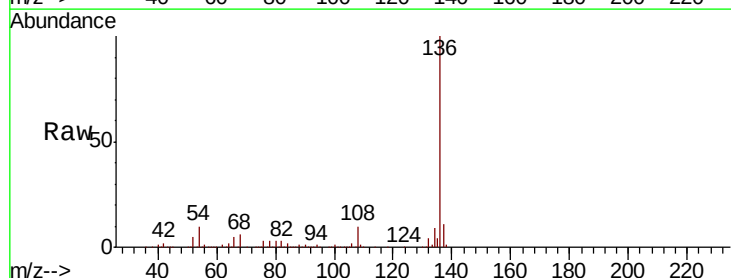

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

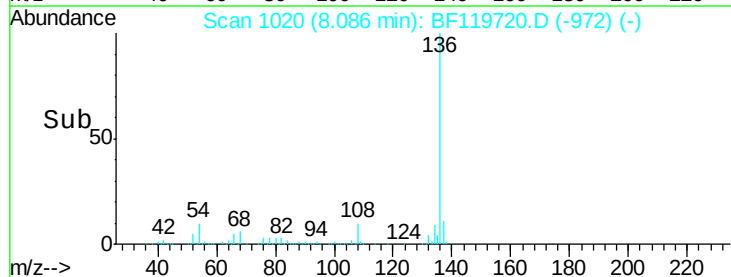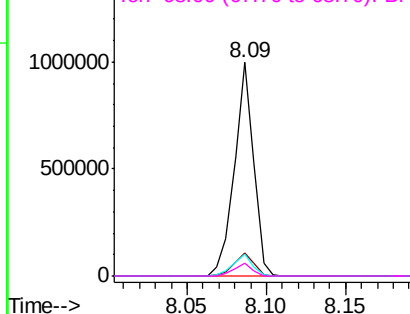


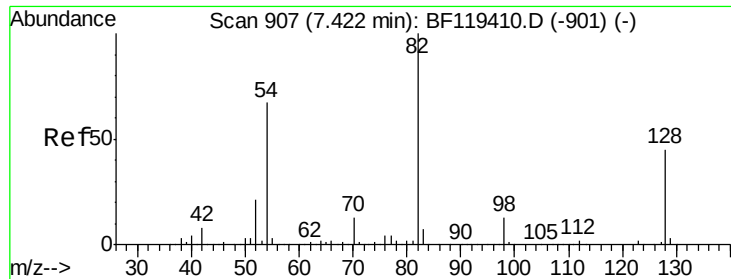




#23
 Nitrobenzene-d5
 Concen: 100.090 ng
 RT: 7.37 min Scan# 898
 Delta R.T. -0.01 min
 Lab File: BF119720.D
 Acq: 3 Apr 2020 15:41

Instrument :
 BNA_F
 ClientSampleId :
 S32-MULTI-IDW01

Tot Ion: 82 Resp: 1547038
 Ion Ratio Lower Upper
 82 100
 128 46.0 36.3 54.5
 54 61.0 50.6 75.8

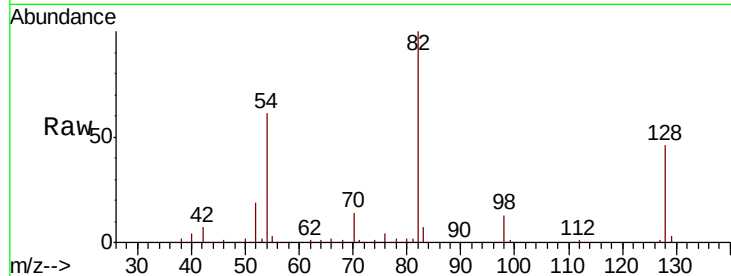


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1

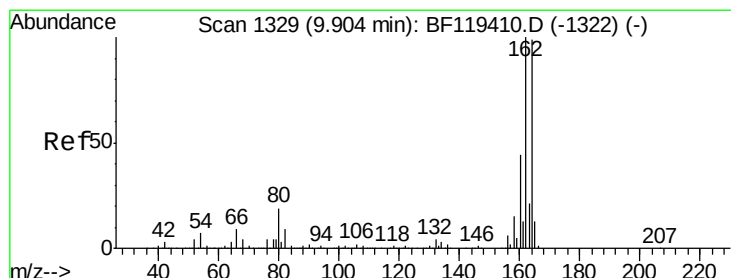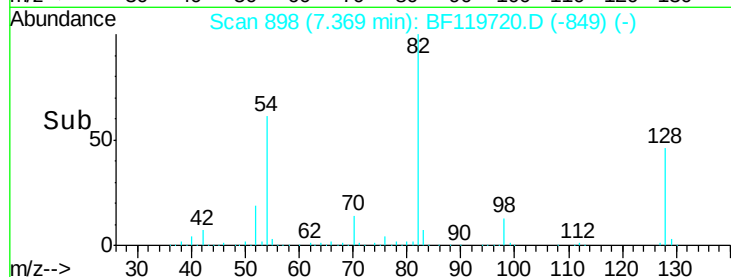
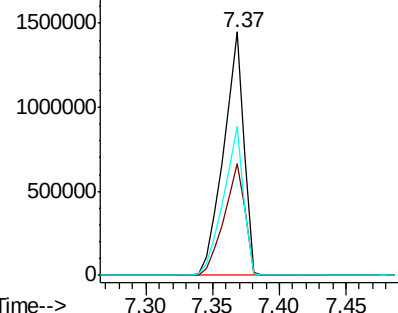



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.85 min Scan# 1319
 Delta R.T. -0.02 min
 Lab File: BF119720.D
 Acq: 3 Apr 2020 15:41

Tgt Ion: 164 Resp: 426117
 Ion Ratio Lower Upper
 164 100
 162 103.9 80.6 121.0
 160 45.4 35.7 53.5

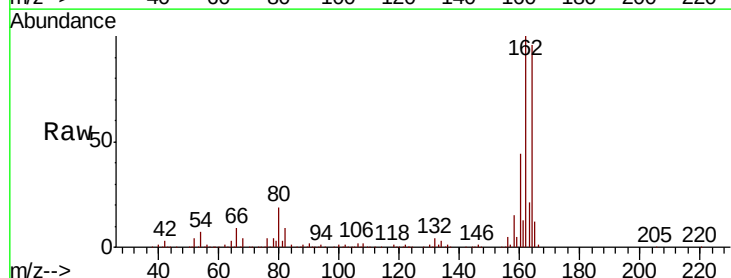

Abundance Ion 164.00 (163.70 to 164.70): BF1
 Ion 162.00 (161.70 to 162.70): BF1
 Ion 160.00 (159.70 to 160.70): BF1

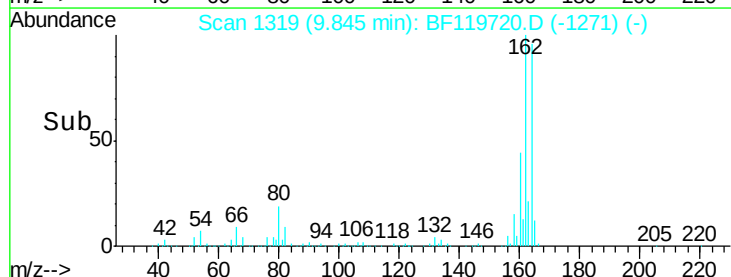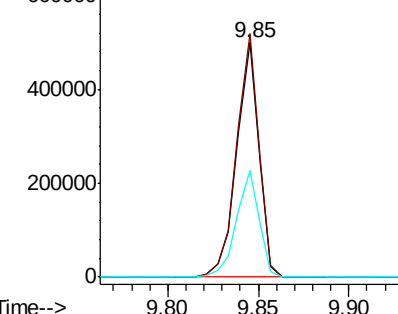

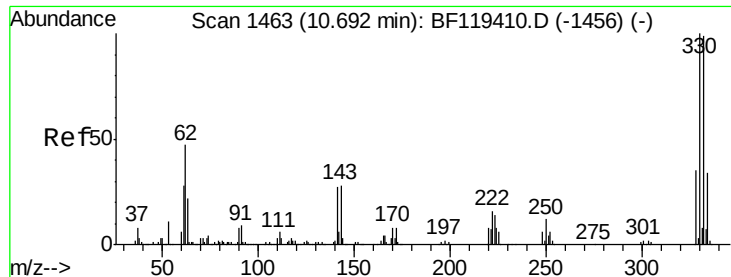

#42

2,4,6-Tribromophenol

Concen: 160.981 ng

RT: 10.64 min Scan# 1454

Delta R.T. -0.01 min

Lab File: BF119720.D

Acq: 3 Apr 2020 15:41

Instrument :

BNA_F

ClientSampleId :

S32-MULTI-IDW01


Tot Ion:330 Resp: 707688

Ion Ratio Lower Upper

330 100

332 96.9 75.7 113.5




141 30.2 25.4 38.0

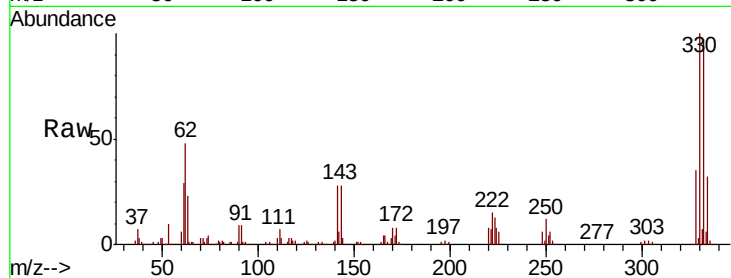

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

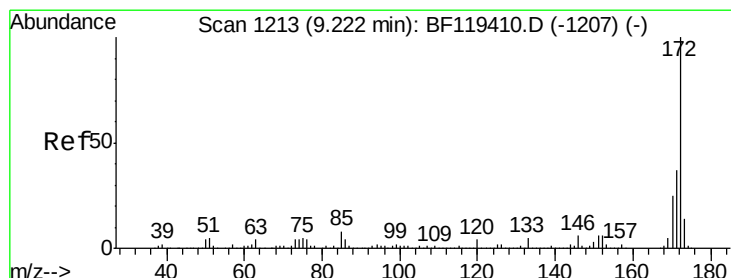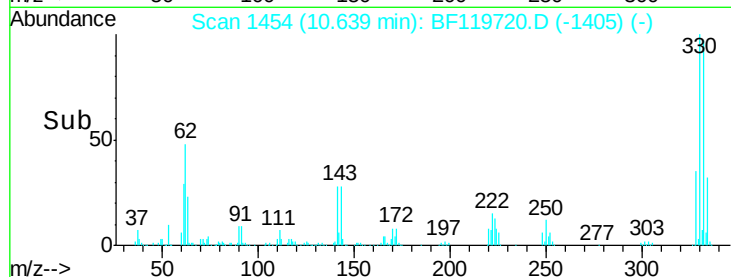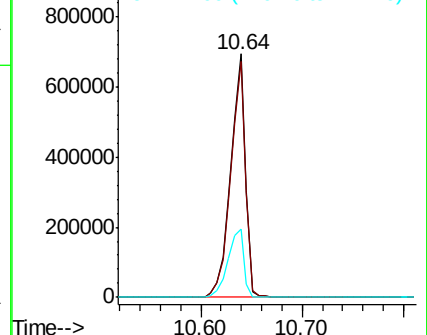

#45

2-Fluorobiphenyl

Concen: 95.988 ng

RT: 9.17 min Scan# 1204

Delta R.T. -0.01 min

Lab File: BF119720.D

Acq: 3 Apr 2020 15:41


Tgt Ion:172 Resp: 2760911

Ion Ratio Lower Upper

172 100

171 37.6 29.6 44.4



170 24.8 20.2 30.2

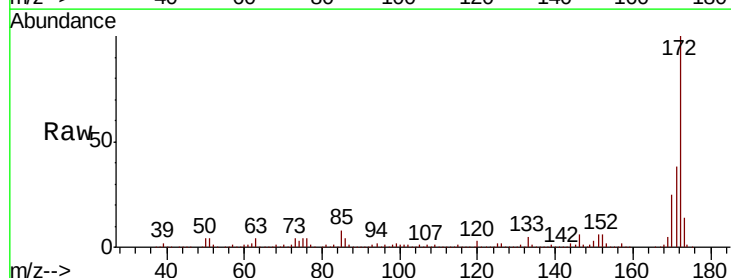


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



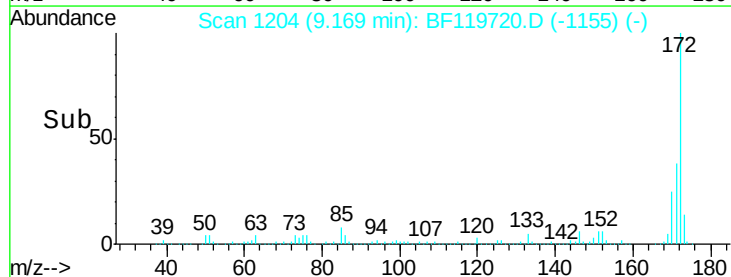
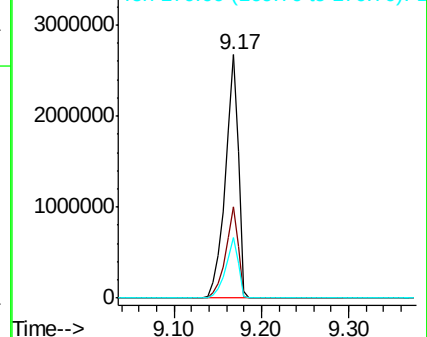


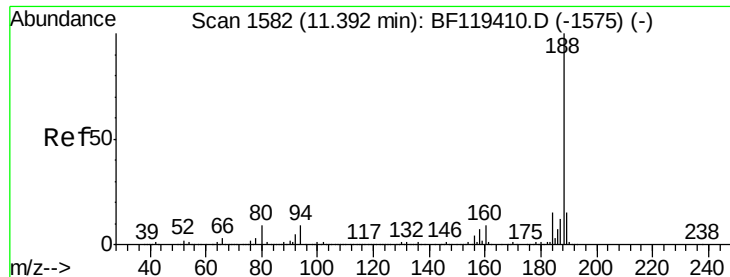

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.33 min Scan# 1572
Delta R.T. -0.02 min
Lab File: BF119720.D
Acq: 3 Apr 2020 15:41




Instrument :
BNA_F
ClientSampleId :
S32-MULTI-IDW01


Tot Ion:188 Resp: 832523
Ion Ratio Lower Upper
188 100
94 9.1 7.5 11.3
80 9.7 9.0 13.4

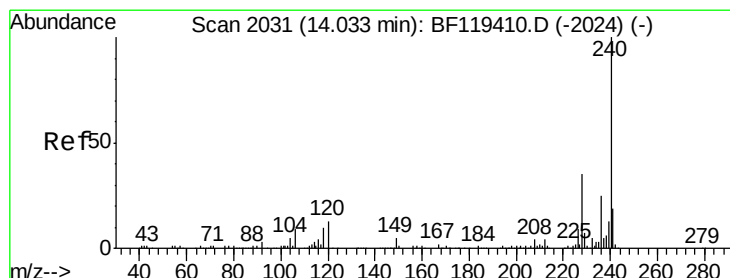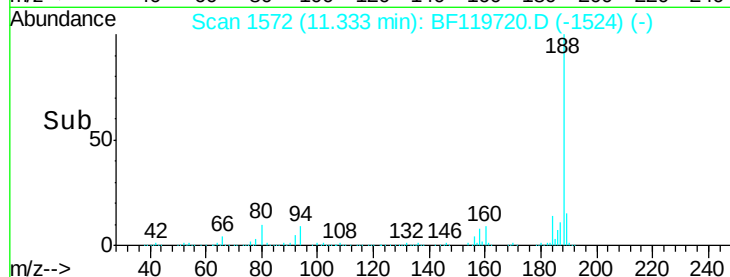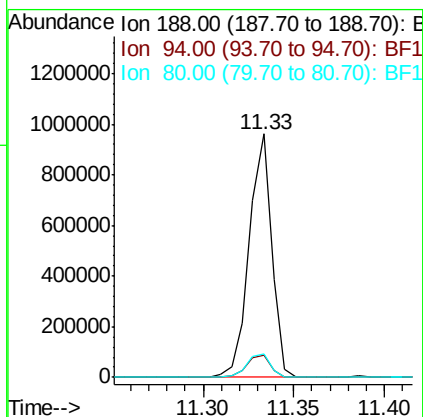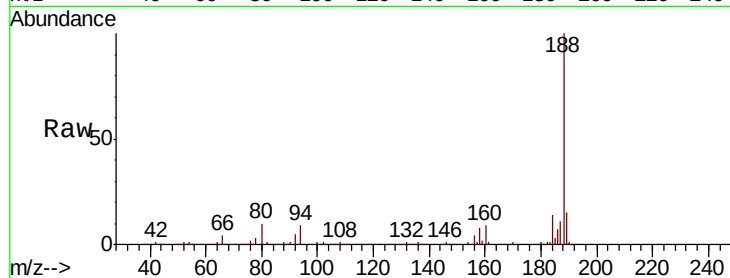

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.97 min Scan# 2021
Delta R.T. -0.02 min
Lab File: BF119720.D
Acq: 3 Apr 2020 15:41

Tgt Ion:240 Resp: 660030
Ion Ratio Lower Upper
240 100
120 11.3 10.6 15.8
236 25.6 20.2 30.2

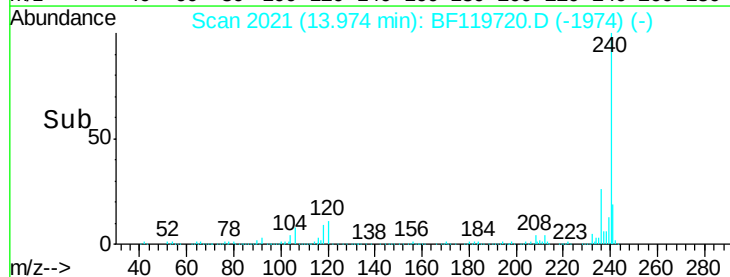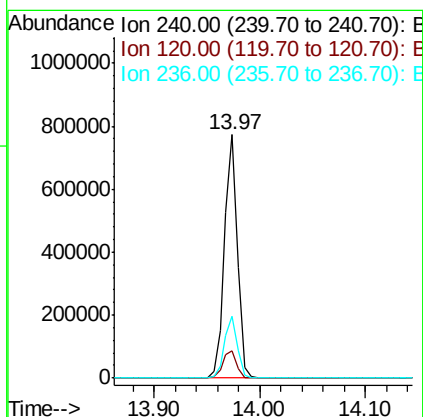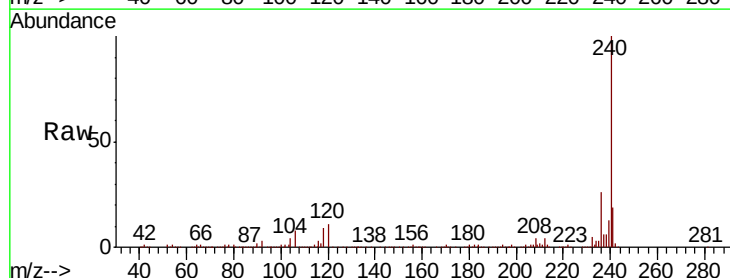

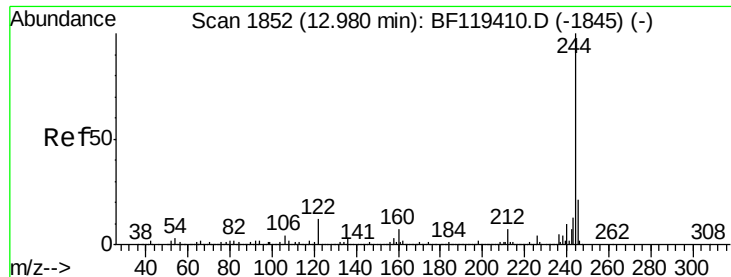

#79

Terphenyl-d14

Concen: 93.868 ng

RT: 12.93 min Scan# 1843

Delta R.T. -0.01 min

Lab File: BF119720.D

Acq: 3 Apr 2020 15:41

Instrument :

BNA_F

ClientSampleId :

S32-MULTI-IDW01


Tot Ion:244 Resp: 3162262

Ion Ratio Lower Upper

244 100

212 6.9 5.8 8.8




122 13.1 10.3 15.5

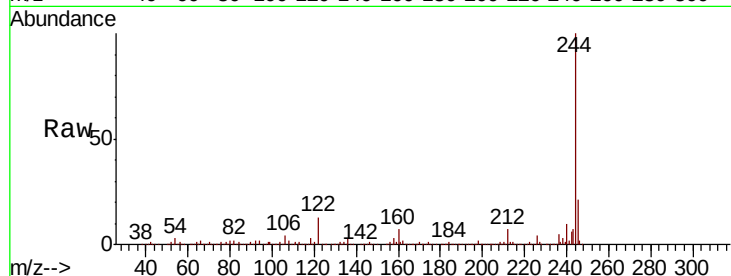

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

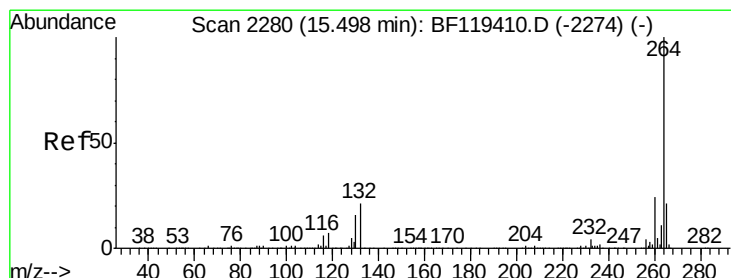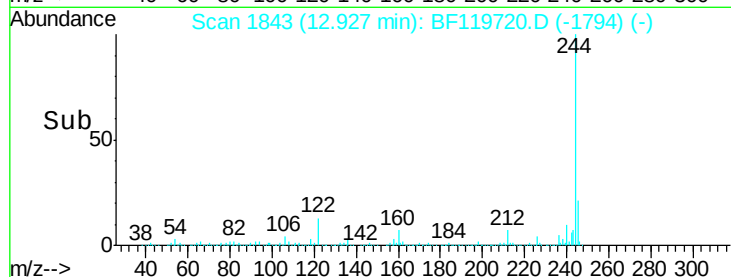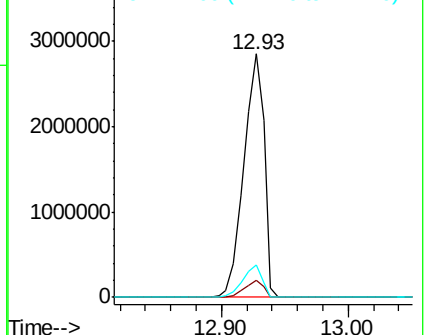

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.43 min Scan# 2268

Delta R.T. -0.02 min

Lab File: BF119720.D

Acq: 3 Apr 2020 15:41


Tgt Ion:264 Resp: 610532

Ion Ratio Lower Upper

264 100

260 22.7 18.7 28.1

265 21.5 17.7 26.5

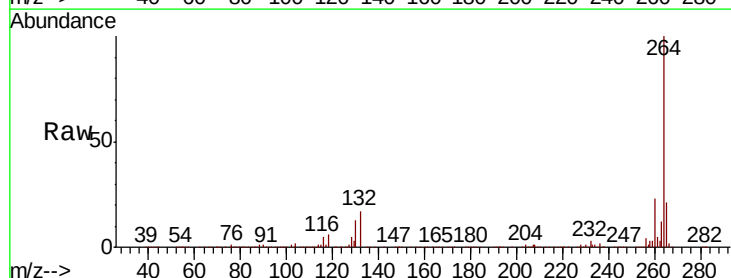

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

