


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040320\
 Data File : BF119707.D
 Acq On : 3 Apr 2020 9:17
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 01 11:59:45 2020

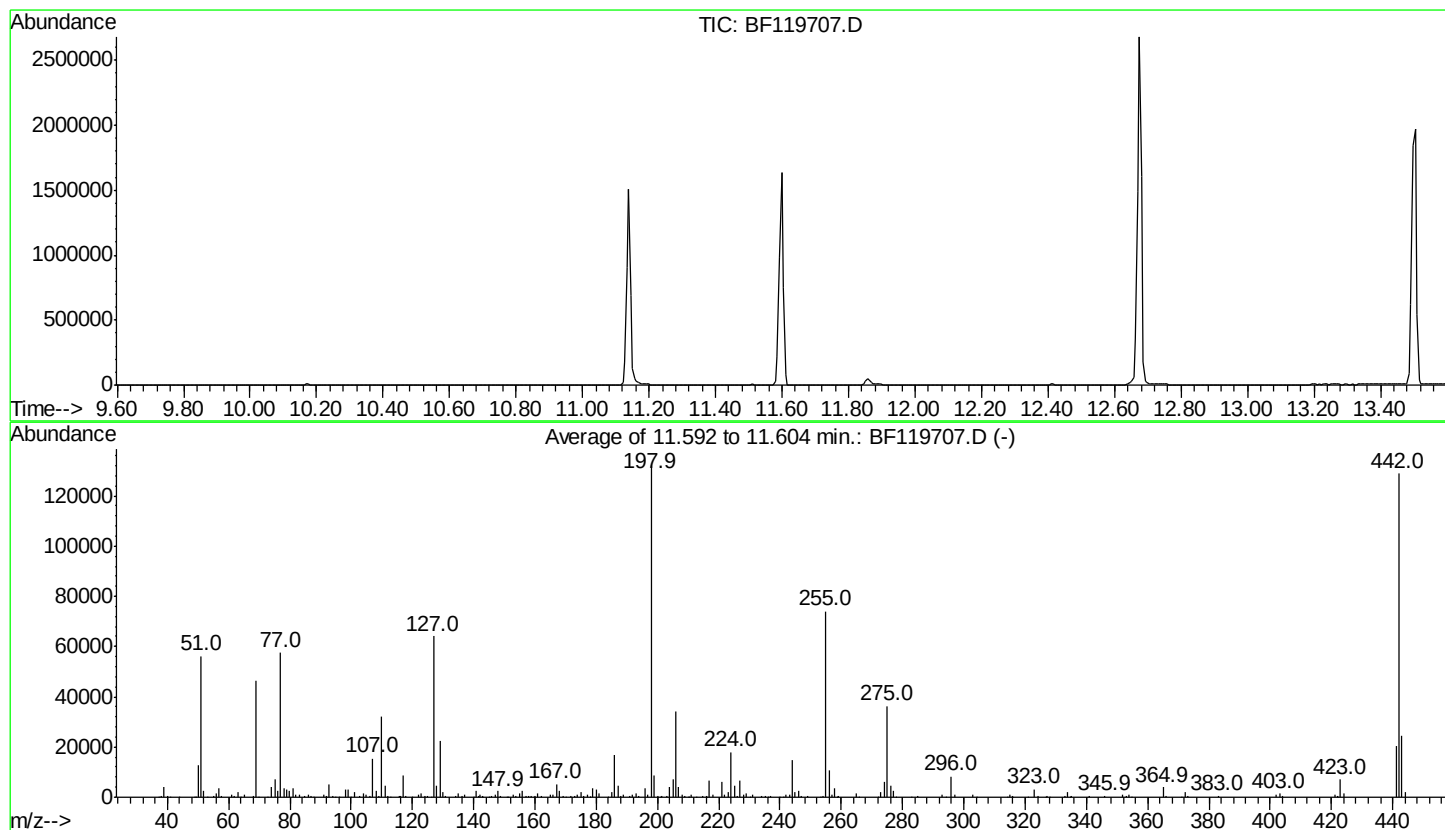

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.7	56317	PASS
68	69	0.00	2	1.6	726	PASS
69	198	0.00	100	35.3	46640	PASS
70	69	0.00	2	0.4	196	PASS
127	198	10	80	48.5	63976	PASS
197	198	0.00	2	0.7	882	PASS
198	198	100	100	100.0	132021	PASS
199	198	5	9	6.7	8805	PASS
275	198	10	60	27.6	36410	PASS
365	198	1	100	2.9	3889	PASS
441	198	0.01	100	15.5	20495	PASS
442	198	50	100	97.7	129032	PASS
443	442	15	24	19.0	24549	PASS