


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040320\
 Data File : BF119728.D
 Acq On : 3 Apr 2020 19:47
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 06 11:15:16 2020

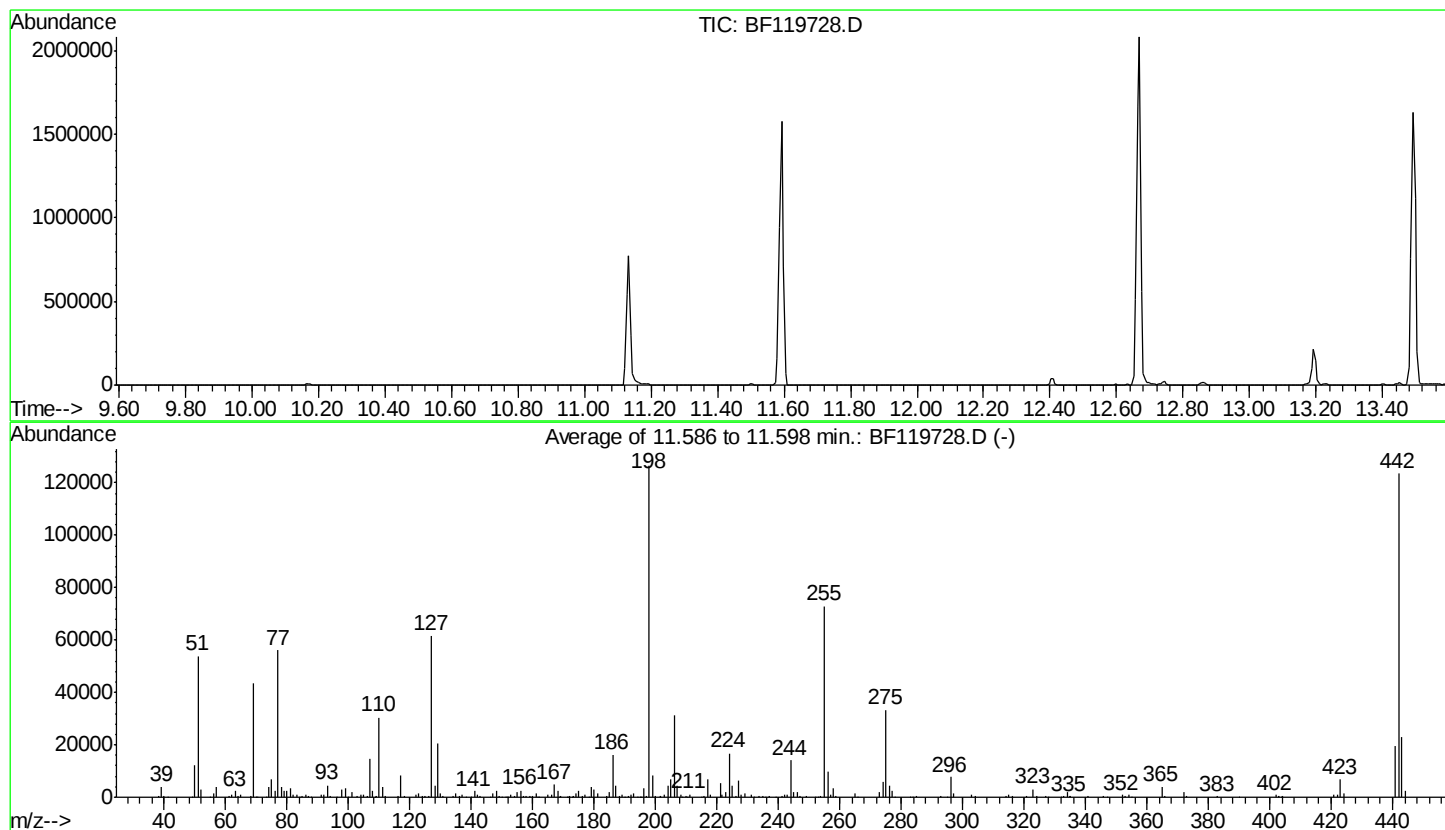

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.7	53976	PASS
68	69	0.00	2	1.5	635	PASS
69	198	0.00	100	34.2	43250	PASS
70	69	0.00	2	0.3	120	PASS
127	198	10	80	48.7	61650	PASS
197	198	0.00	2	0.3	418	PASS
198	198	100	100	100.0	126549	PASS
199	198	5	9	6.5	8273	PASS
275	198	10	60	26.4	33426	PASS
365	198	1	100	3.2	4036	PASS
441	198	0.01	100	15.4	19551	PASS
442	198	50	100	97.6	123554	PASS
443	442	15	24	18.7	23107	PASS