


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040320\
 Data File : BF119739.D
 Acq On : 4 Apr 2020 2:10
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 06 11:15:16 2020

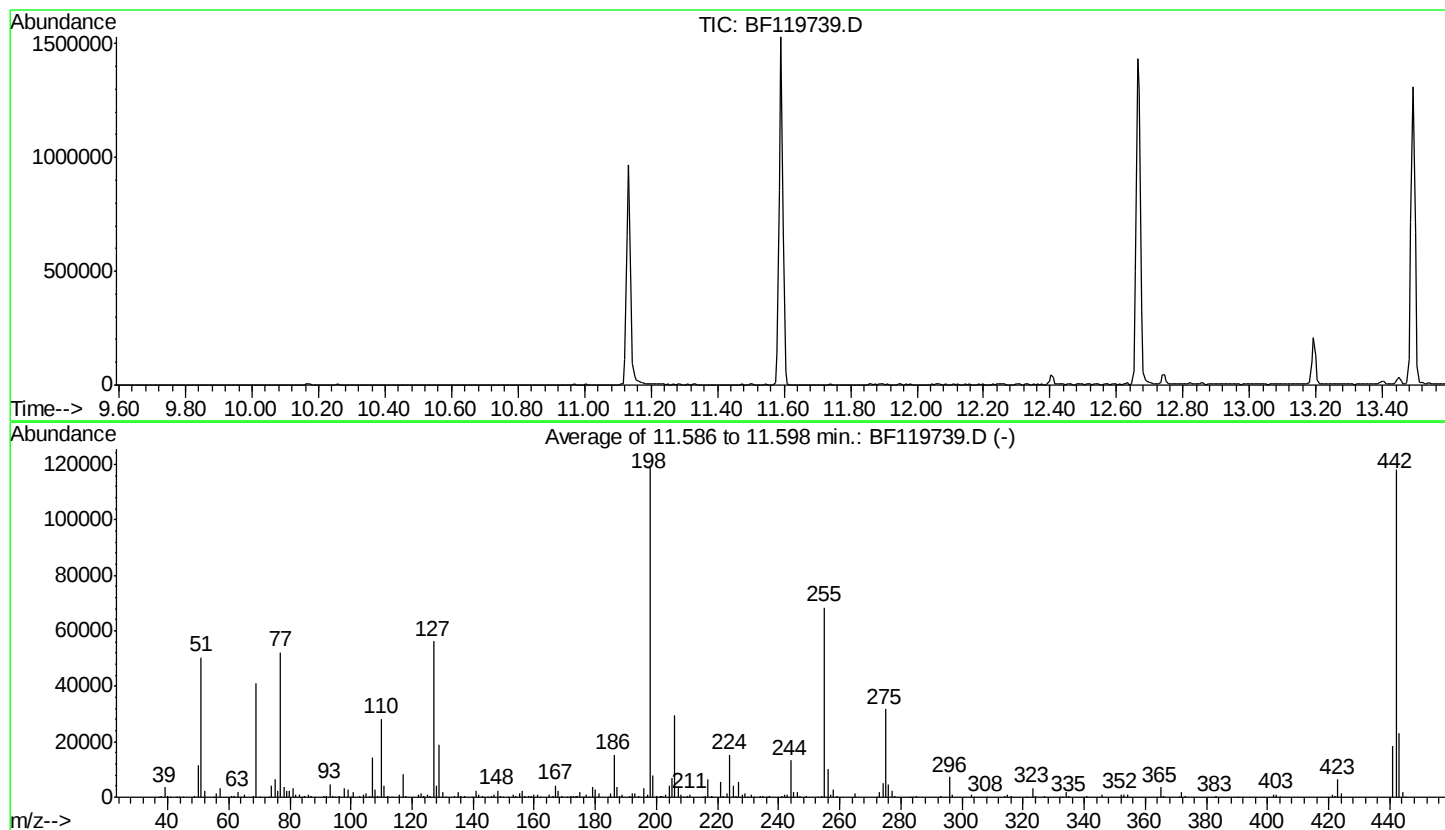

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.2	50389	PASS
68	69	0.00	2	1.6	652	PASS
69	198	0.00	100	34.5	41228	PASS
70	69	0.00	2	0.2	103	PASS
127	198	10	80	47.1	56282	PASS
197	198	0.00	2	0.7	797	PASS
198	198	100	100	100.0	119533	PASS
199	198	5	9	6.7	7976	PASS
275	198	10	60	26.6	31752	PASS
365	198	1	100	3.1	3668	PASS
441	198	0.01	100	15.3	18346	PASS
442	198	50	100	98.8	118056	PASS
443	442	15	24	19.4	22868	PASS