

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF040419\
 Data File : BF113590.D
 Acq On : 4 Apr 2019 18:39
 Operator : JU/SJ
 Sample : K2221-08
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Apr 05 01:32:04 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 04 04:05:31 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.68	152	118777	20.00	ng	0.00
21) Naphthalene-d8	7.96	136	446623	20.00	ng	0.00
39) Acenaphthene-d10	9.71	164	220123	20.00	ng	-0.01
64) Phenanthrene-d10	11.19	188	475197	20.00	ng	-0.02
76) Chrysene-d12	13.82	240	454587	20.00	ng	-0.03
87) Perylene-d12	15.22	264	396441	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.30	112	831036	119.31	ng	0.00
7) Phenol-d6	6.33	99	928913	108.20	ng	0.00
23) Nitrobenzene-d5	7.25	82	753994	98.89	ng	-0.01
42) 2,4,6-Tribromophenol	10.50	330	424735	160.63	ng	-0.01
45) 2-Fluorobiphenyl	9.04	172	1388460	101.55	ng	-0.01
79) Terphenyl-d14	12.77	244	1826297	81.80	ng	-0.02
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.25	70	97975	18.507	ng	# 77
25) Isophorone	7.25	82	753988	51.333	ng	# 64
50) Dimethylphthalate	9.71	163	56506	3.482	ng	# 1
51) 2,6-Dinitrotoluene	9.71	165	28282	7.907	ng	# 27
57) 2,4-Dinitrotoluene	9.71	165	28282	6.538	ng	# 24
67) 4-Bromophenyl-phenylether	10.50	248	24530	4.603	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF040419\
Data File : BF113590.D
Acq On : 4 Apr 2019 18:39
Operator : JU/SJ
Sample : K2221-08
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Apr 05 01:32:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 04 04:05:31 2019
Response via : Initial Calibration

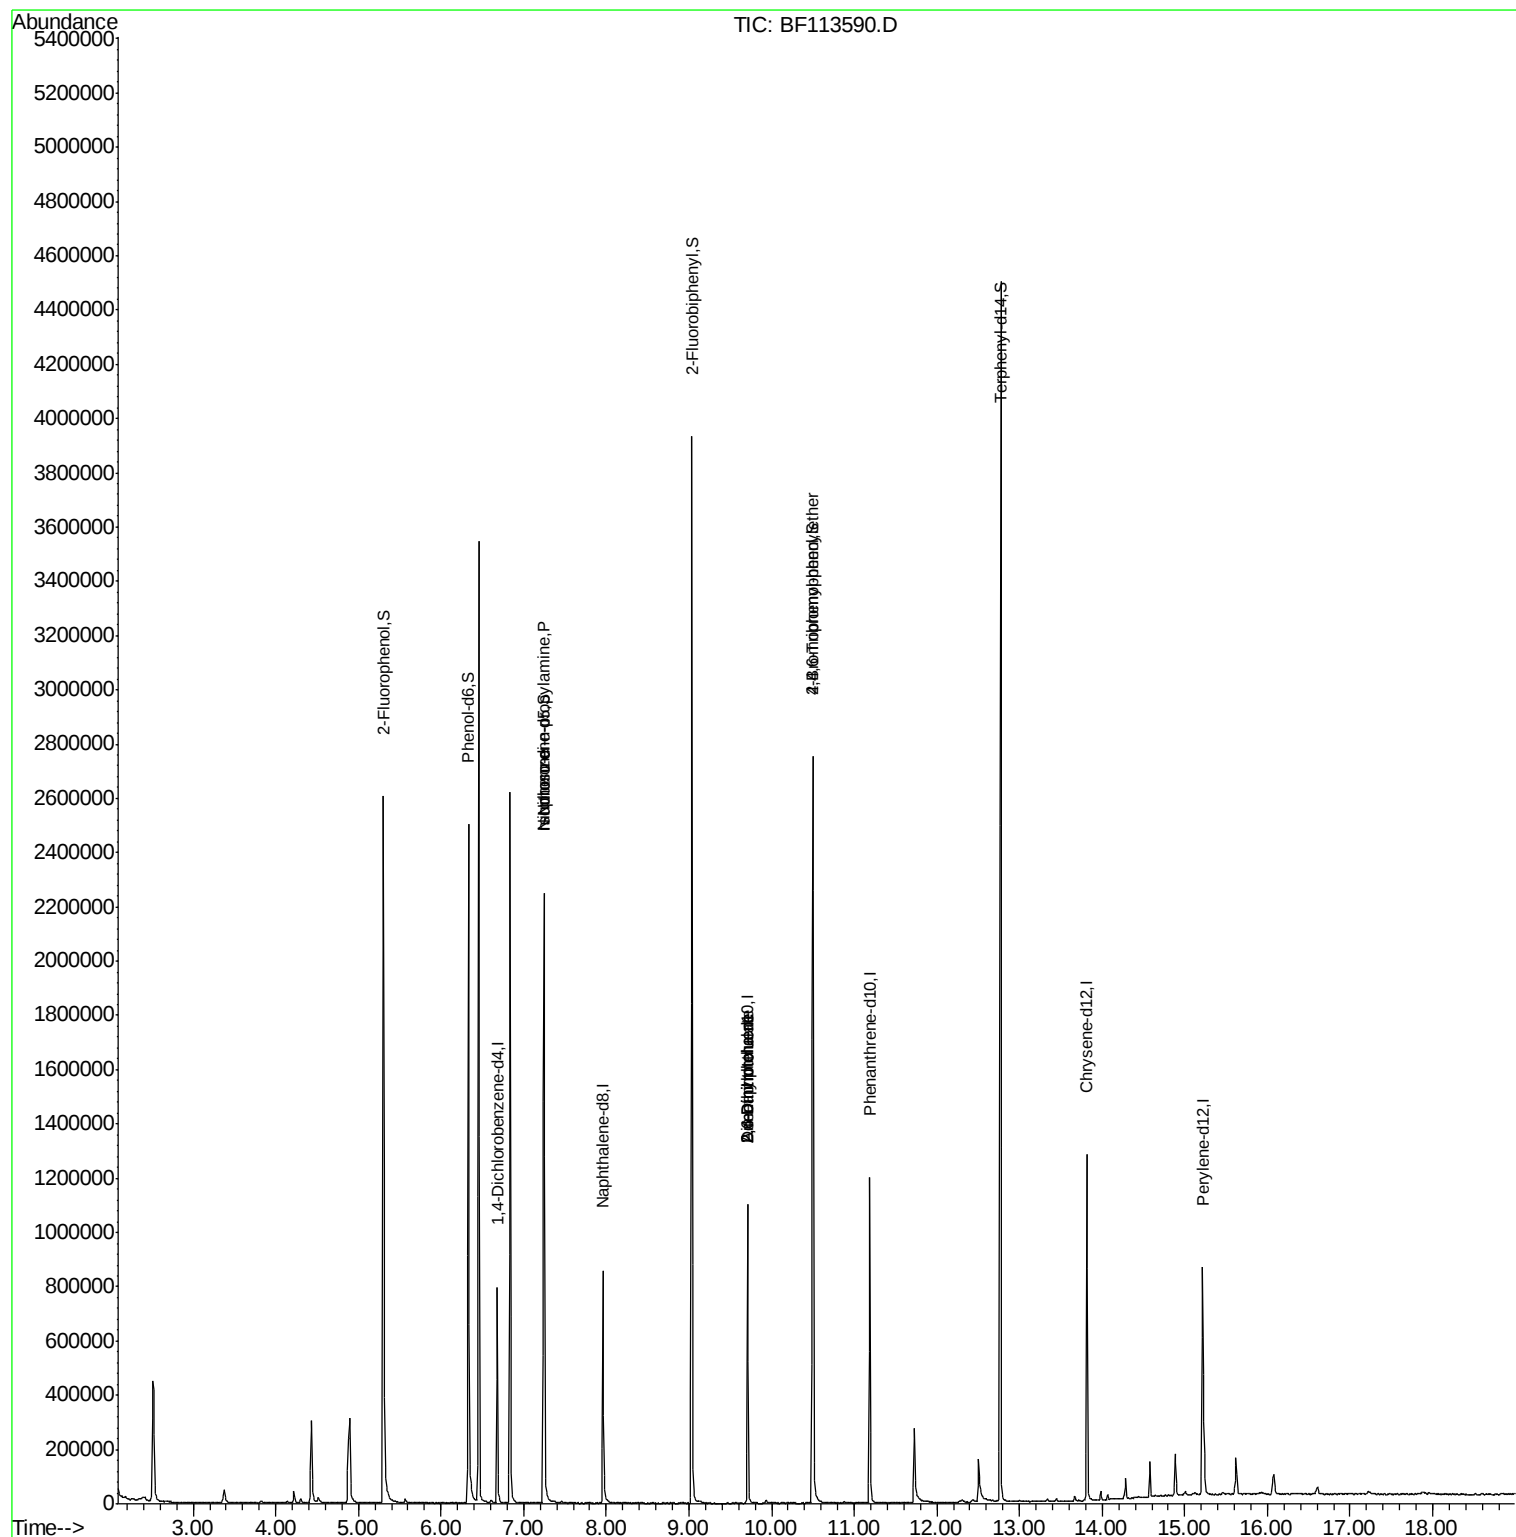




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.68 min Scan# 781
Delta R.T. -0.01 min
Lab File: BF113590.D
Acq: 4 Apr 2019 18:39

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 118777
Ion Ratio Lower Upper
152 100
150 157.2 124.7 187.1
115 56.7 46.0 69.0

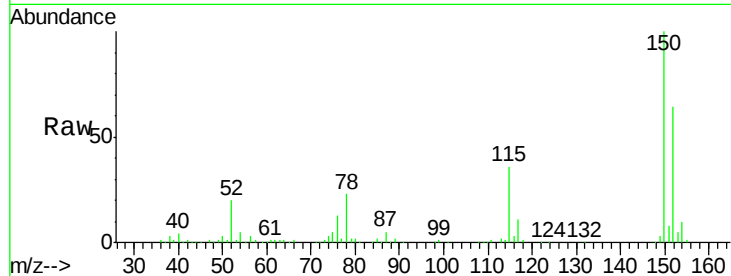


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

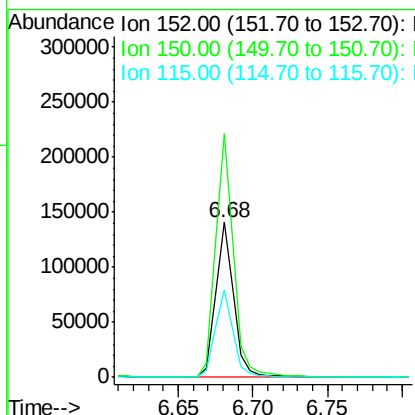



#5


2-Fluorophenol
Concen: 119.308 ng
RT: 5.30 min Scan# 547
Delta R.T. 0.01 min
Lab File: BF113590.D
Acq: 4 Apr 2019 18:39

Tgt Ion:112 Resp: 831036
Ion Ratio Lower Upper
112 100
64 58.5 49.2 73.8
63 29.8 24.9 37.3



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

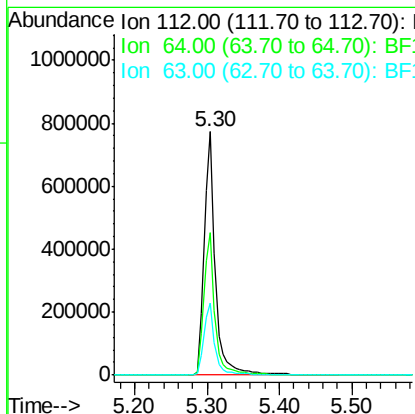

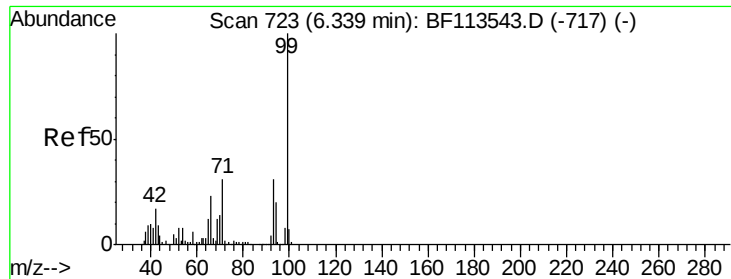

#7

Phenol-d6

Concen: 108.202 ng

RT: 6.33 min Scan# 722

Delta R.T. -0.01 min

Lab File: BF113590.D

Acq: 4 Apr 2019 18:39

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 928913

Ion Ratio Lower Upper

99 100

42 17.1 14.8 22.2




71 30.7 24.9 37.3

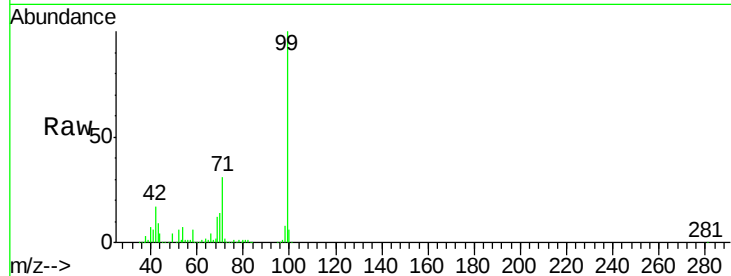

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

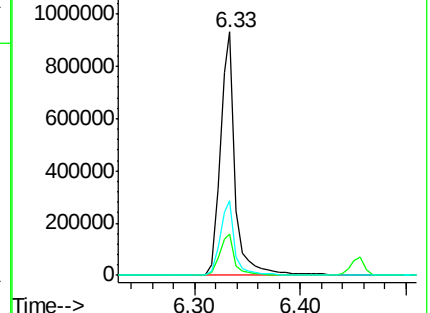

#19

n-Nitroso-di-n-propylamine

Concen: 18.507 ng

RT: 7.25 min Scan# 877

Delta R.T. 0.14 min

Lab File: BF113590.D

Acq: 4 Apr 2019 18:39

Tgt Ion: 70 Resp: 97975


Ion Ratio Lower Upper

70 100

42 49.1 48.4 72.6

101 0.0 7.8 11.8#

130 2.5 18.2 27.4#





Abundance Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): BF1

Ion 130.00 (129.70 to 130.70): BF1

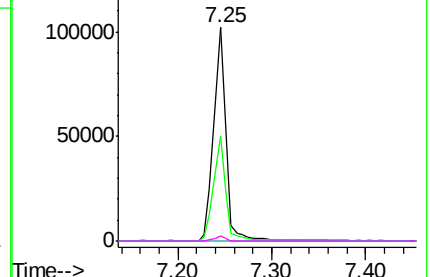



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.96 min Scan# 999

Delta R.T. -0.01 min

Lab File: BF113590.D

Acq: 4 Apr 2019 18:39

Instrument :

BNA_F

ClientSampleId :

Tot Ion:136 Resp: 446623


Ion Ratio Lower Upper

136 100

137 10.6 8.9 13.3

54 7.1 7.0 10.6

68 5.2 4.8 7.2




Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1



Time-->



#23

Nitrobenzene-d5

Concen: 98.887 ng

RT: 7.25 min Scan# 877

Delta R.T. -0.01 min

Lab File: BF113590.D

Acq: 4 Apr 2019 18:39


Tgt Ion: 82 Resp: 753994

Ion Ratio Lower Upper

82 100

128 46.7 36.5 54.7


54 52.5 42.2 63.2




Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

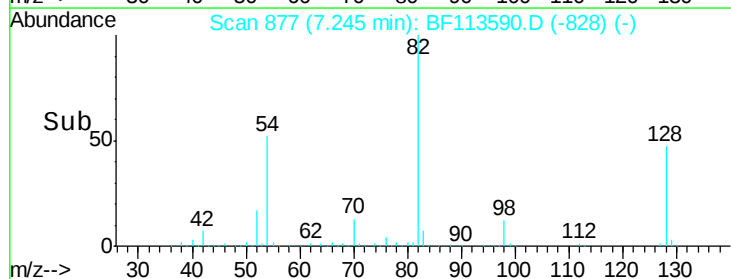





Time-->

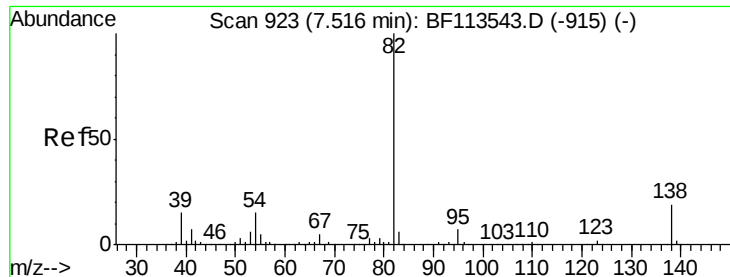

#25
Isophorone
Concen: 51.333 ng
RT: 7.25 min Scan# 877
Delta R.T. -0.27 min
Lab File: BF113590.D
Acq: 4 Apr 2019 18:39




Instrument :
BNA_F
ClientSampleId :


Tot Ion: 82 Resp: 753988
Ion Ratio Lower Upper
82 100
95 0.0 5.5 8.3#
138 0.0 15.2 22.8#

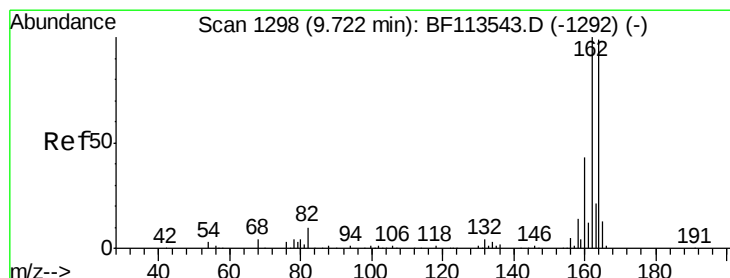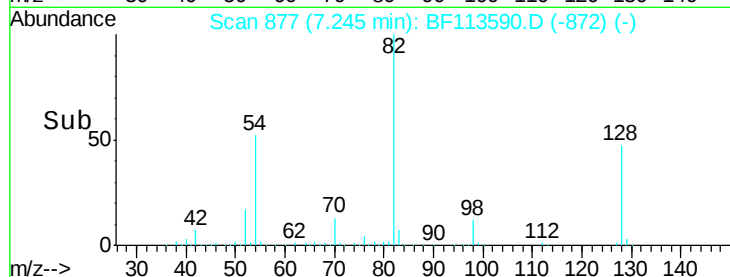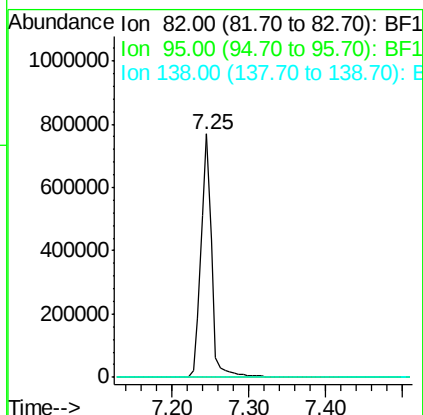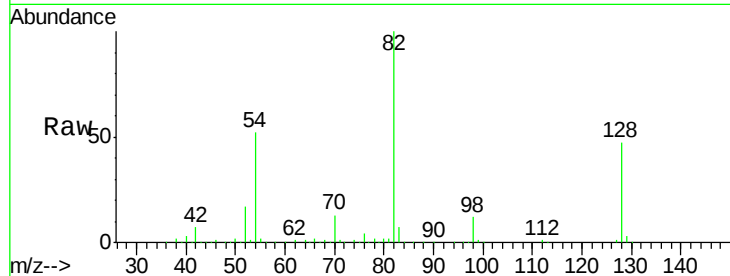

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.71 min Scan# 1296
Delta R.T. -0.01 min
Lab File: BF113590.D
Acq: 4 Apr 2019 18:39

Tgt Ion:164 Resp: 220123
Ion Ratio Lower Upper
164 100
162 102.6 81.8 122.6
160 45.3 36.4 54.6

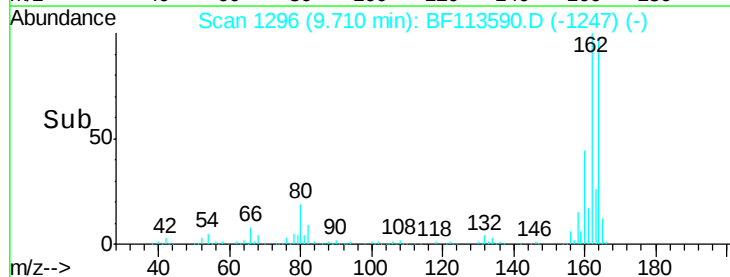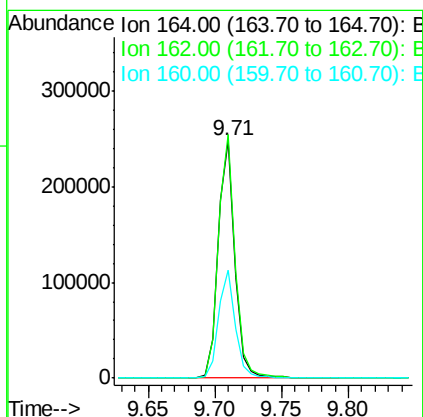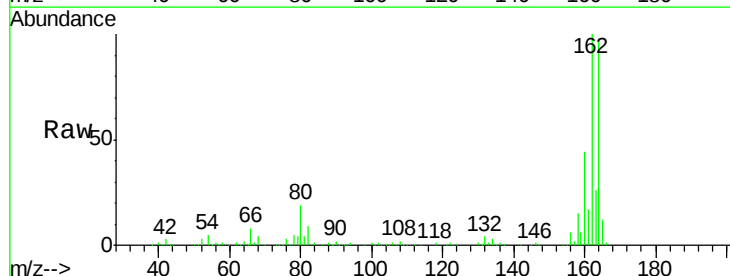


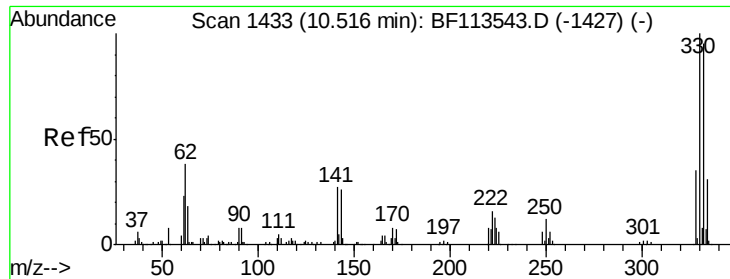




#42
 2,4,6-Tribromophenol
 Concen: 160.628 ng
 RT: 10.50 min Scan# 1431
 Delta R.T. -0.01 min
 Lab File: BF113590.D
 Acq: 4 Apr 2019 18:39

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:330 Resp: 424735
 Ion Ratio Lower Upper
 330 100
 332 95.5 77.8 116.6
 141 27.4 22.7 34.1

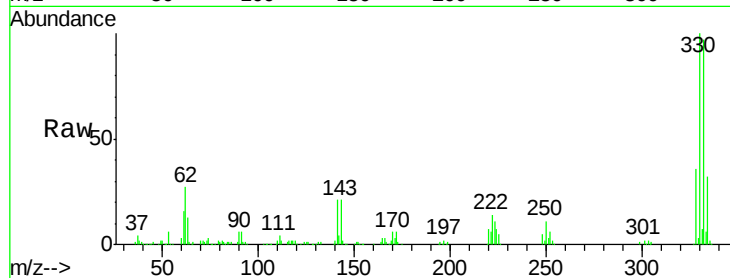


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

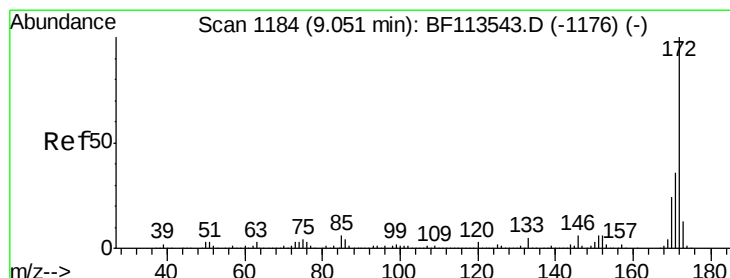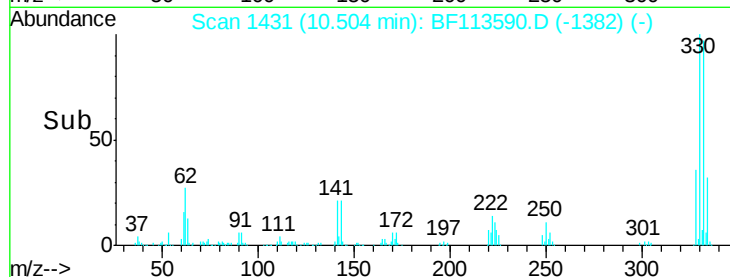
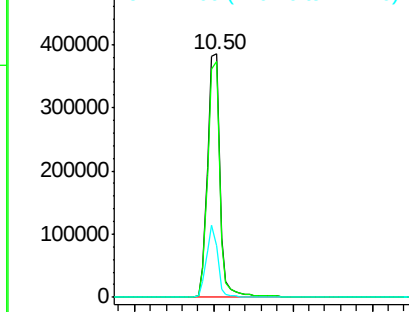


#45
 2-Fluorobiphenyl
 Concen: 101.546 ng
 RT: 9.04 min Scan# 1182
 Delta R.T. -0.01 min
 Lab File: BF113590.D
 Acq: 4 Apr 2019 18:39

Tgt Ion:172 Resp: 1388460
 Ion Ratio Lower Upper
 172 100
 171 35.8 29.0 43.6
 170 24.3 19.5 29.3

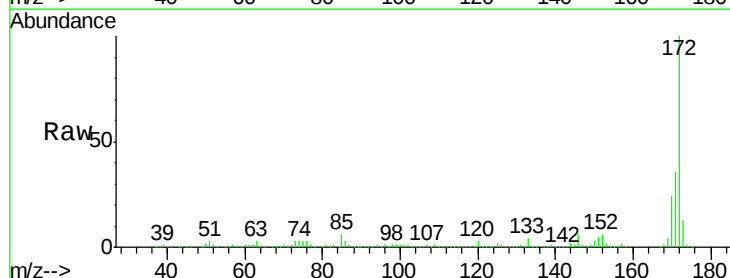

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

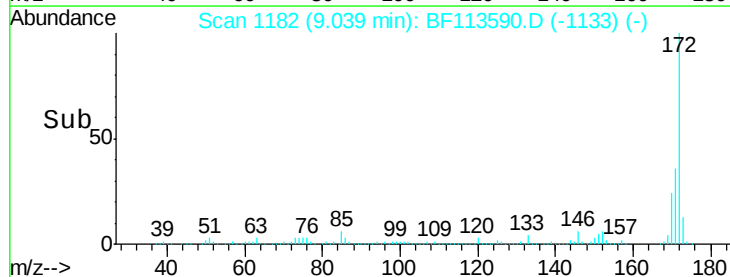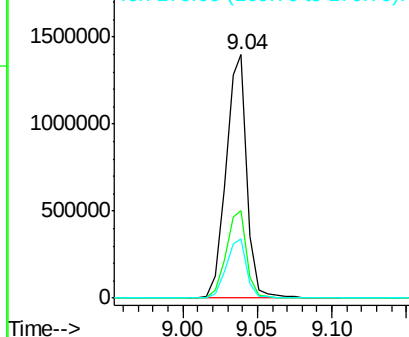



#50

Dimethylphthalate

Concen: 3.482 ng

RT: 9.71 min Scan# 1296

Delta R.T. 0.26 min

Lab File: BF113590.D

Acq: 4 Apr 2019 18:39

Instrument :

BNA_F

ClientSampleId :


Tot Ion:163 Resp: 56506

Ion Ratio Lower Upper

163 100

194 0.0 3.0 4.6#




164 372.3 8.1 12.1#

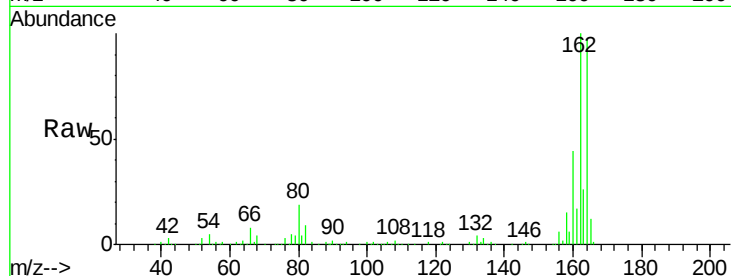

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

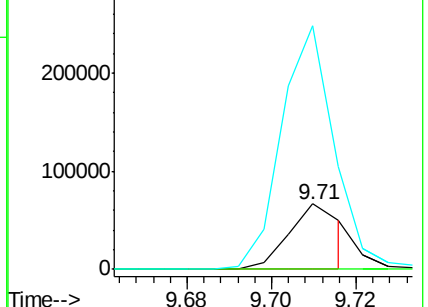

#51

2,6-Dinitrotoluene

Concen: 7.907 ng

RT: 9.71 min Scan# 1296

Delta R.T. 0.19 min

Lab File: BF113590.D

Acq: 4 Apr 2019 18:39


Tgt Ion:165 Resp: 28282

Ion Ratio Lower Upper

165 100

63 1.3 43.4 65.0#



89 2.1 43.1 64.7#




Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 89.00 (88.70 to 89.70): BF1

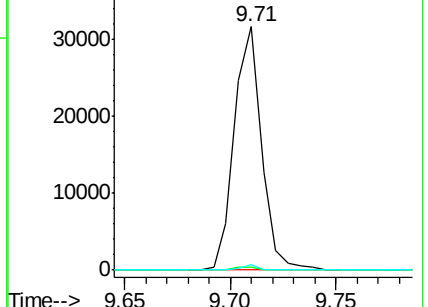


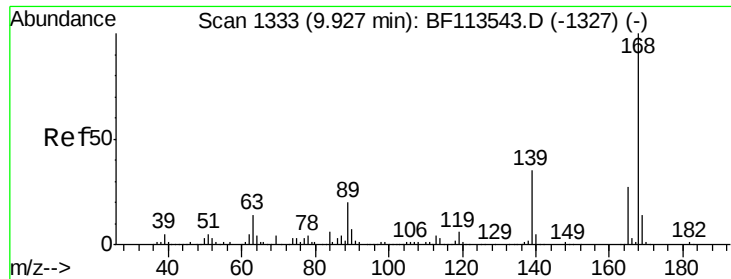




#57
 2,4-Dinitrotoluene
 Concen: 6.538 ng
 RT: 9.71 min Scan# 1296
 Delta R.T. -0.22 min
 Lab File: BF113590.D
 Acq: 4 Apr 2019 18:39

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:165 Resp: 28282
 Ion Ratio Lower Upper
 165 100
 63 1.3 37.5 56.3#
 89 2.1 57.4 86.2#
 182 0.0 2.0 3.0#




Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF1
 Ion 89.00 (88.70 to 89.70): BF1
 Ion 182.00 (181.70 to 182.70): E

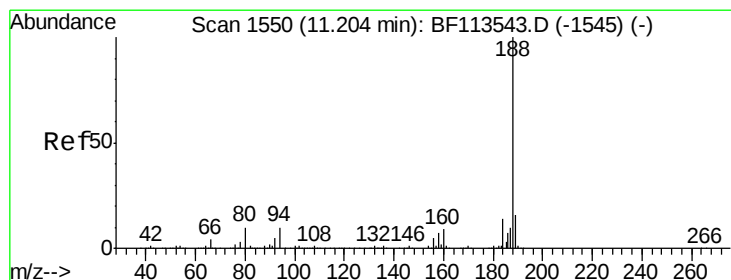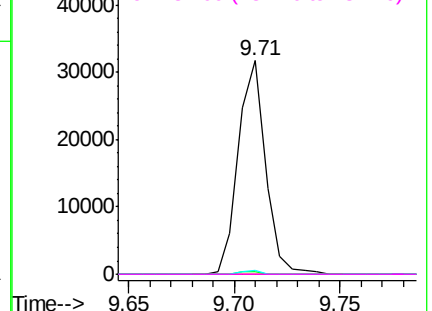




#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.19 min Scan# 1547
 Delta R.T. -0.02 min
 Lab File: BF113590.D
 Acq: 4 Apr 2019 18:39

Tgt Ion:188 Resp: 475197
 Ion Ratio Lower Upper
 188 100
 94 10.0 7.0 10.6
 80 10.3 7.7 11.5



Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF1
 Ion 80.00 (79.70 to 80.70): BF1

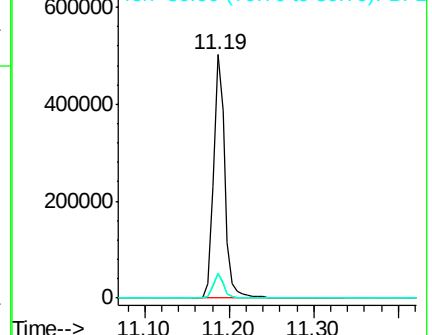


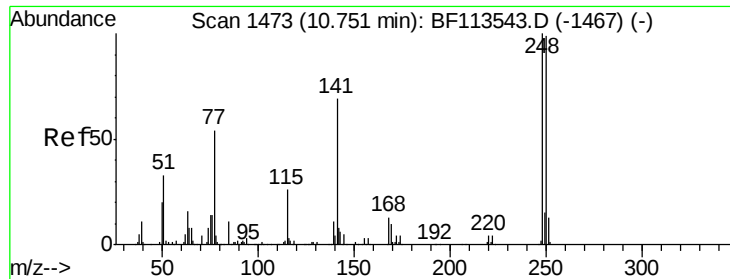




#67
4-Bromophenyl-phenylether
Concen: 4.603 ng
RT: 10.50 min Scan# 1430
Delta R.T. -0.25 min
Lab File: BF113590.D
Acq: 4 Apr 2019 18:39

Instrument :
BNA_F
ClientSampled :

Tot Ion:248 Resp: 24530
Ion Ratio Lower Upper
248 100
250 189.0 78.3 117.5#
141 467.9 56.2 84.4#

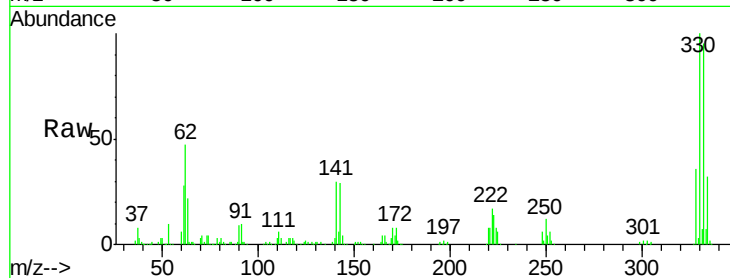


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

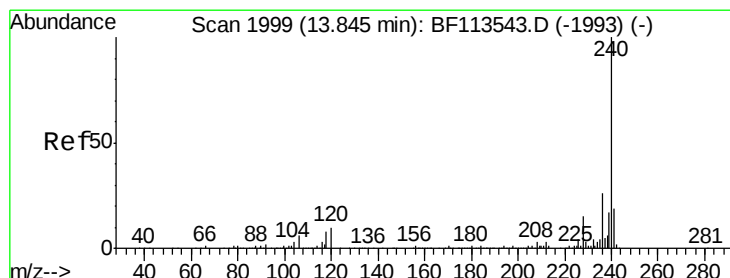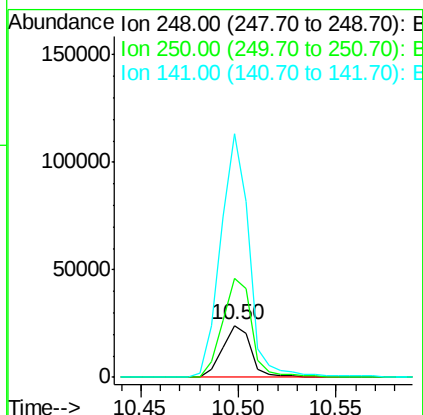
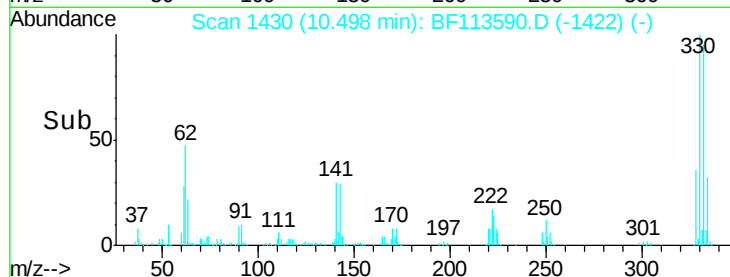



#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.82 min Scan# 1994
Delta R.T. -0.03 min
Lab File: BF113590.D
Acq: 4 Apr 2019 18:39

Tgt Ion:240 Resp: 454587
Ion Ratio Lower Upper
240 100
120 11.3 8.8 13.2
236 25.5 20.9 31.3

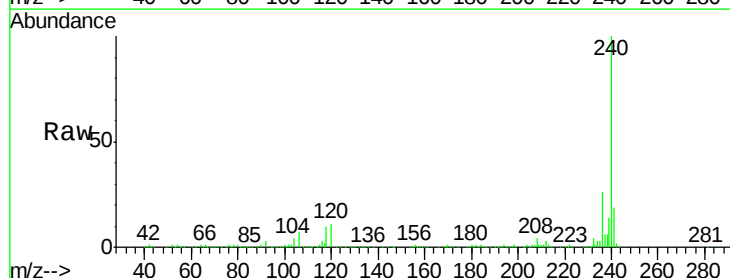

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

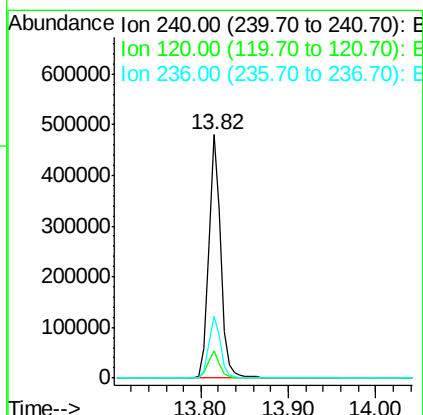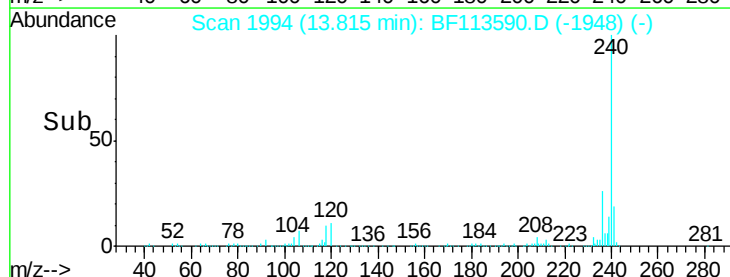



#79

Terphenyl-d14

Concen: 81.797 ng

RT: 12.77 min Scan# 1817

Delta R.T. -0.02 min

Lab File: BF113590.D

Acq: 4 Apr 2019 18:39

Instrument :

BNA_F

ClientSampleId :


Tot Ion:244 Resp: 1826297

Ion Ratio Lower Upper

244 100

212 6.9 5.5 8.3




122 10.8 8.6 13.0



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

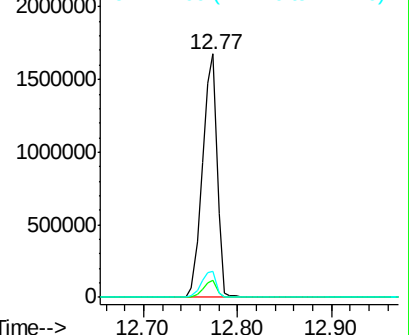

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.22 min Scan# 2232

Delta R.T. -0.04 min

Lab File: BF113590.D

Acq: 4 Apr 2019 18:39


Tgt Ion:264 Resp: 396441

Ion Ratio Lower Upper

264 100

260 23.9 19.1 28.7

265 21.8 17.1 25.7



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

