

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040419\
 Data File : BF113582.D
 Acq On : 4 Apr 2019 14:38
 Operator : JU/SJ
 Sample : PB118303BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB118303BL

Quant Time: Apr 05 04:08:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 04 04:05:31 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.68	152	156559	20.00	ng	0.00
21) Naphthalene-d8	7.96	136	595357	20.00	ng	0.00
39) Acenaphthene-d10	9.71	164	301148	20.00	ng	-0.01
64) Phenanthrene-d10	11.19	188	663036	20.00	ng	-0.01
76) Chrysene-d12	13.82	240	626857	20.00	ng	-0.02
87) Perylene-d12	15.22	264	571157	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.31	112	956037	104.13	ng	0.01
7) Phenol-d6	6.33	99	1244758	110.00	ng	0.00
23) Nitrobenzene-d5	7.25	82	758739	74.65	ng	-0.01
42) 2,4,6-Tribromophenol	10.50	330	421356	116.48	ng	-0.01
45) 2-Fluorobiphenyl	9.04	172	1477746	79.00	ng	-0.01
79) Terphenyl-d14	12.77	244	1822363	59.19	ng	-0.02


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040419\
Data File : BF113582.D
Acq On : 4 Apr 2019 14:38
Operator : JU/SJ
Sample : PB118303BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB118303BL

Quant Time: Apr 05 04:08:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 04 04:05:31 2019
Response via : Initial Calibration

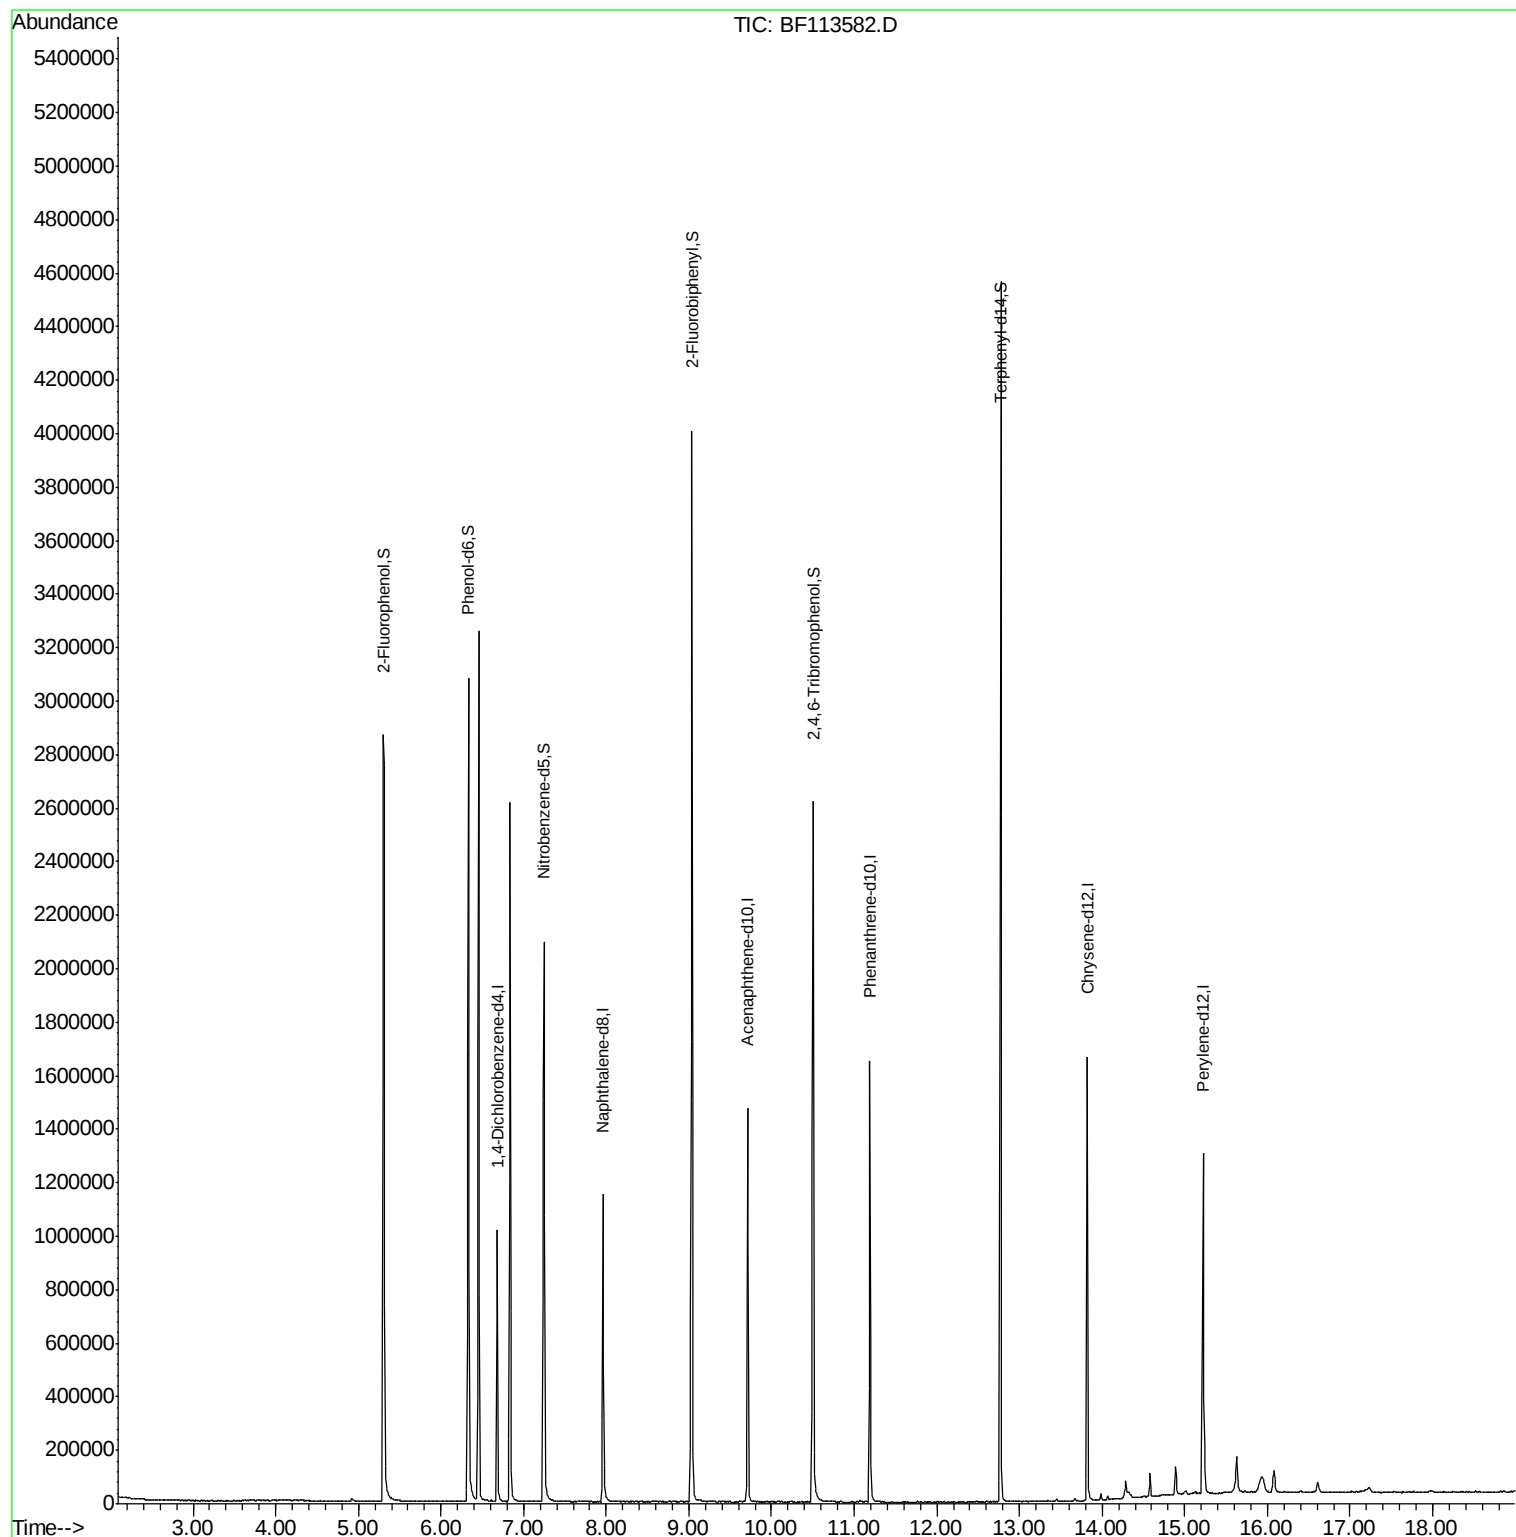

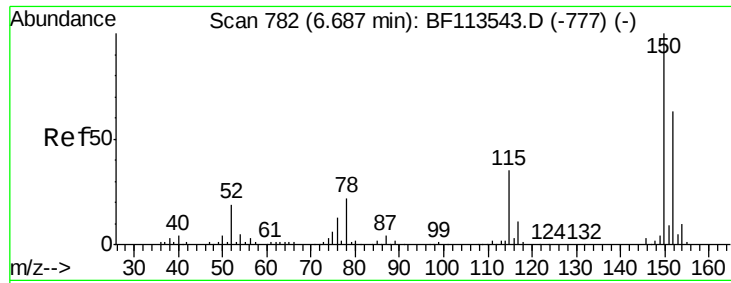


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.68 min Scan# 781
Delta R.T. -0.01 min
Lab File: BF113582.D
Acq: 4 Apr 2019 14:38

Instrument :
BNA_F
ClientSampleId :
PB118303BL

Tgt Ion:152 Resp: 156559
Ion Ratio Lower Upper
152 100
150 155.9 124.7 187.1
115 56.0 46.0 69.0

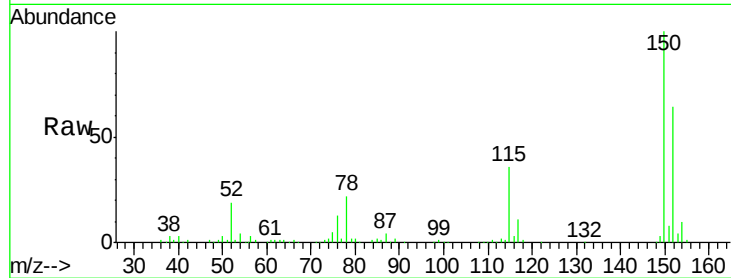


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

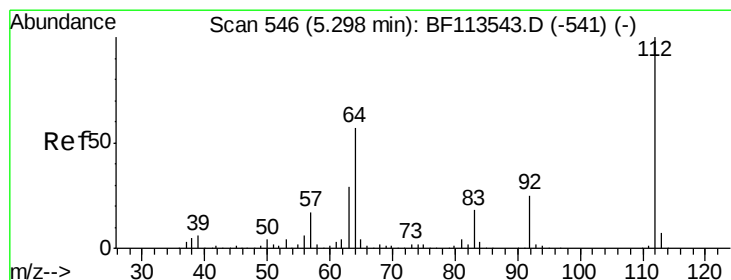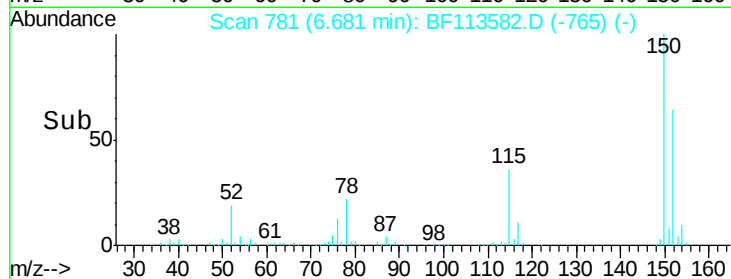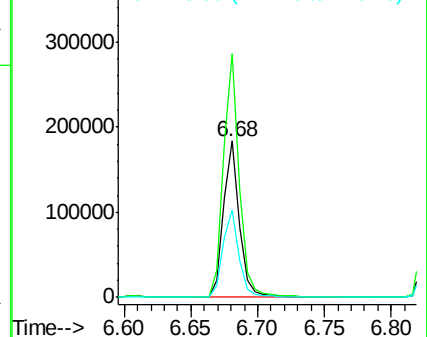



#5


2-Fluorophenol
Concen: 104.131 ng
RT: 5.31 min Scan# 548
Delta R.T. 0.01 min
Lab File: BF113582.D
Acq: 4 Apr 2019 14:38

Tgt Ion:112 Resp: 956037
Ion Ratio Lower Upper
112 100
64 56.4 49.2 73.8
63 28.9 24.9 37.3

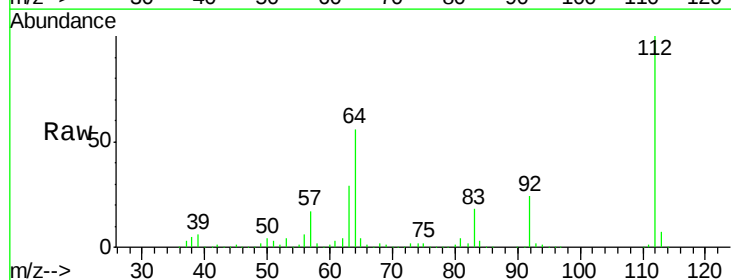

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

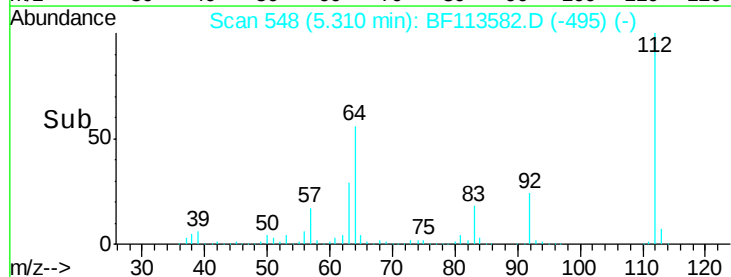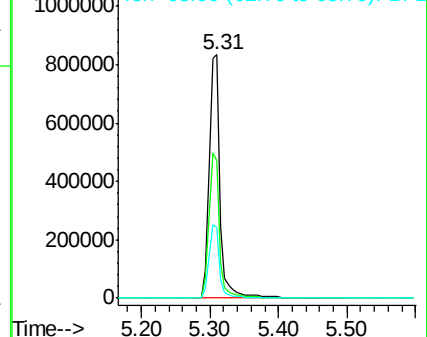

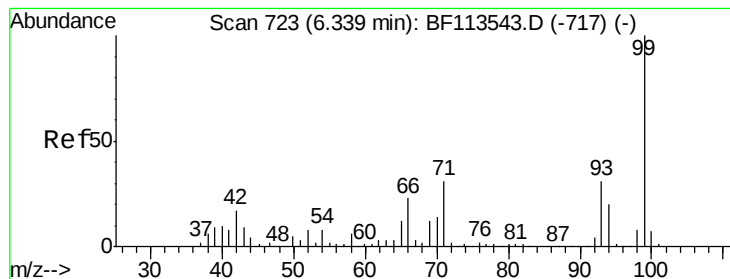

#7

Phenol-d6

Concen: 110.002 ng

RT: 6.33 min Scan# 722

Delta R.T. -0.01 min

Lab File: BF113582.D

Acq: 4 Apr 2019 14:38

Instrument :

BNA_F

ClientSampleId :

PB118303BL


Tgt Ion: 99 Resp: 1244758

Ion Ratio Lower Upper




99 100

42 18.0 14.8 22.2

71 31.7 24.9 37.3

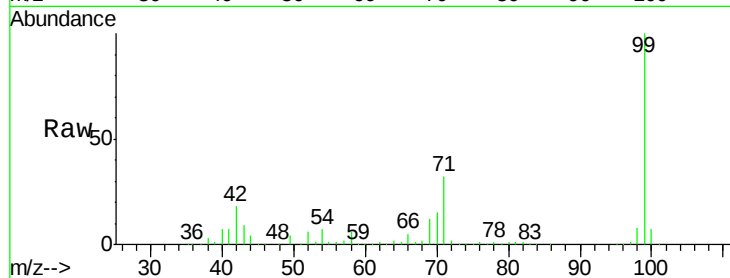

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

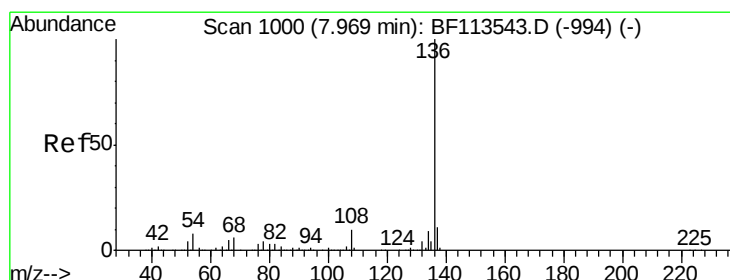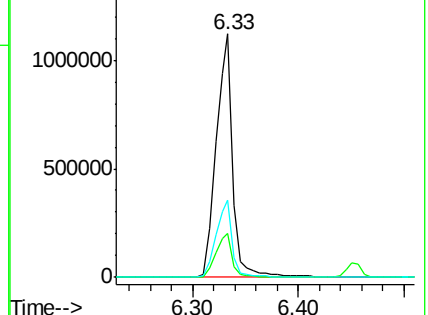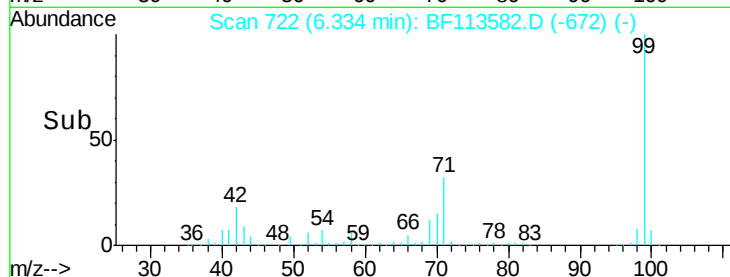

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.96 min Scan# 999

Delta R.T. -0.01 min

Lab File: BF113582.D

Acq: 4 Apr 2019 14:38

Tgt Ion: 136 Resp: 595357


Ion Ratio Lower Upper

136 100



137 11.2 8.9 13.3


54 7.8 7.0 10.6

68 5.9 4.8 7.2

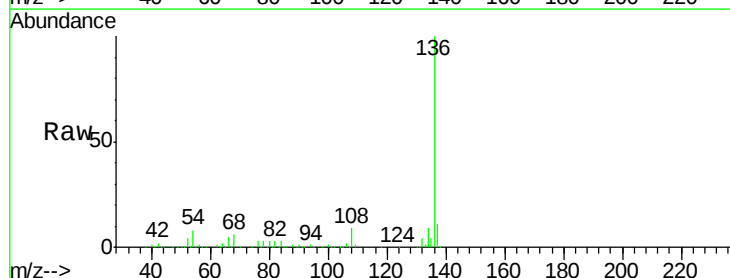

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

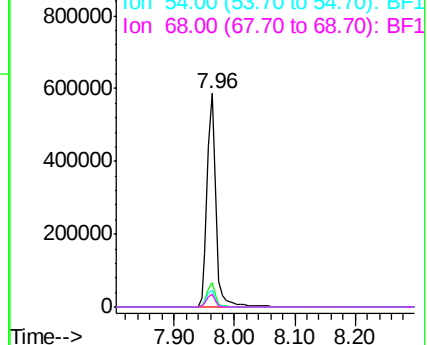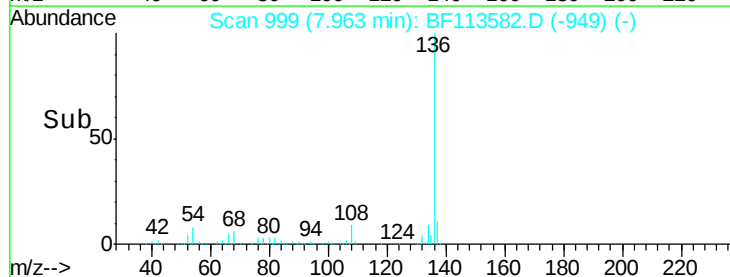


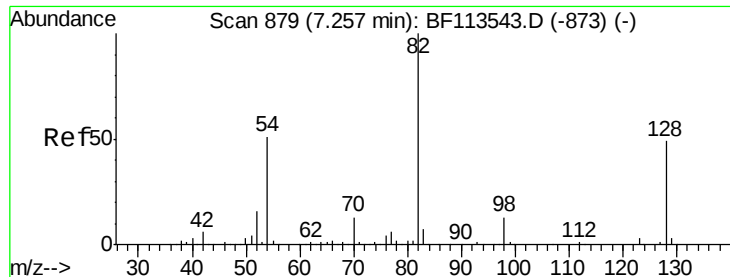




#23
 Nitrobenzene-d5
 Concen: 74.650 ng
 RT: 7.25 min Scan# 877
 Delta R.T. -0.01 min
 Lab File: BF113582.D
 Acq: 4 Apr 2019 14:38

Instrument :
 BNA_F
 ClientSampleID :
 PB118303BL

Tgt Ion: 82 Resp: 758739
 Ion Ratio Lower Upper
 82 100
 128 47.6 36.5 54.7
 54 51.9 42.2 63.2

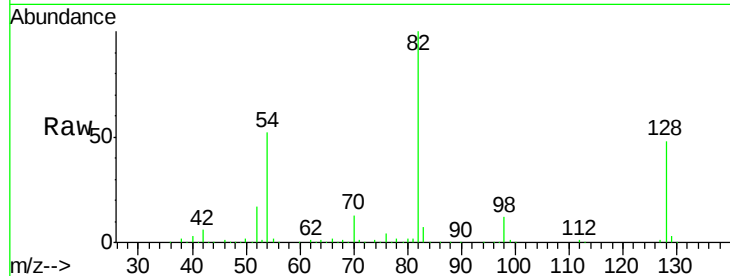


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1

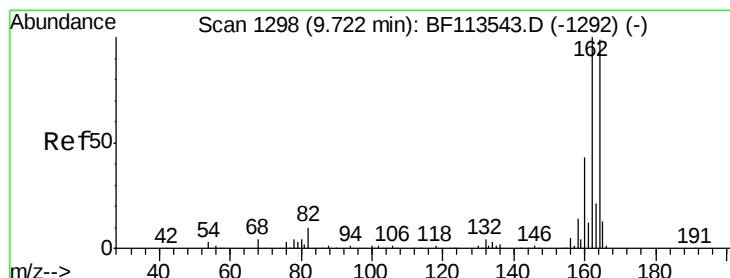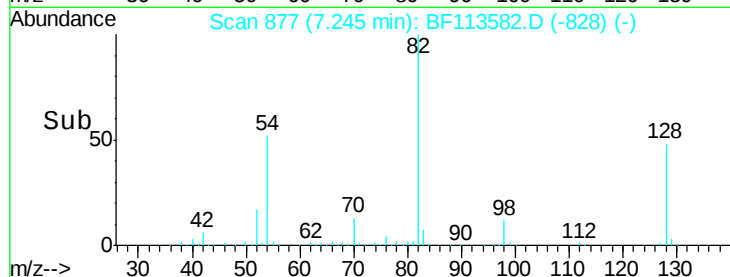
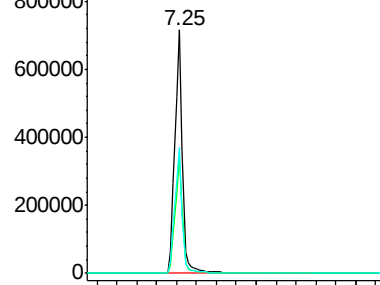



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.71 min Scan# 1296
 Delta R.T. -0.01 min
 Lab File: BF113582.D
 Acq: 4 Apr 2019 14:38

Tgt Ion: 164 Resp: 301148
 Ion Ratio Lower Upper
 164 100
 162 101.6 81.8 122.6
 160 45.6 36.4 54.6

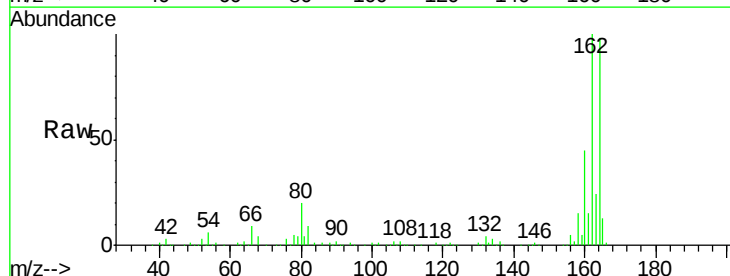

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E



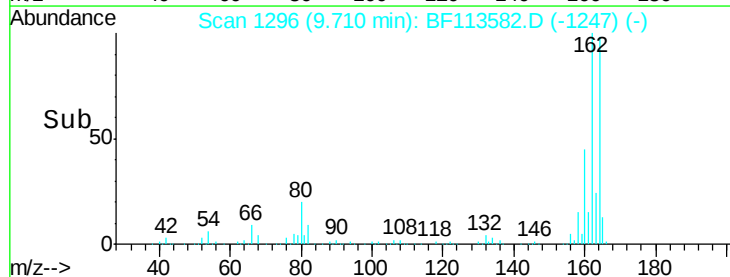
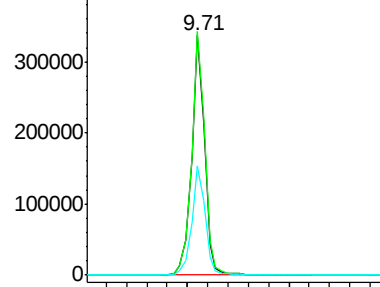


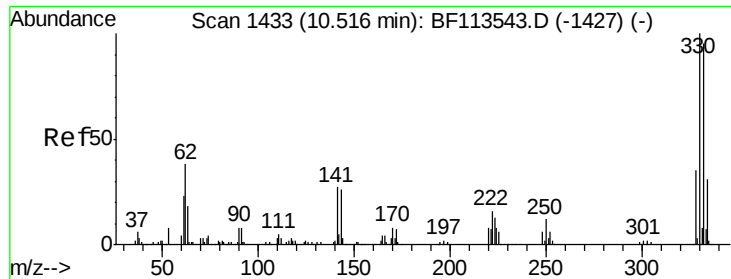

#42
 2,4,6-Tribromophenol
 Concen: 116.476 ng
 RT: 10.50 min Scan# 1431
 Delta R.T. -0.01 min
 Lab File: BF113582.D
 Acq: 4 Apr 2019 14:38




Instrument :
 BNA_F
 ClientSampleId :
 PB118303BL


Tgt Ion:330 Resp: 421356
 Ion Ratio Lower Upper
 330 100
 332 97.4 77.8 116.6
 141 27.9 22.7 34.1

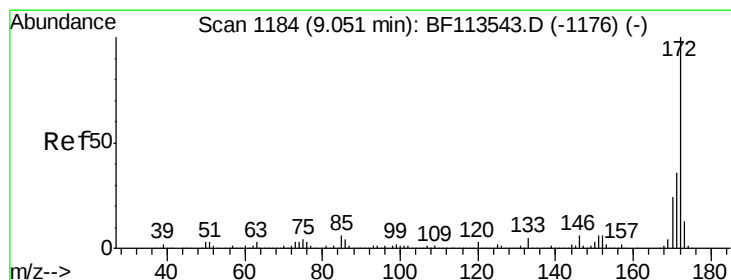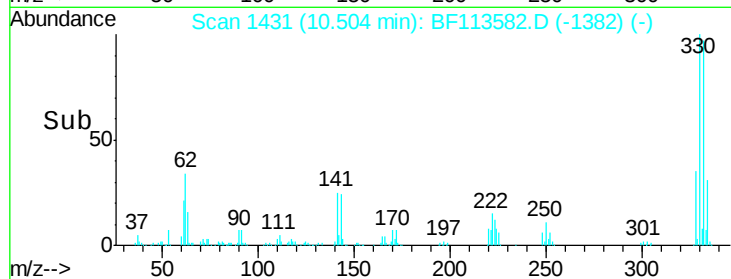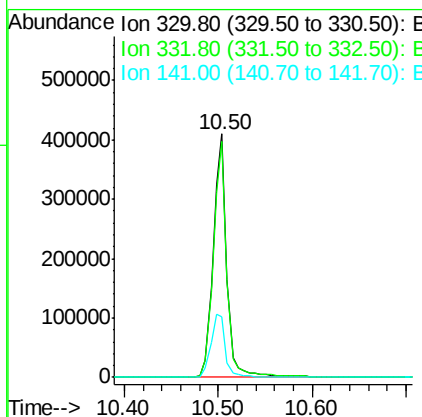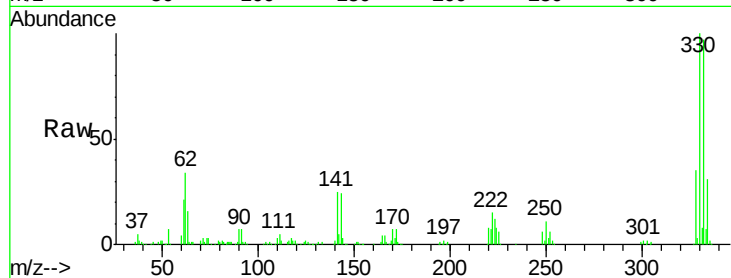

#45
 2-Fluorobiphenyl
 Concen: 78.998 ng
 RT: 9.04 min Scan# 1182
 Delta R.T. -0.01 min
 Lab File: BF113582.D
 Acq: 4 Apr 2019 14:38

Tgt Ion:172 Resp: 1477746
 Ion Ratio Lower Upper
 172 100
 171 36.1 29.0 43.6
 170 24.3 19.5 29.3


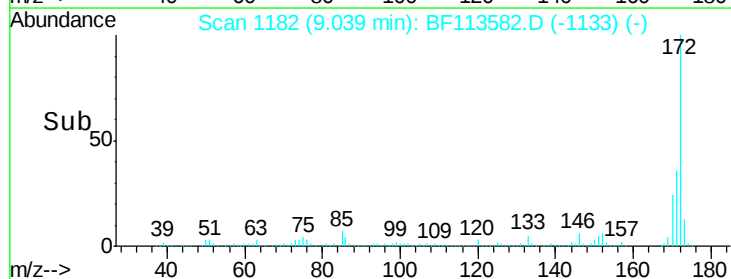
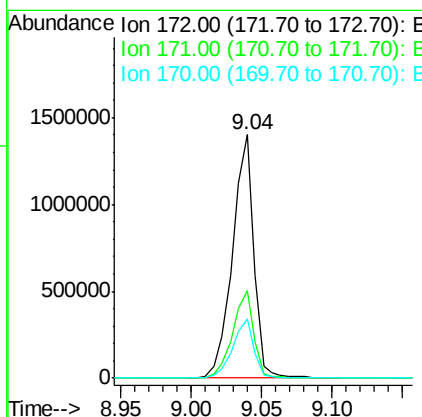
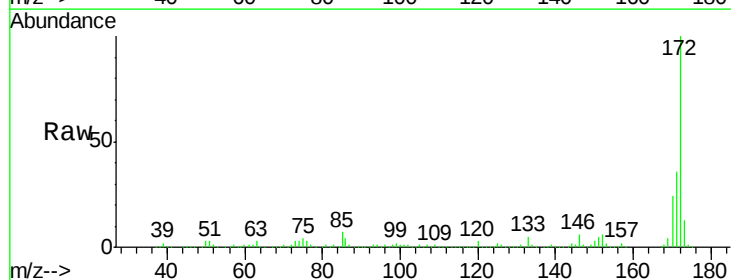


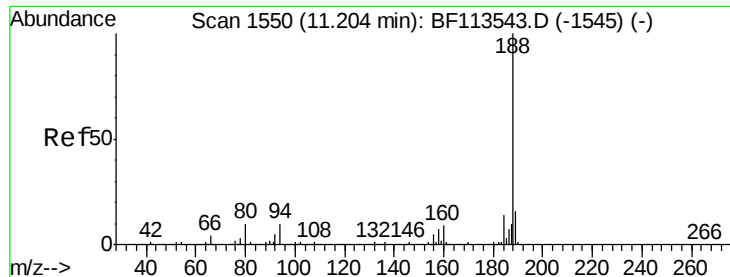

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.19 min Scan# 1548
Delta R.T. -0.01 min
Lab File: BF113582.D
Acq: 4 Apr 2019 14:38




Instrument :
BNA_F
ClientSampleId :
PB118303BL


Tgt Ion:188 Resp: 663036
Ion Ratio Lower Upper
188 100
94 8.9 7.0 10.6
80 8.9 7.7 11.5

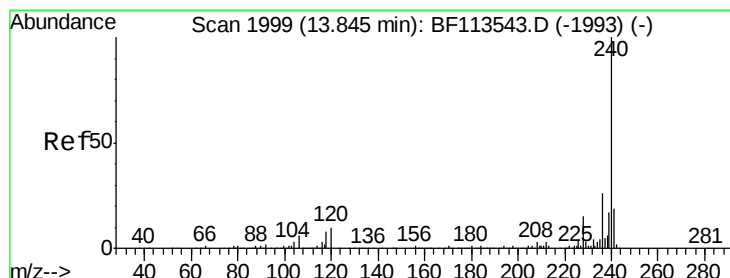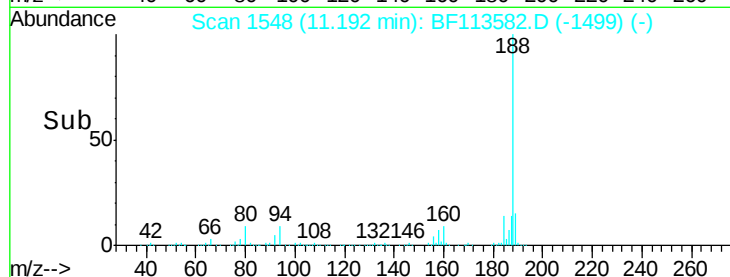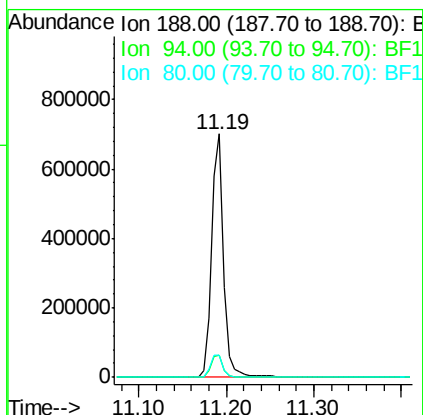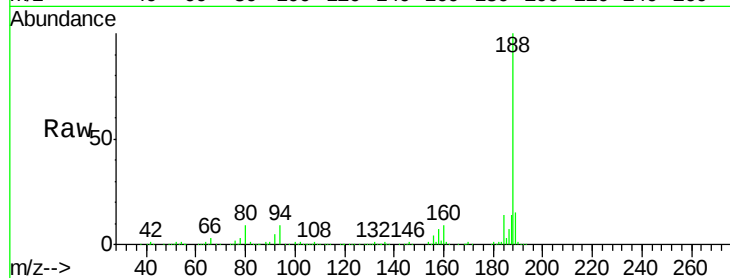

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.82 min Scan# 1995
Delta R.T. -0.02 min
Lab File: BF113582.D
Acq: 4 Apr 2019 14:38

Tgt Ion:240 Resp: 626857
Ion Ratio Lower Upper
240 100
120 10.7 8.8 13.2
236 26.1 20.9 31.3


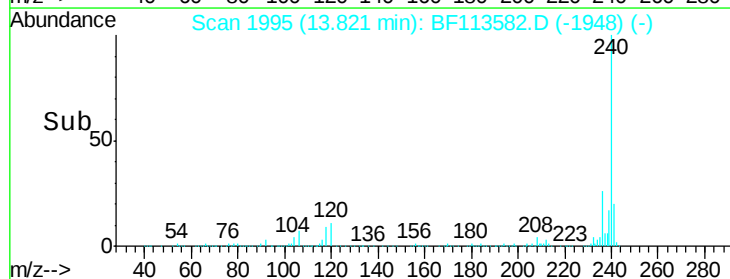
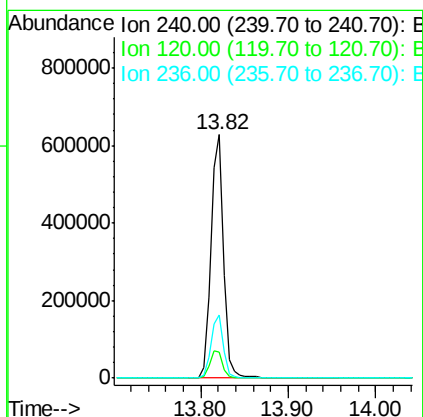
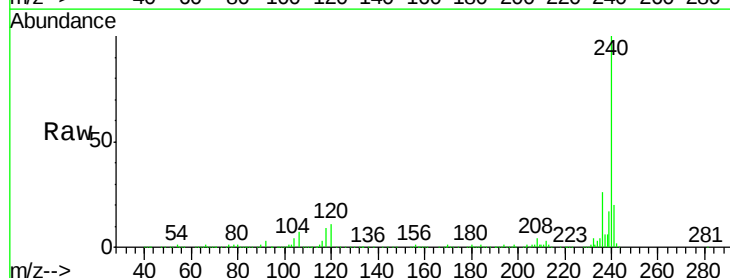


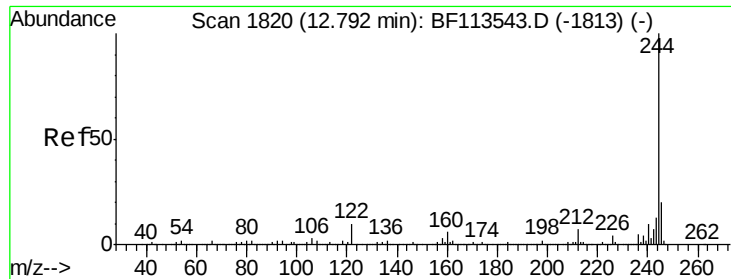

#79
 Terphenyl-d14
 Concen: 59.190 ng
 RT: 12.77 min Scan# 1817
 Delta R.T. -0.02 min
 Lab File: BF113582.D
 Acq: 4 Apr 2019 14:38

Instrument :
 BNA_F
 ClientSampleId :
 PB118303BL

Tgt Ion:244 Resp: 1822363
 Ion Ratio Lower Upper
 244 100
 212 6.8 5.5 8.3
 122 11.1 8.6 13.0

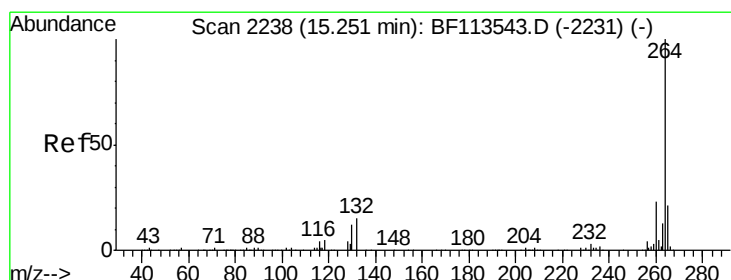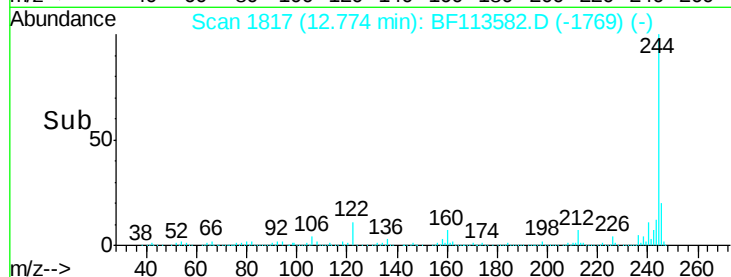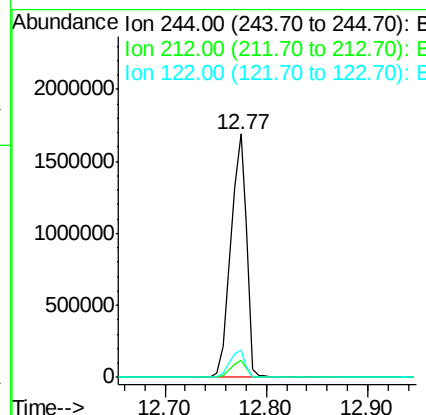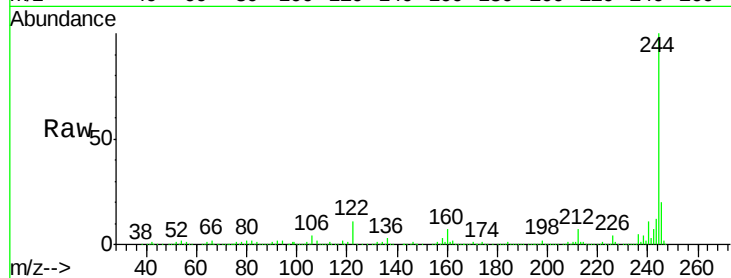

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.22 min Scan# 2233
 Delta R.T. -0.03 min
 Lab File: BF113582.D
 Acq: 4 Apr 2019 14:38

Tgt Ion:264 Resp: 571157
 Ion Ratio Lower Upper
 264 100
 260 24.0 19.1 28.7
 265 22.1 17.1 25.7

